

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
 Data File : PD060283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 09:30
 Operator : DD\AJ
 Sample : RESC08
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 06:26:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 26 01:04:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.022	20914843	68272323	19.043	18.908
27)	SA Decachlor...	8.297	9.106	50691733	105.1E6	38.662	37.624
Target Compounds							
2)	A alpha-BHC	3.944	4.413	16272282	50773923	9.427	9.422
3)	MA gamma-BHC...	4.231	4.699	15806061	45467795	9.715	9.333
4)	MA Heptachlor	4.537	5.210	15407754	43100769	9.729	9.136
5)	MB Aldrin	4.789	5.517	15734184	41969444	9.878	9.451
6)	B beta-BHC	4.481	4.866	6673825	20153427	9.985	9.624
7)	B delta-BHC	4.689	5.086	16242107	25978386	9.737	7.236 #
8)	B Heptachlo...	5.235	5.903	14780635	25085881	9.874	7.104 #
9)	A Endosulfan I	5.578	6.261	13505205	35713549	9.609	9.409
10)	B trans-Chl...	5.464	6.138	14801345	37635480	9.644	9.031
11)	B cis-Chlor...	5.523	6.210	14074131	38358284	9.527	9.399
12)	B 4,4'-DDE	5.688	6.366	29660317	74288165	19.276	18.755
13)	MA Dieldrin	5.823	6.518	30621036	77519085	19.158	18.696
14)	MA Endrin	6.082	6.736	27081571	65823860	20.039	18.932
15)	B Endosulfa...	6.356	6.944	24378935	60220418	19.473	18.700
16)	A 4,4'-DDD	6.207	6.855	24984050	60619455	19.177	18.672
17)	MA 4,4'-DDT	6.450	7.155	25004942	62153432	19.144	18.788
18)	B Endrin al...	6.524	7.068	19516324	52426148	19.641	19.298
19)	B Endosulfa...	6.739	7.292	21715311	61348816	19.050	19.465
20)	A Methoxychlor	6.997	7.612	61819573	166.9E6	99.887	100.056
21)	B Endrin ke...	7.233	7.764	27403330	65952924	19.636	19.491

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 09:30
Operator : DD\AJ
Sample : RESC08
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 06:26:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 26 01:04:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

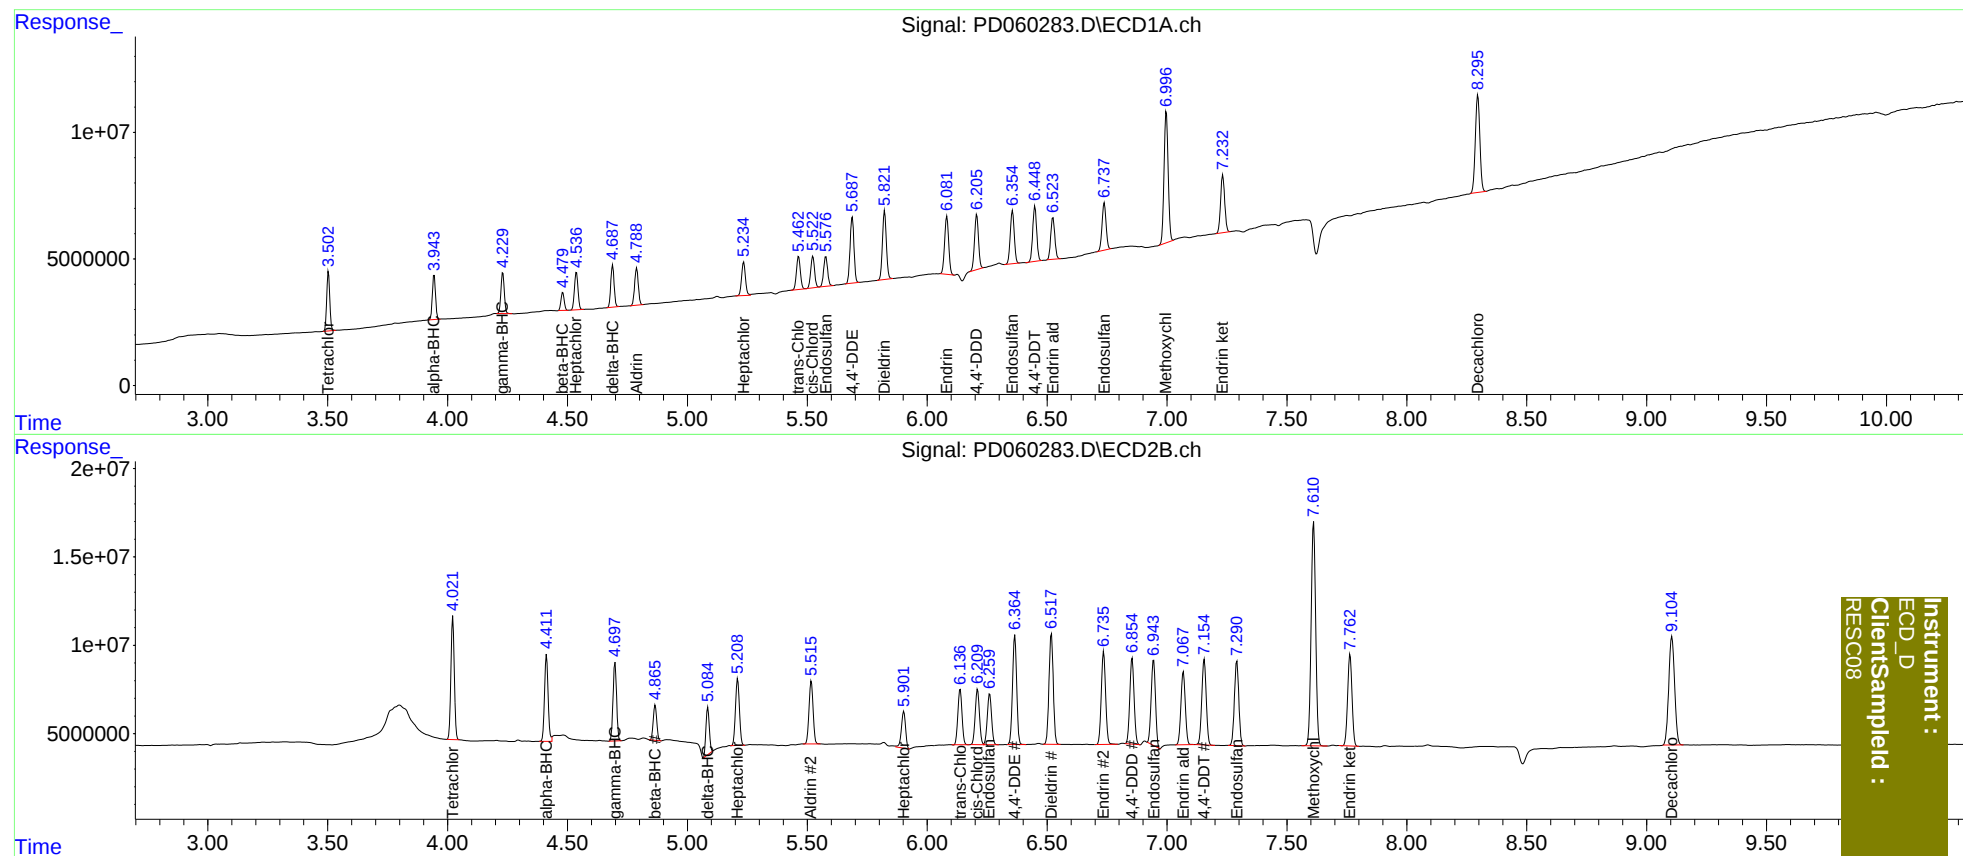

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060283.D
Acq On : 25 Nov 2020 09:30
Operator : DD\AJ
Sample : RESC08
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Title : GC Extractables
Last Update : Thu Nov 26 01:04:31 2020
Integrator: ChemStation

RT#1	RT#2	Resolution
3.503	3.944	100.00%
3.944	4.231	100.00%
4.231	4.481	100.00%
4.481	4.537	100.00%
4.537	4.689	100.00%
4.689	4.789	100.00%
4.789	5.235	100.00%
5.235	5.464	100.00%
5.464	5.523	100.00%
5.523	5.578	100.00%
5.578	5.688	100.00%
5.688	5.823	100.00%
5.823	6.082	100.00%
6.082	6.207	100.00%
6.207	6.356	100.00%
6.356	6.450	100.00%
6.450	6.525	100.00%
6.525	6.739	100.00%
6.739	6.997	100.00%
6.997	7.233	100.00%
7.233	8.297	100.00%

Signal #2


4.022	4.413	100.00%
4.413	4.699	100.00%
4.699	4.866	100.00%
4.866	5.086	100.00%
5.086	5.210	100.00%
5.210	5.517	100.00%
5.517	5.903	100.00%
5.903	6.138	100.00%
6.138	6.210	100.00%
6.210	6.261	98.44%
6.261	6.366	100.00%
6.366	6.518	100.00%
6.518	6.736	100.00%
6.736	6.855	100.00%
6.855	6.944	100.00%
6.944	7.068	100.00%
7.068	7.155	100.00%
7.155	7.292	100.00%
7.292	7.612	100.00%
7.612	7.764	100.00%
7.764	9.106	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 09:30
Operator : DD\AJ
Sample : RESC08
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 06:26:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 26 01:04:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

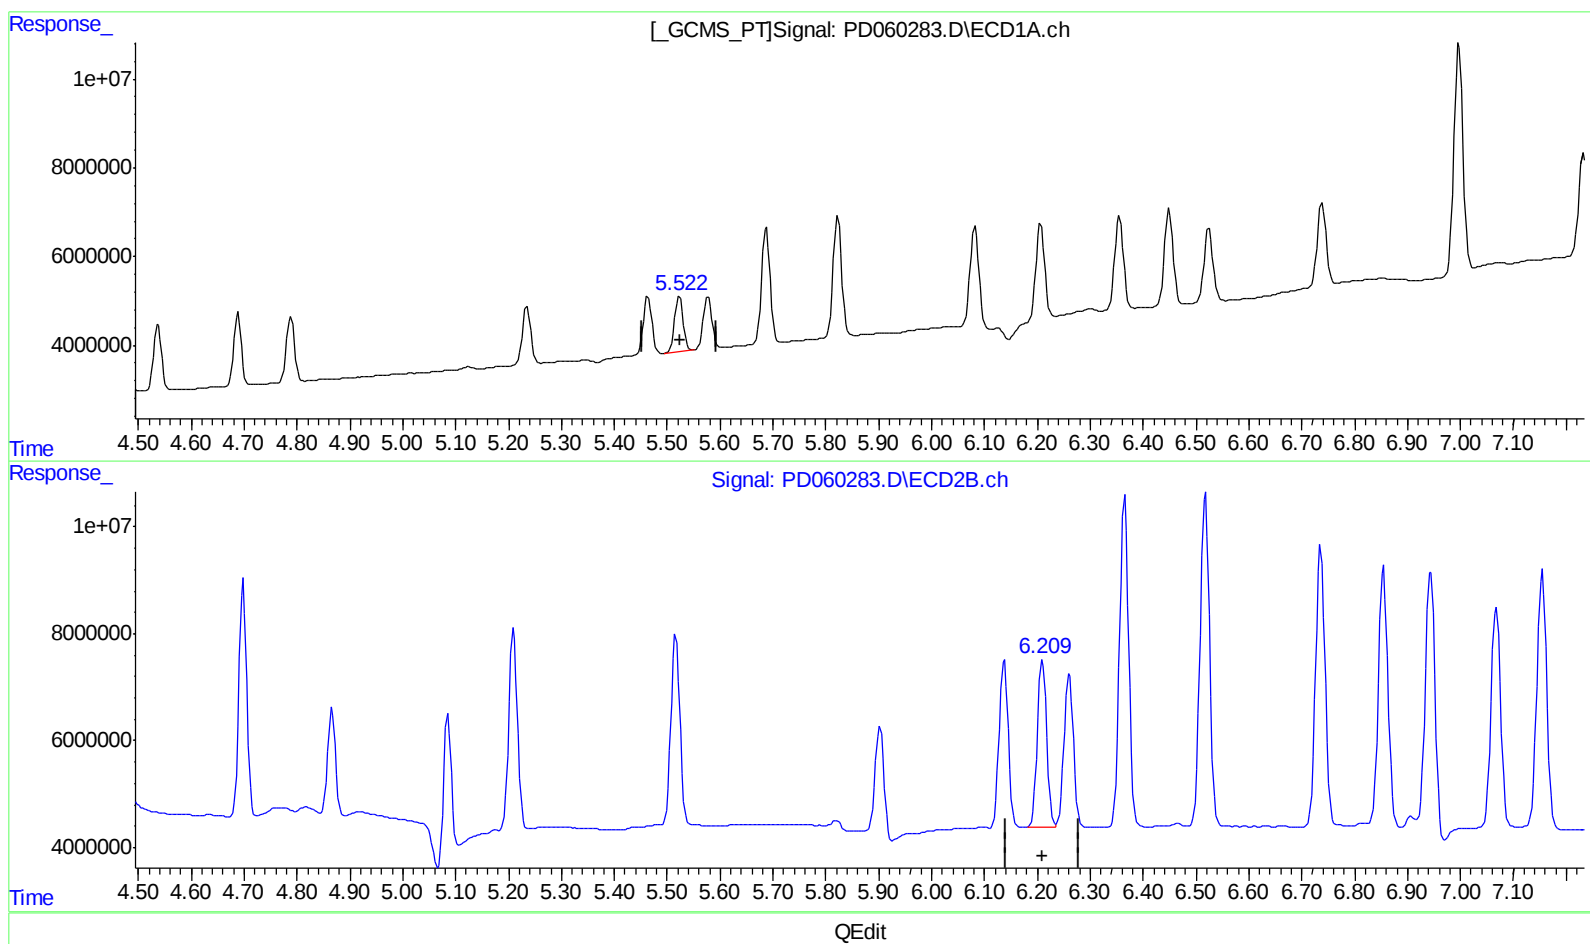

(11) cis-Chlordane (B)

5.523min 9.527 ng/ml

response 14074131

(11) cis-Chlordane #2 (B)

6.210min 9.399 ng/ml

response 38358284