

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
 Data File : PD060315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 17:02
 Operator : DD\AJ
 Sample : L4793-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B38

Manual Integrations
 APPROVED

Ankita
 11/27/2020 12:54:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 05:07:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 26 01:04:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.505	4.022	10655732	33897701	9.702	9.388
27) SA Decachlor...	8.299	9.106	21995611	43672566	16.776	15.629
Target Compounds						
8) B Heptachlo...	5.237	5.897	2705967	12214636	1.808	3.459m#
10) B trans-Chl...	5.470	6.138	1877045	5224632	1.223m	1.254m
11) B cis-Chlor...	5.522	6.214	1453521	17188682	0.984m	4.212 #
12) B 4,4'-DDE	5.689	6.362	1497292	4370621	0.973	1.103m
17) MA 4,4'-DDT	6.450	7.156	2727091	6800701	2.088m	2.056

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 17:02
Operator : DD\AJ
Sample : L4793-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 05:07:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 26 01:04:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

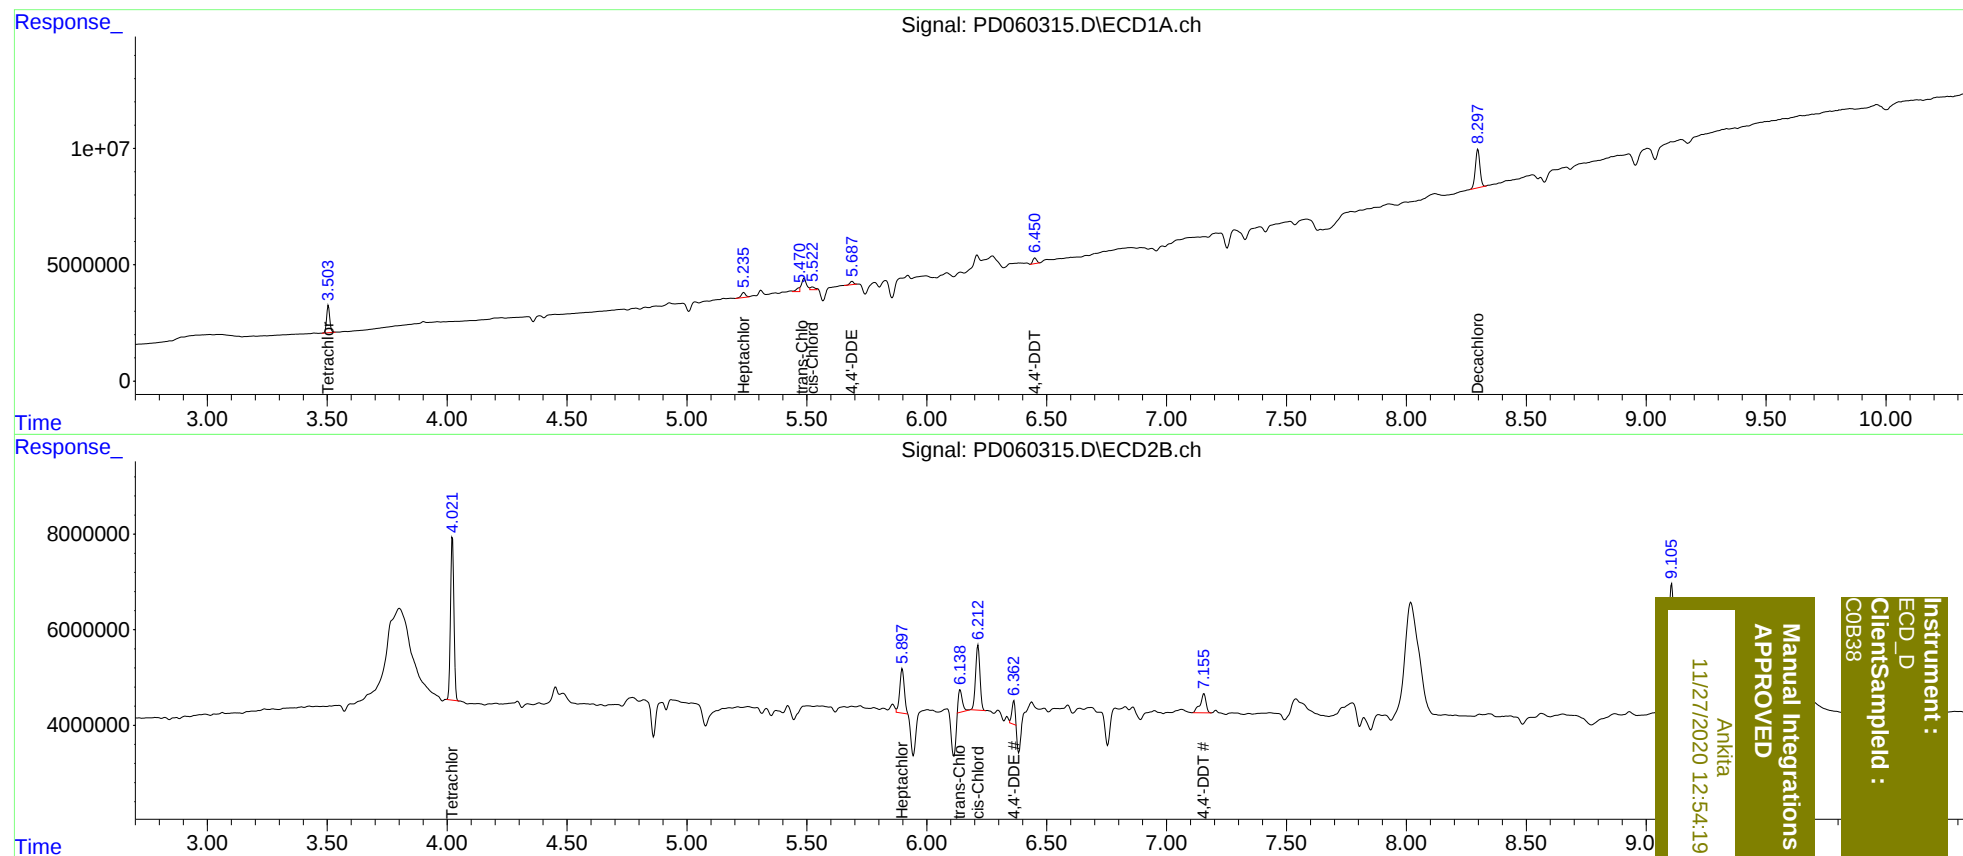

Manual Integrations
APPROVED

Ankita
11/27/2020 12:54:19 PM

Instrument :
ECD_D
ClientSample :
COB38