

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
 Data File : PD060331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 20:46
 Operator : DD\AJ
 Sample : L4859-17
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B95

Manual Integrations
 APPROVED

Ankita
 11/27/2020 12:54:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 01:37:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 26 01:04:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.505	4.023	10668405	34667738	9.714	9.601
27) SA Decachlor...	8.299	9.107	22263176	46648040	16.980	16.694
Target Compounds						
12) B 4,4'-DDE	5.689	6.366	9025803	33482668	5.866	8.453 #
13) MA Dieldrin	5.814	6.524	6374389	2992080	3.988m	0.722m#
14) MA Endrin	6.077	6.727	2352455	12196522	1.741m	3.508 #
16) A 4,4'-DDD	6.209	6.860	4494294	15303423	3.450	4.714 #
17) MA 4,4'-DDT	6.450	7.156	95090603	260.4E6	72.804	78.728

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 20:46
Operator : DD\AJ
Sample : L4859-17
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 01:37:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 26 01:04:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

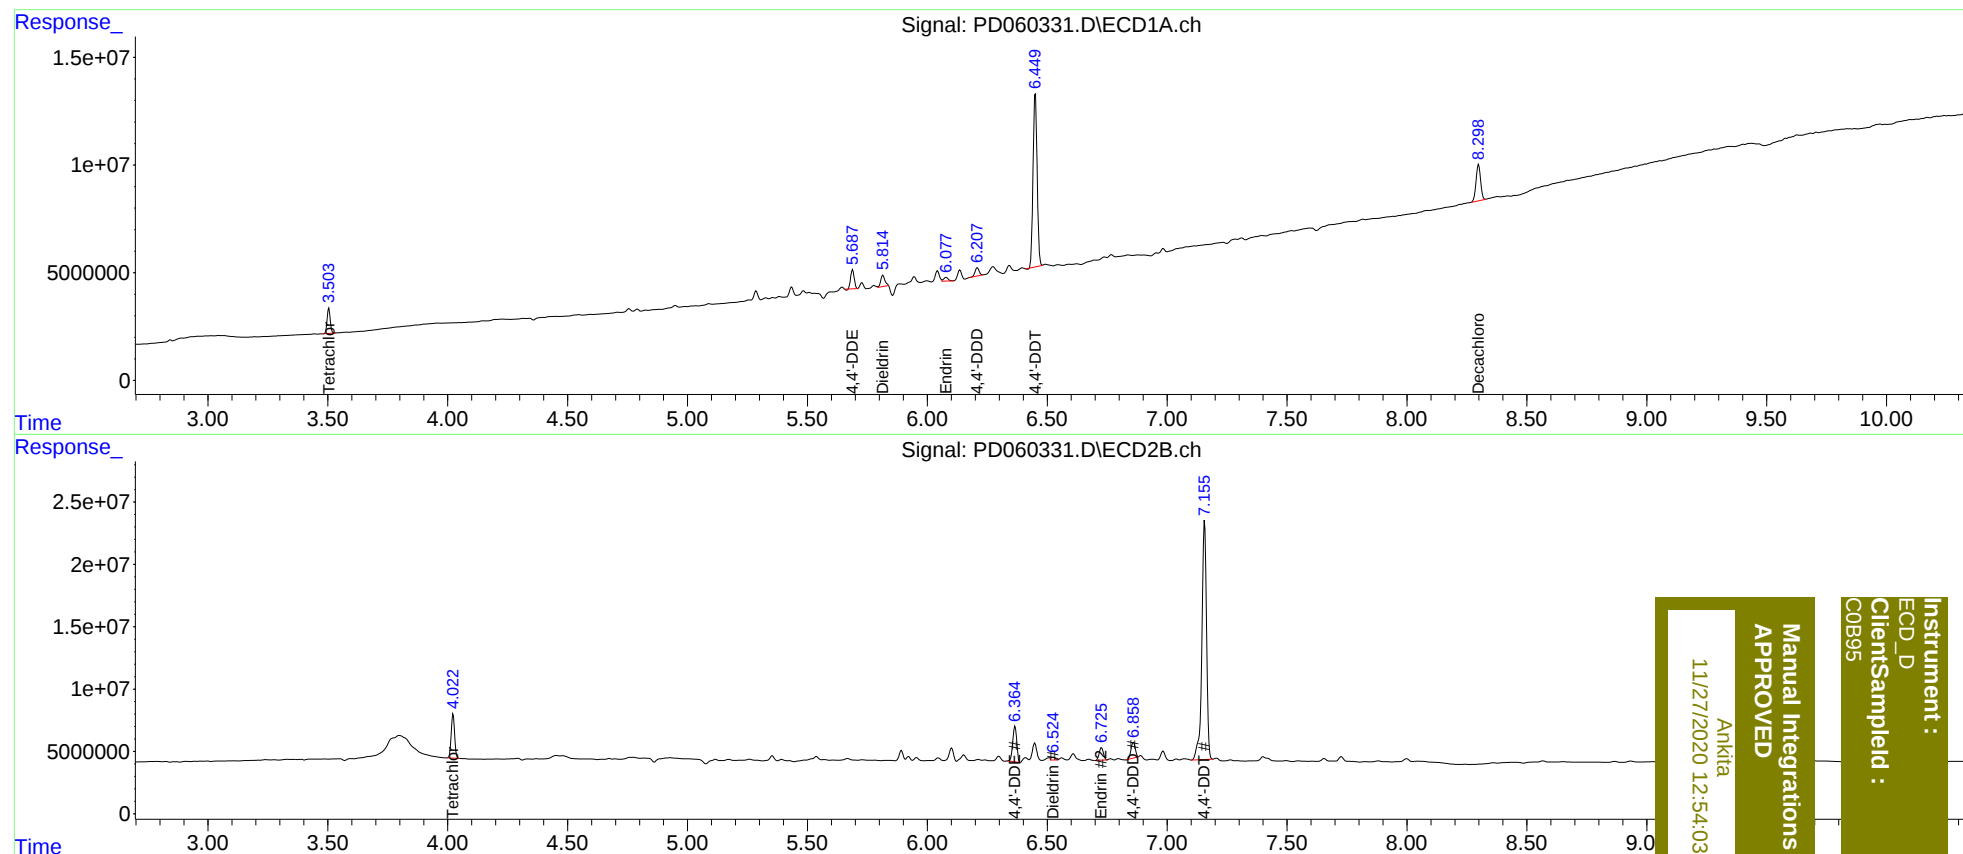

Manual Integrations
APPROVED

Ankita
11/27/2020 12:54:03 PM

Instrument :
ECD_D
ClientSampled :
C0895