

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112525\
 Data File : PD091358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 19:52
 Operator : AR\AJ
 Sample : Q3710-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMPRESSOR-EXCAVATION

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 00:06:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:46:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.873	41852927	480.0E6	12.136	13.105
28)	SA Decachlor...	9.061	8.056	59657627	452.6E6	11.975	11.437
Target Compounds							
12)	B 4,4'-DDE	6.186	5.361	46743986	551.9E6	8.060	10.328 #
16)	A 4,4'-DDD	6.696	5.916	4419764	43087516	0.900	0.882
17)	MA 4,4'-DDT	7.011	6.169	17322900	174.7E6	4.189	4.464



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112525\
Data File : PD091358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 19:52
Operator : AR\AJ
Sample : Q3710-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
COMPRESSOR-EXCAVATION

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 00:06:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:46:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

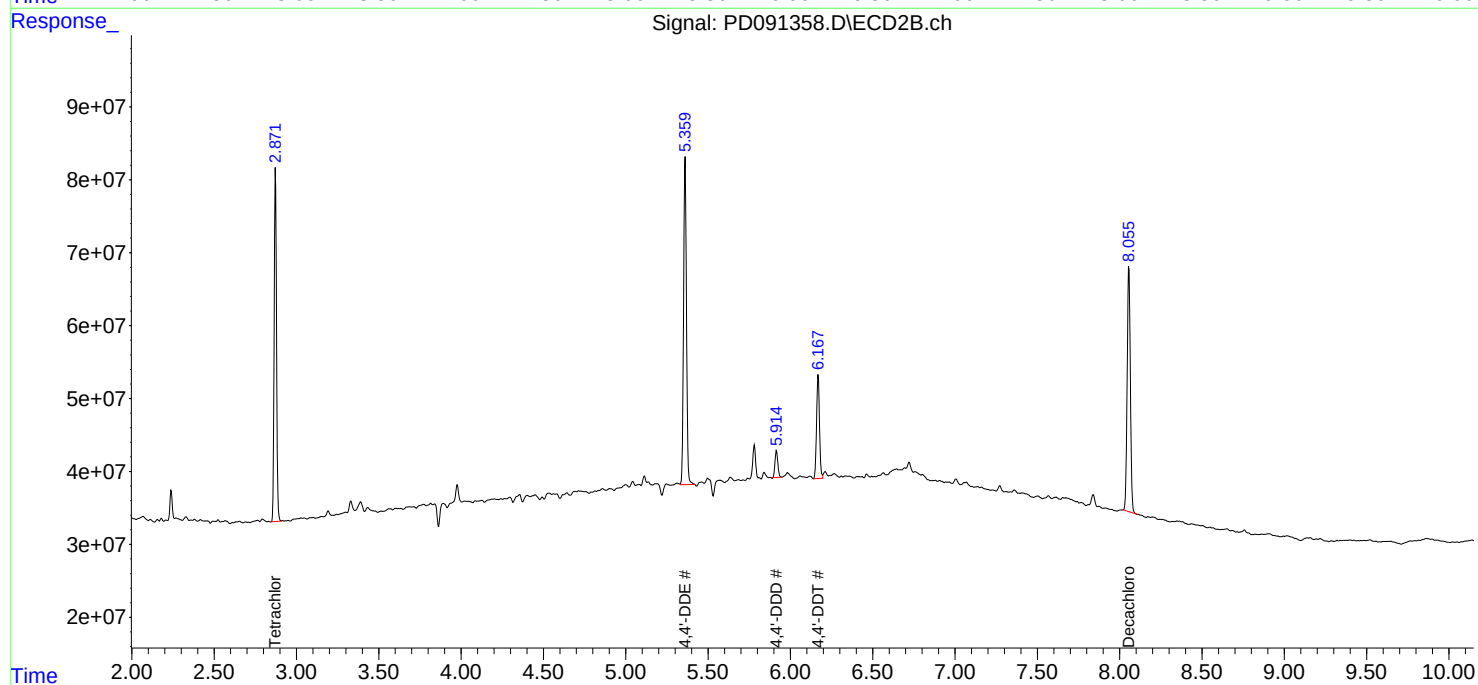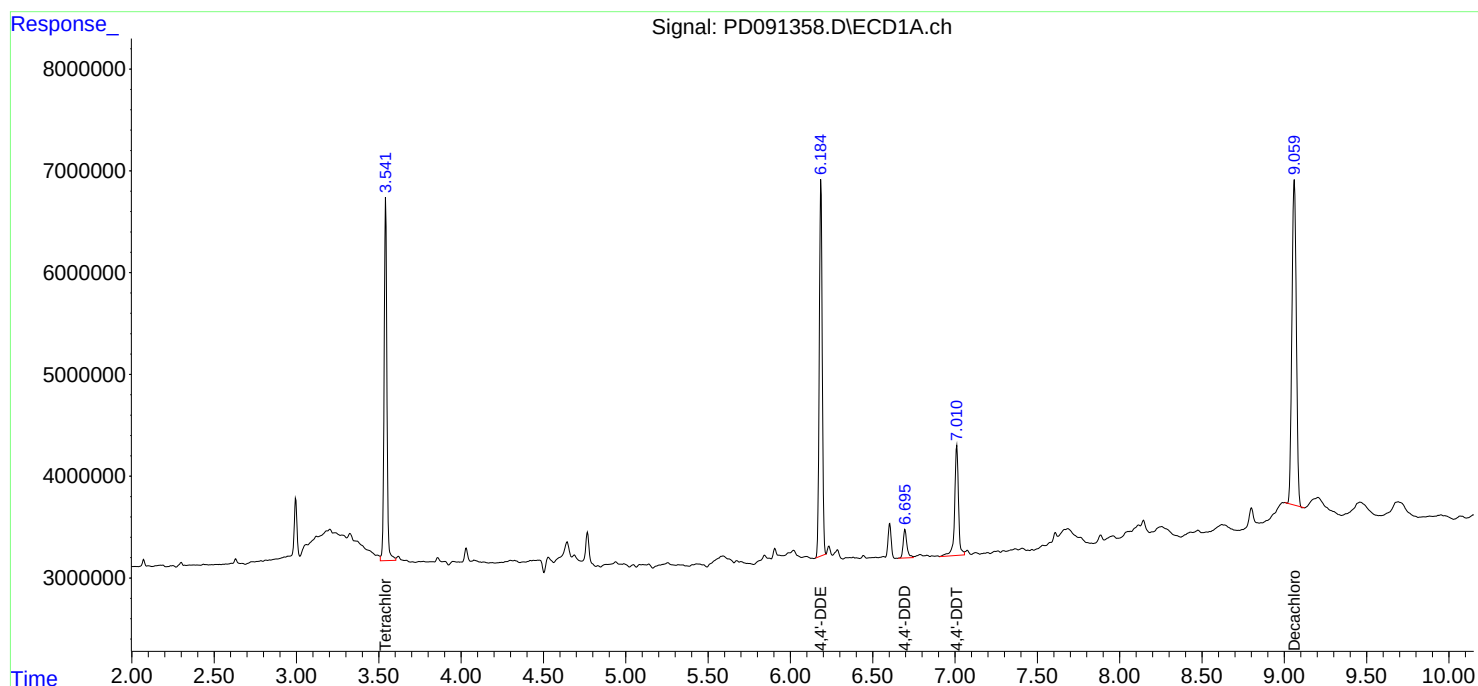


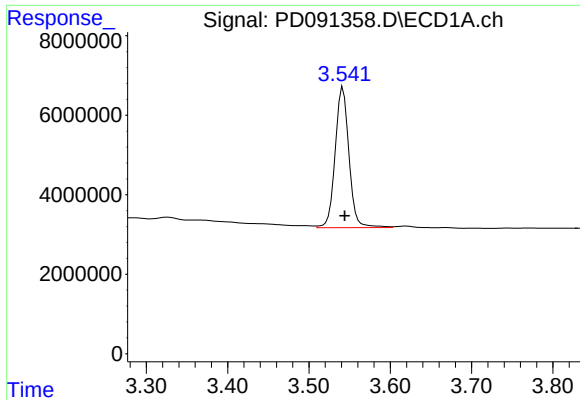

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 41852927
Conc: 12.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPRESSOR-EXCAVATION

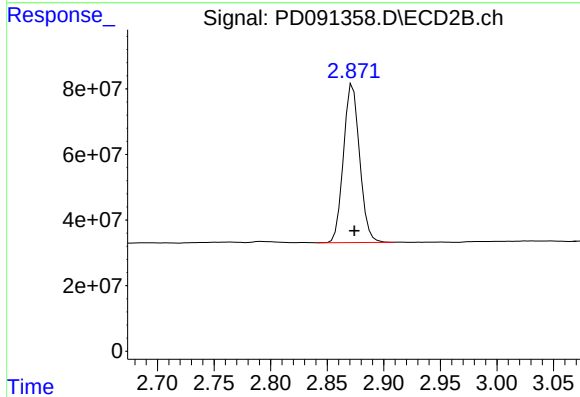


#1 Tetrachloro-m-xylene

R.T.: 2.873 min
Delta R.T.: -0.002 min
Response: 480023708
Conc: 13.10 ng/ml

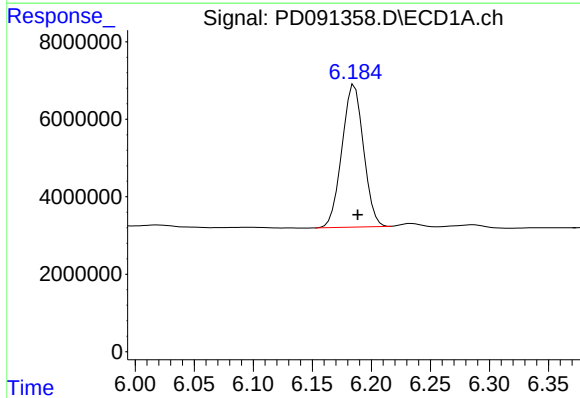


#12 4,4'-DDE

R.T.: 6.186 min
Delta R.T.: -0.003 min
Response: 46743986
Conc: 8.06 ng/ml

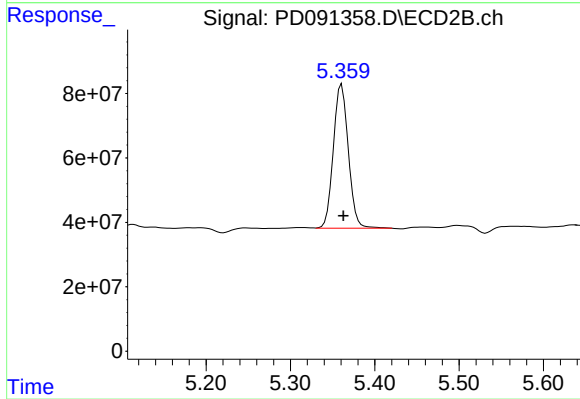

#12 4,4'-DDE


R.T.: 5.361 min
Delta R.T.: -0.002 min
Response: 551940322
Conc: 10.33 ng/ml

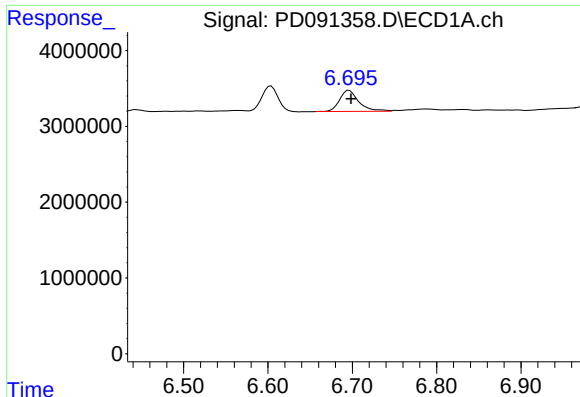

#16 4,4'-DDD


R.T.: 6.696 min
Delta R.T.: -0.002 min
Response: 4419764
Conc: 0.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPRESSOR-EXCAVATION

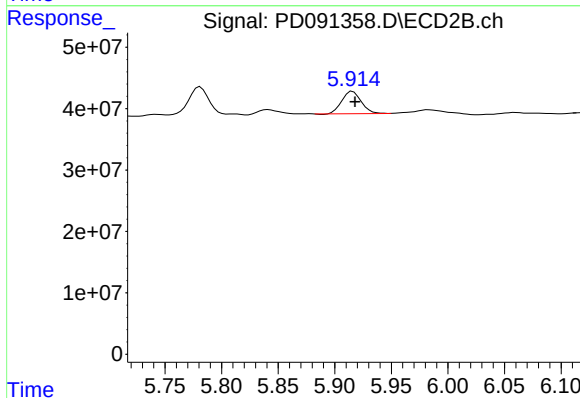


#16 4,4'-DDD

R.T.: 5.916 min
Delta R.T.: -0.002 min
Response: 43087516
Conc: 0.88 ng/ml

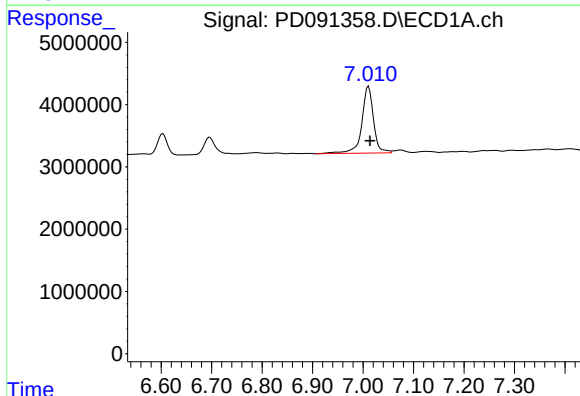


#17 4,4'-DDT

R.T.: 7.011 min
Delta R.T.: -0.003 min
Response: 17322900
Conc: 4.19 ng/ml

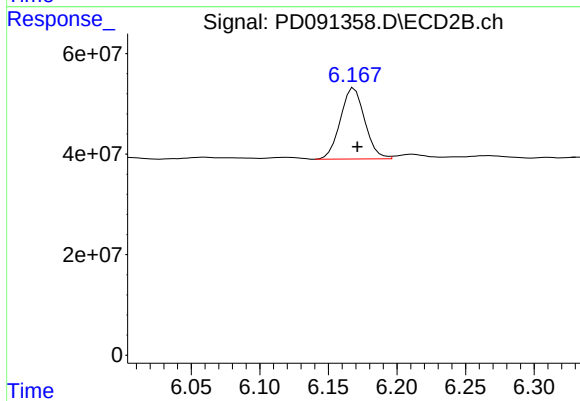

#17 4,4'-DDT


R.T.: 6.169 min
Delta R.T.: -0.002 min
Response: 174680442
Conc: 4.46 ng/ml

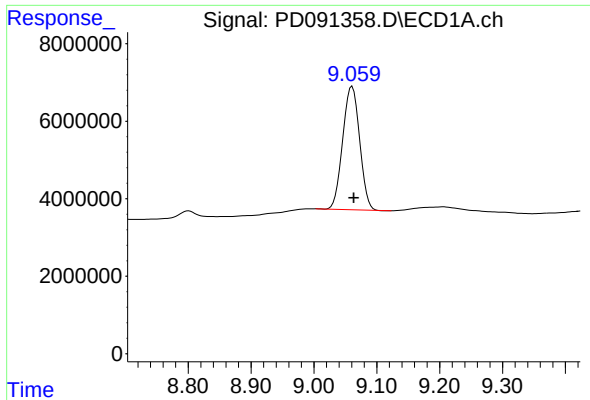

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: -0.002 min
Response: 59657627
Conc: 11.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPRESSOR-EXCAVATION

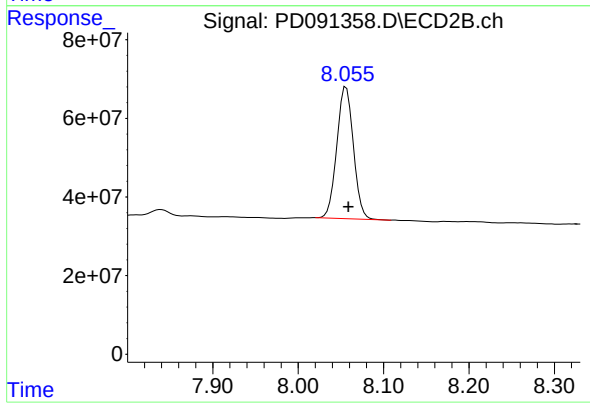

#28 Decachlorobiphenyl

R.T.: 8.056 min
Delta R.T.: -0.002 min
Response: 452628578
Conc: 11.44 ng/ml