

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
 Data File : PD060344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2020 15:33
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 01:36:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:35:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.023	6149288	18781581	5.464	5.105
27)	SA Decachlor...	8.293	9.108	14922972	32019109	11.255	11.312
Target Compounds							
2)	A alpha-BHC	3.944	4.413	8412809	27471109	5.263	5.098
3)	MA gamma-BHC...	4.230	4.699	8226950	24717225	5.426	5.030
4)	MA Heptachlor	4.537	5.211	8196384	24916130	5.371	5.201
9)	A Endosulfan I	5.575	6.262	7272191	20341966	5.397	5.260
13)	MA Dieldrin	5.821	6.519	15514194	43196088	10.445	10.309
14)	MA Endrin	6.079	6.738	13134445	35516593	10.830	10.438
16)	A 4,4'-DDD	6.203	6.857	12665400	33207648	10.668	10.122
17)	MA 4,4'-DDT	6.447	7.156	12093708	33054048	10.138	10.270
20)	A Methoxychlor	6.993	7.613	31790385	89507957	54.222	55.204


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
Data File : PD060344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2020 15:33
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 01:36:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:35:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

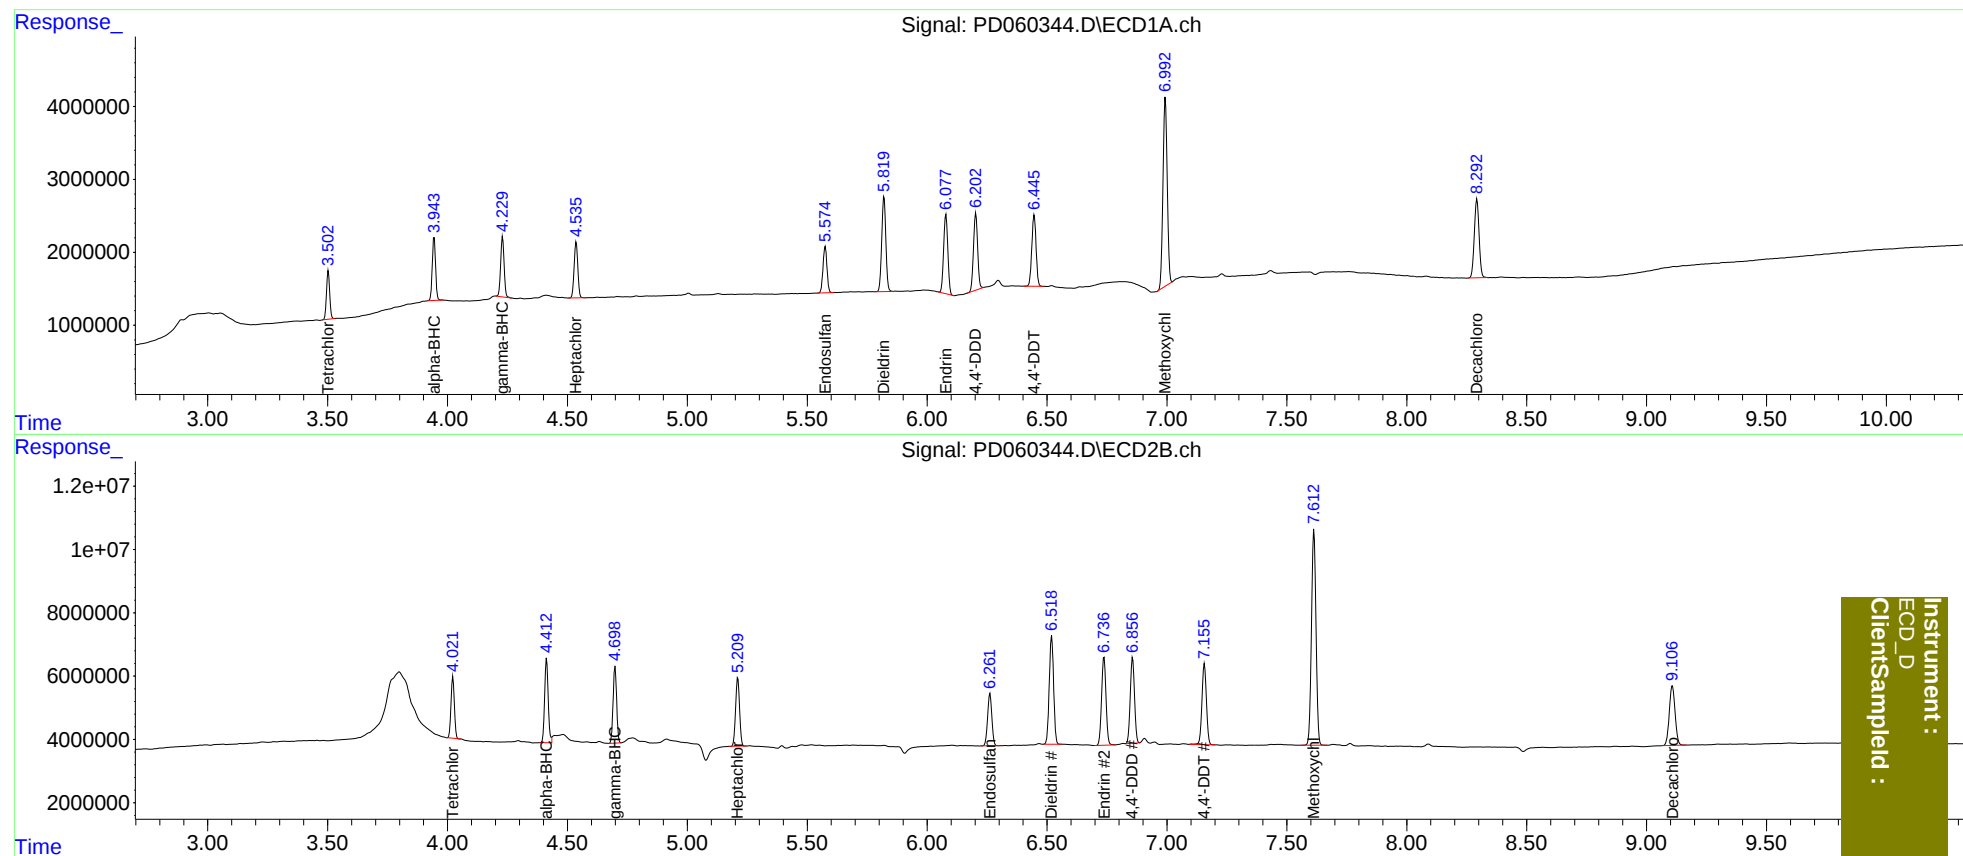


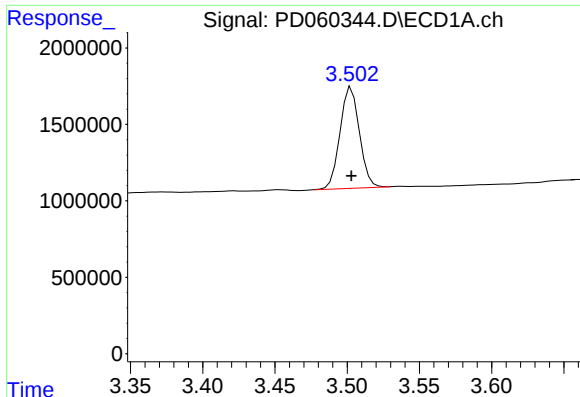

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 6149288
Conc: 5.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

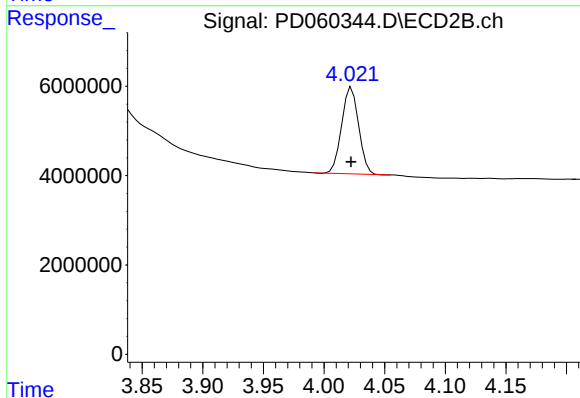


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 18781581
Conc: 5.10 ng/ml

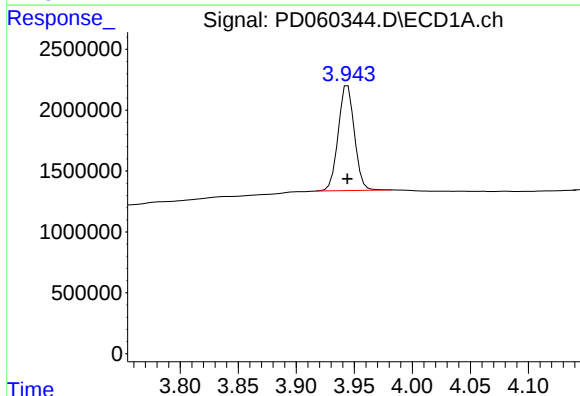


#2 alpha-BHC

R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 8412809
Conc: 5.26 ng/ml

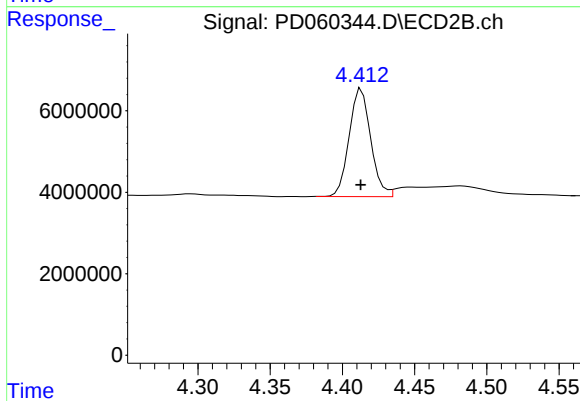

#2 alpha-BHC


R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 27471109
Conc: 5.10 ng/ml

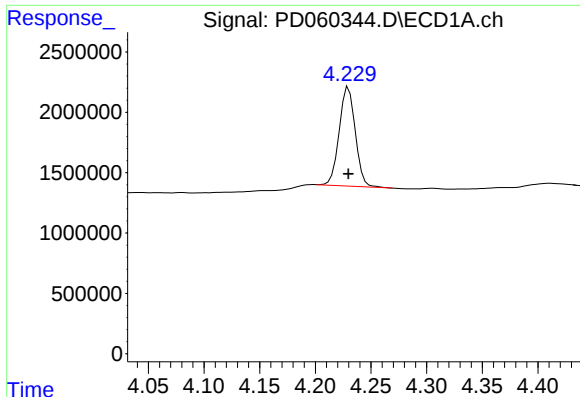

#3 gamma-BHC (Lindane)


R.T.: 4.230 min
Delta R.T.: 0.000 min
Response: 8226950
Conc: 5.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

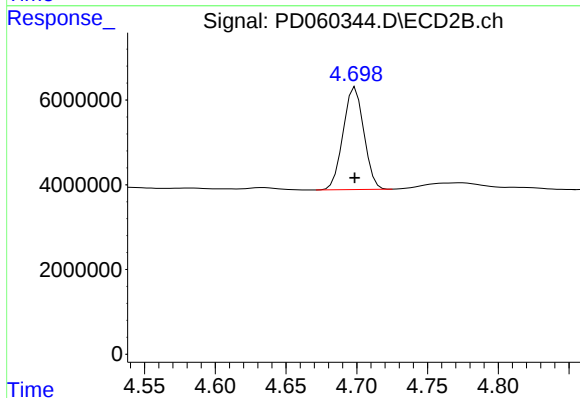


#3 gamma-BHC (Lindane)

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 24717225
Conc: 5.03 ng/ml

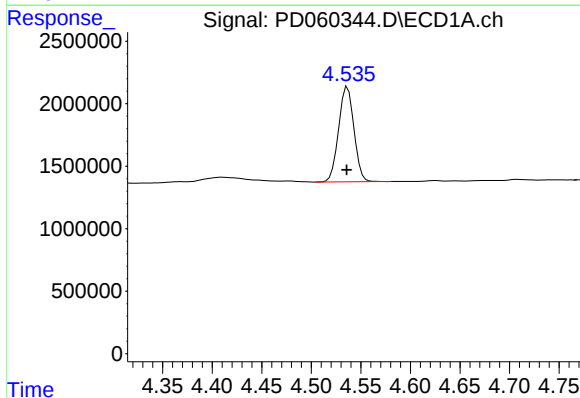


#4 Heptachlor

R.T.: 4.537 min
Delta R.T.: 0.000 min
Response: 8196384
Conc: 5.37 ng/ml

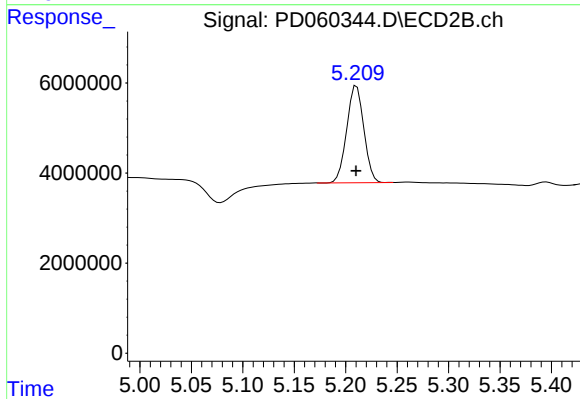

#4 Heptachlor


R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 24916130
Conc: 5.20 ng/ml

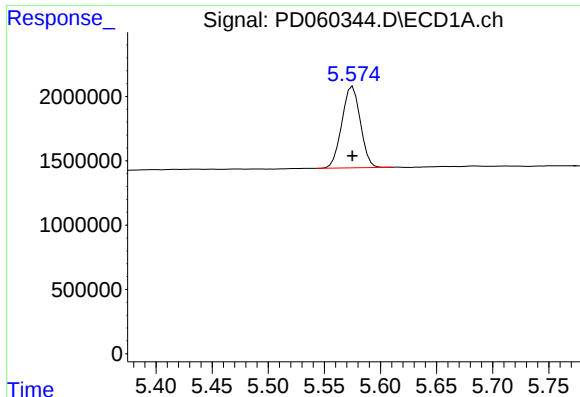

#9 Endosulfan I


R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 7272191
Conc: 5.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

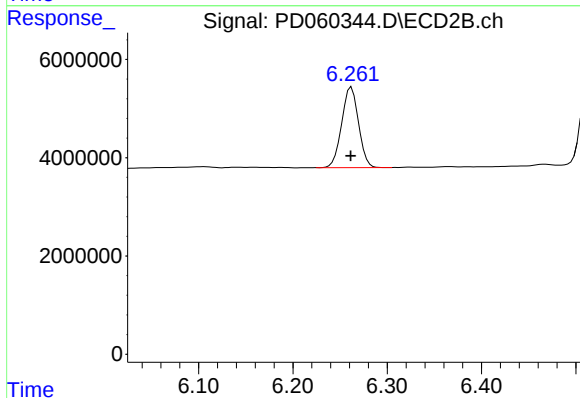


#9 Endosulfan I

R.T.: 6.262 min
Delta R.T.: 0.000 min
Response: 20341966
Conc: 5.26 ng/ml

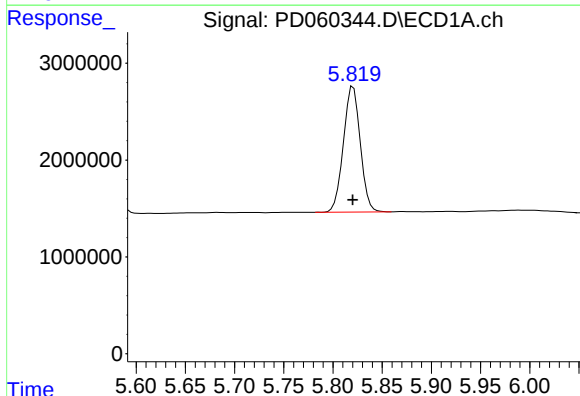


#13 Dieldrin

R.T.: 5.821 min
Delta R.T.: 0.000 min
Response: 15514194
Conc: 10.44 ng/ml

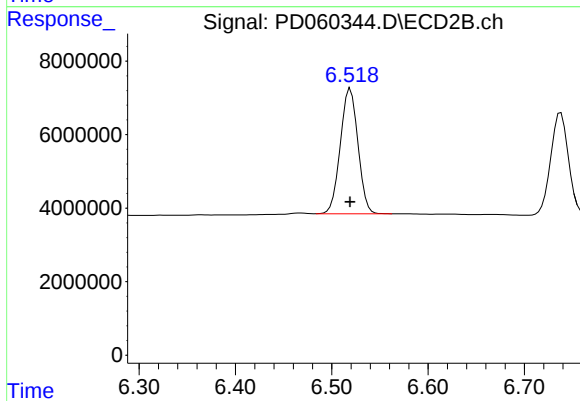

#13 Dieldrin


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 43196088
Conc: 10.31 ng/ml

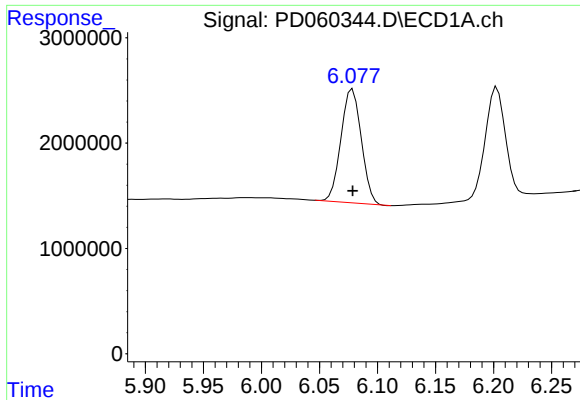

#14 Endrin


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 13134445
Conc: 10.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

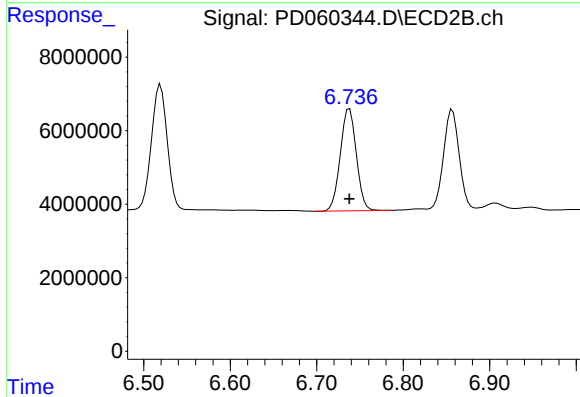


#14 Endrin

R.T.: 6.738 min
Delta R.T.: 0.000 min
Response: 35516593
Conc: 10.44 ng/ml

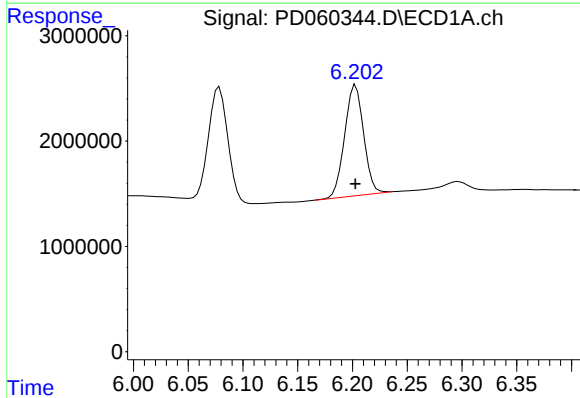


#16 4,4'-DDD

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 12665400
Conc: 10.67 ng/ml

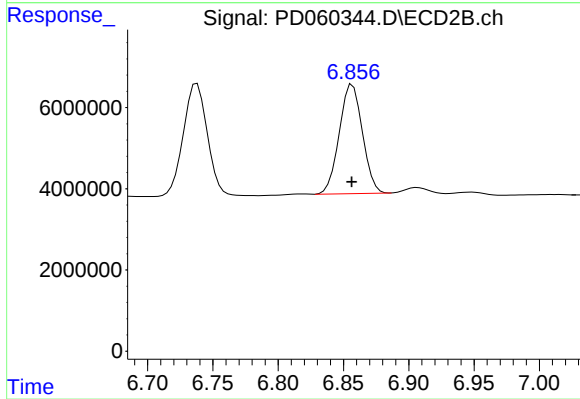

#16 4,4'-DDD


R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 33207648
Conc: 10.12 ng/ml

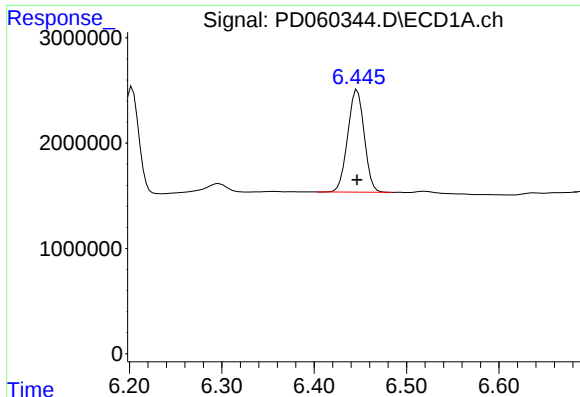

#17 4,4'-DDT


R.T.: 6.447 min
Delta R.T.: 0.000 min
Response: 12093708
Conc: 10.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

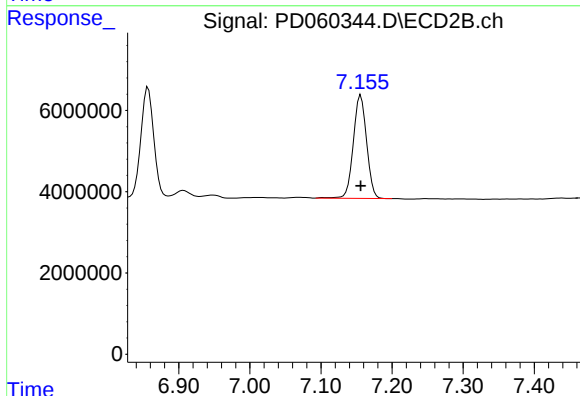


#17 4,4'-DDT

R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 33054048
Conc: 10.27 ng/ml

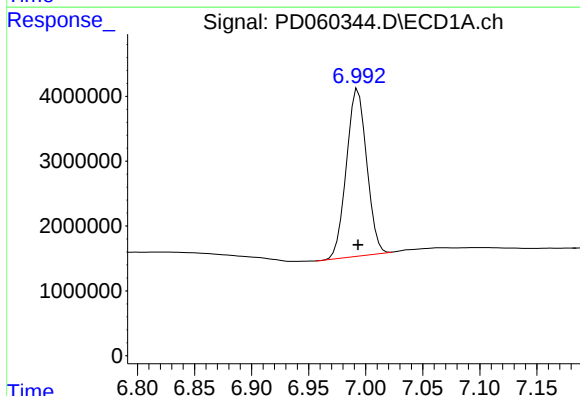


#20 Methoxychlor

R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 31790385
Conc: 54.22 ng/ml

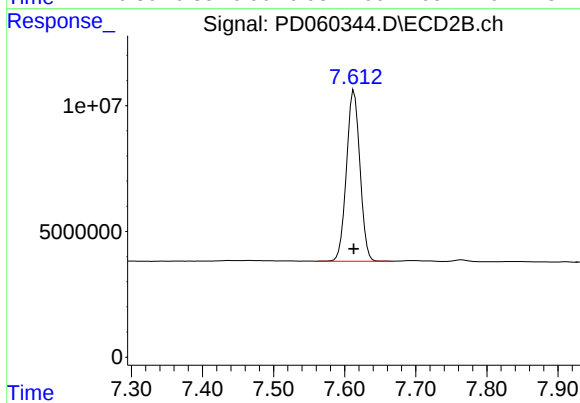

#20 Methoxychlor


R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 89507957
Conc: 55.20 ng/ml

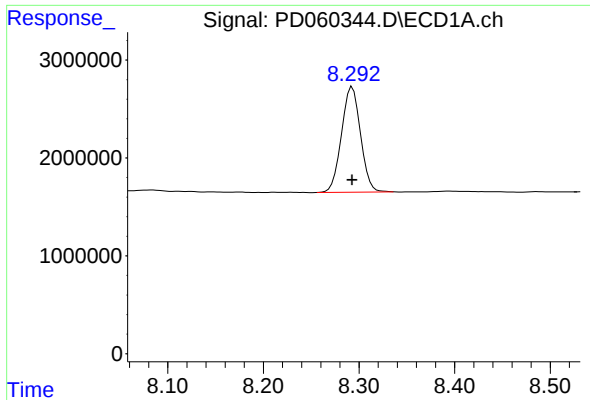

#27 Decachlorobiphenyl

R.T.: 8.293 min
Delta R.T.: 0.000 min
Response: 14922972
Conc: 11.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

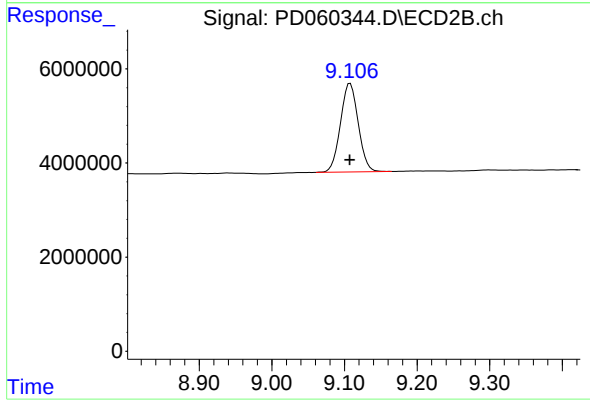

#27 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.000 min
Response: 32019109
Conc: 11.31 ng/ml