

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
 Data File : PD060346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2020 16:01
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 01:36:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:35:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.023	11850894	37526278	10.530	10.199
27)	SA Decachlor...	8.293	9.106	28469927	60956261	21.472	21.536
Target Compounds							
2)	A alpha-BHC	3.944	4.413	16292757	54469622	10.193	10.109
3)	MA gamma-BHC...	4.230	4.699	15592231	49542687	10.284	10.082
4)	MA Heptachlor	4.536	5.210	15840199	49051126	10.379	10.238
9)	A Endosulfan I	5.575	6.262	14170419	39947378	10.517	10.329
13)	MA Dieldrin	5.820	6.519	30404373	85934026	20.469	20.508
14)	MA Endrin	6.079	6.738	25375040	72007069	20.924	21.163
16)	A 4,4'-DDD	6.203	6.856	24420389	67089114	20.570	20.450
17)	MA 4,4'-DDT	6.445	7.156	24147117	65438766	20.242	20.332
20)	A Methoxychlor	6.993	7.612	61449528	172.9E6	104.810	106.637

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
Data File : PD060346.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2020 16:01
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 01:36:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:35:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

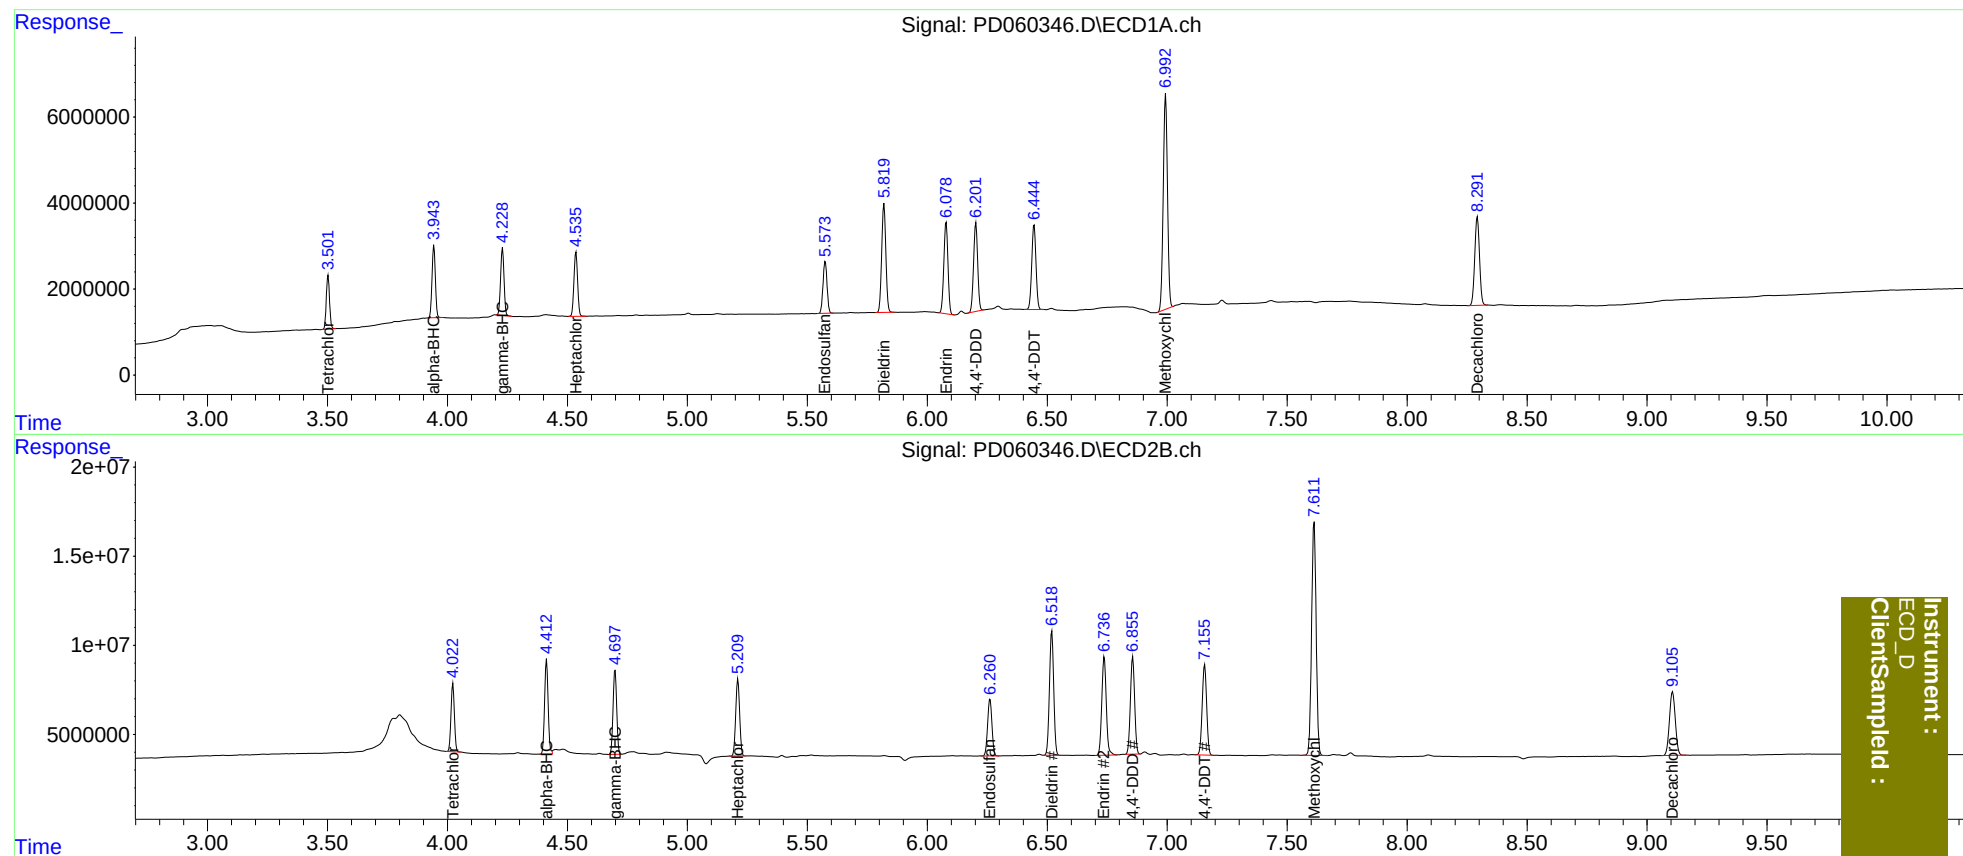


Instrument :
ECD_D
ClientSampled :

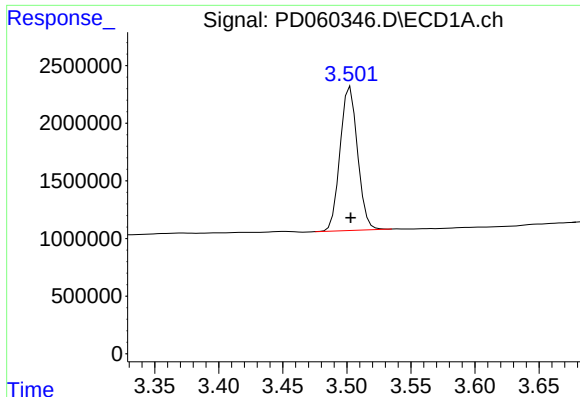

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 11850894
Conc: 10.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

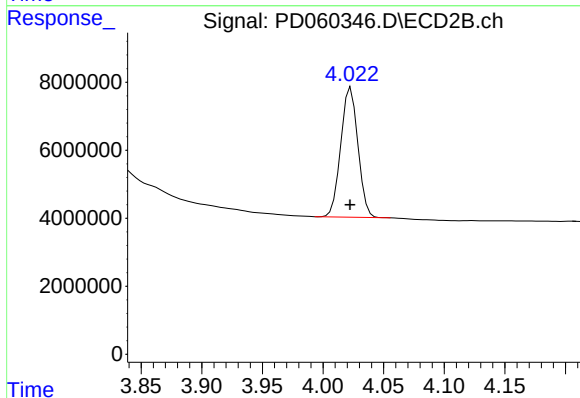


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 37526278
Conc: 10.20 ng/ml

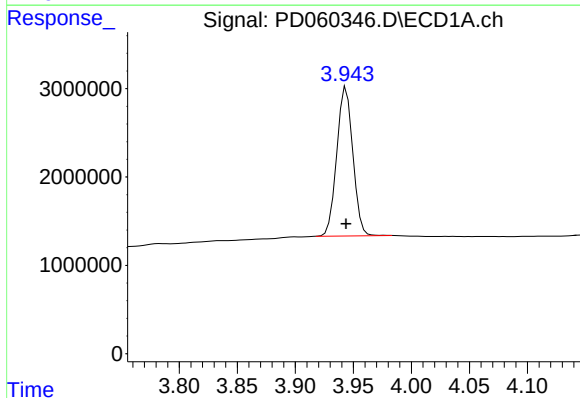


#2 alpha-BHC

R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 16292757
Conc: 10.19 ng/ml

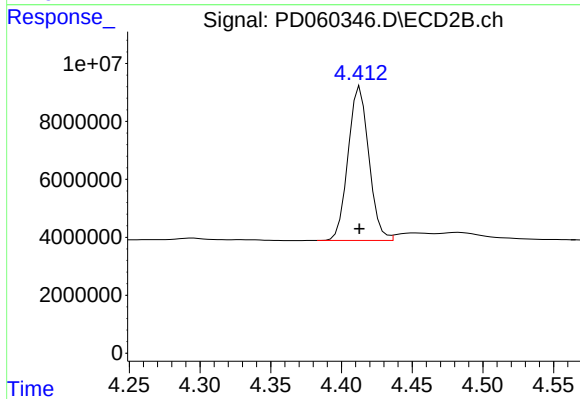

#2 alpha-BHC


R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 54469622
Conc: 10.11 ng/ml

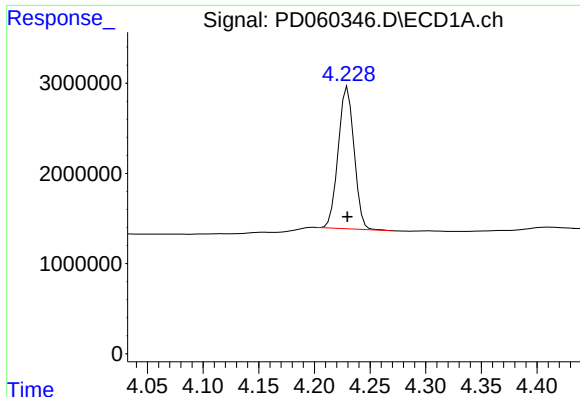

#3 gamma-BHC (Lindane)


R.T.: 4.230 min
Delta R.T.: 0.000 min
Response: 15592231
Conc: 10.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

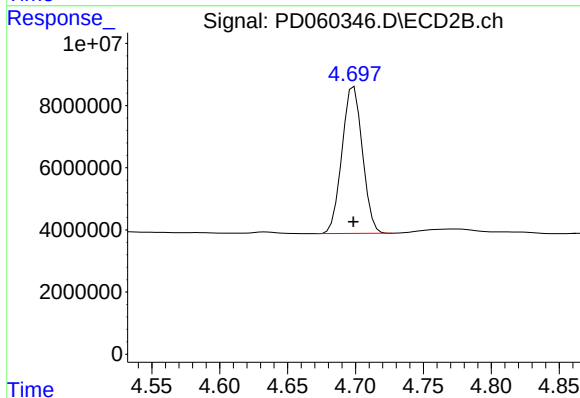


#3 gamma-BHC (Lindane)

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 49542687
Conc: 10.08 ng/ml

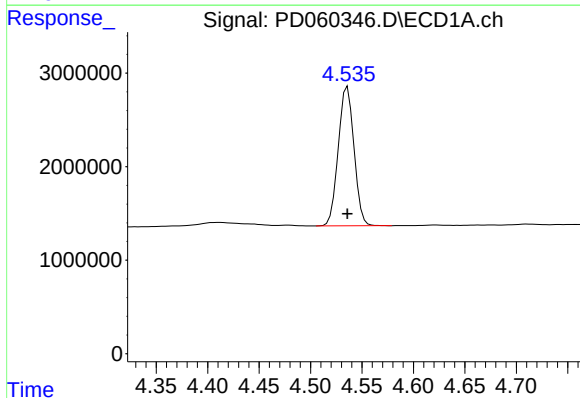


#4 Heptachlor

R.T.: 4.536 min
Delta R.T.: 0.000 min
Response: 15840199
Conc: 10.38 ng/ml

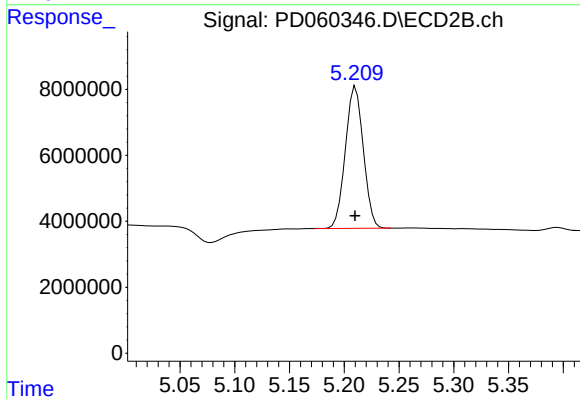

#4 Heptachlor


R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 49051126
Conc: 10.24 ng/ml

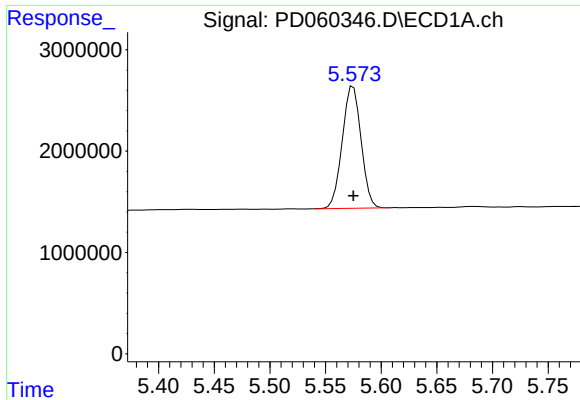

#9 Endosulfan I


R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 14170419
Conc: 10.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

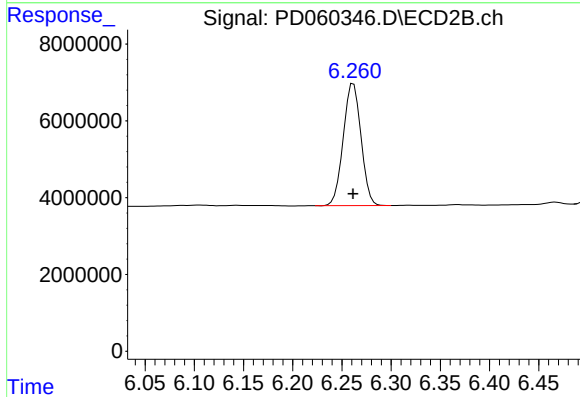


#9 Endosulfan I

R.T.: 6.262 min
Delta R.T.: 0.000 min
Response: 39947378
Conc: 10.33 ng/ml

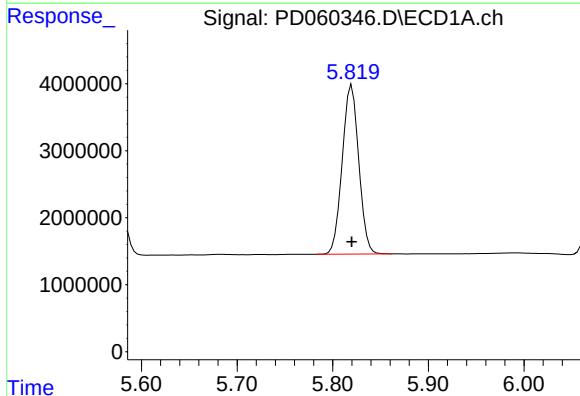


#13 Dieldrin

R.T.: 5.820 min
Delta R.T.: 0.000 min
Response: 30404373
Conc: 20.47 ng/ml

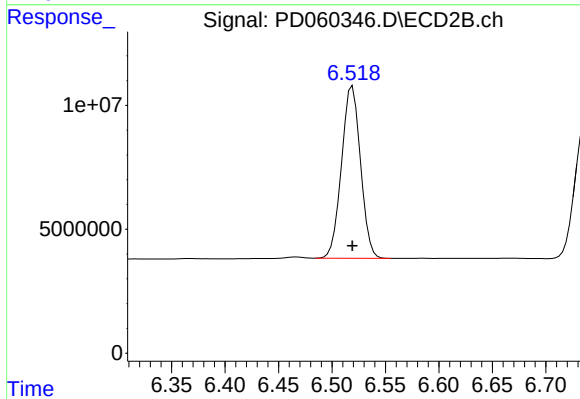

#13 Dieldrin


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 85934026
Conc: 20.51 ng/ml

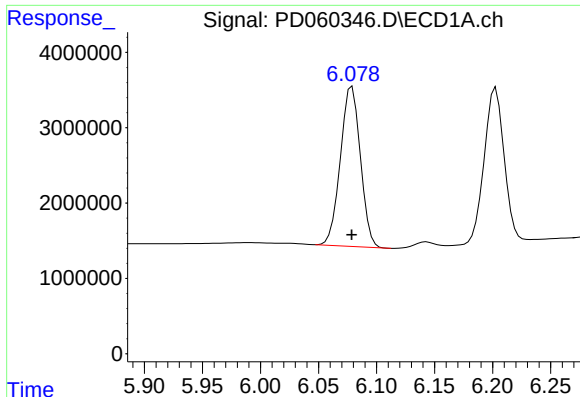

#14 Endrin


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 25375040
Conc: 20.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

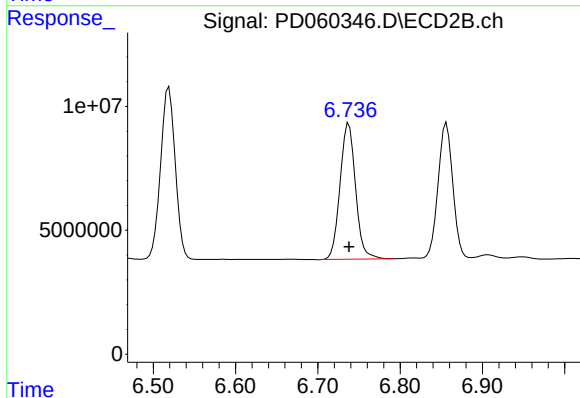


#14 Endrin

R.T.: 6.738 min
Delta R.T.: 0.000 min
Response: 72007069
Conc: 21.16 ng/ml

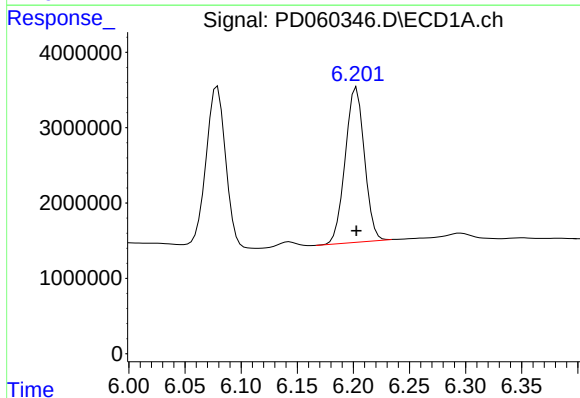


#16 4,4'-DDD

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 24420389
Conc: 20.57 ng/ml

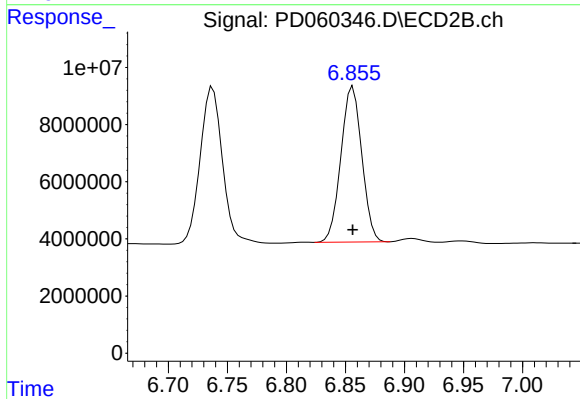

#16 4,4'-DDD


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 67089114
Conc: 20.45 ng/ml

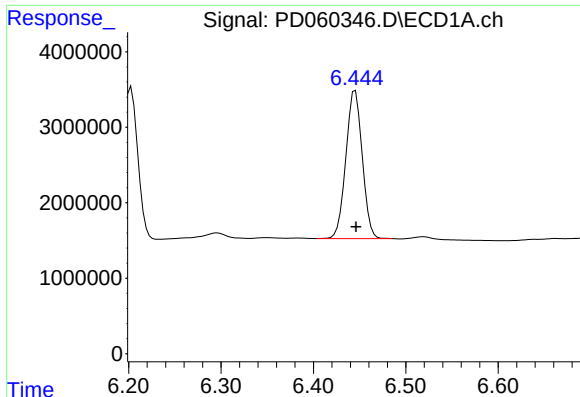

#17 4,4'-DDT


R.T.: 6.445 min
Delta R.T.: 0.000 min
Response: 24147117
Conc: 20.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

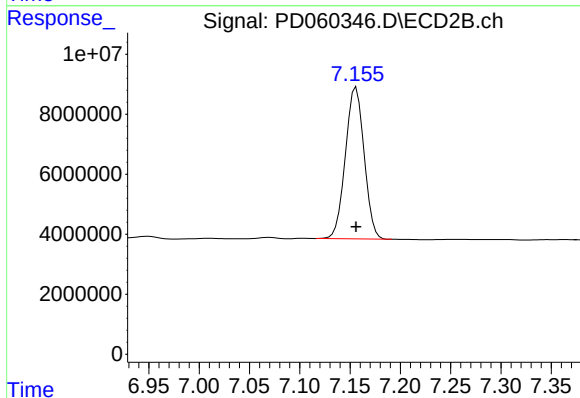


#17 4,4'-DDT

R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 65438766
Conc: 20.33 ng/ml

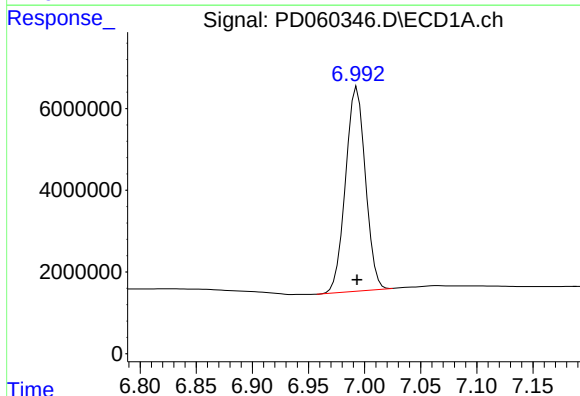


#20 Methoxychlor

R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 61449528
Conc: 104.81 ng/ml

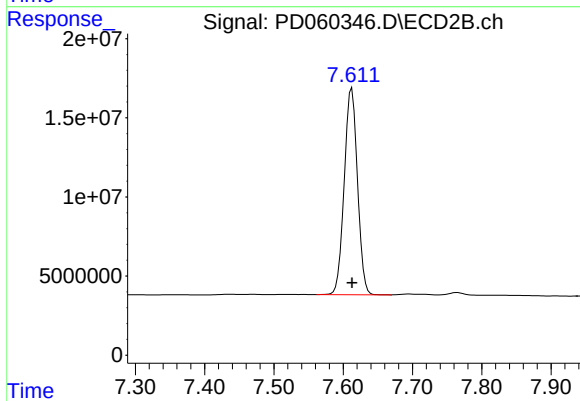

#20 Methoxychlor


R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 172903426
Conc: 106.64 ng/ml

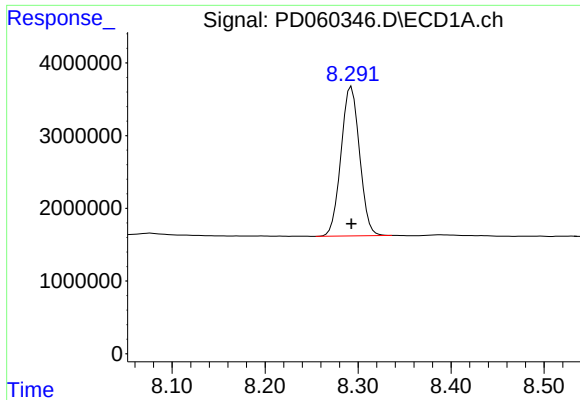

#27 Decachlorobiphenyl

R.T.: 8.293 min
Delta R.T.: 0.000 min
Response: 28469927
Conc: 21.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

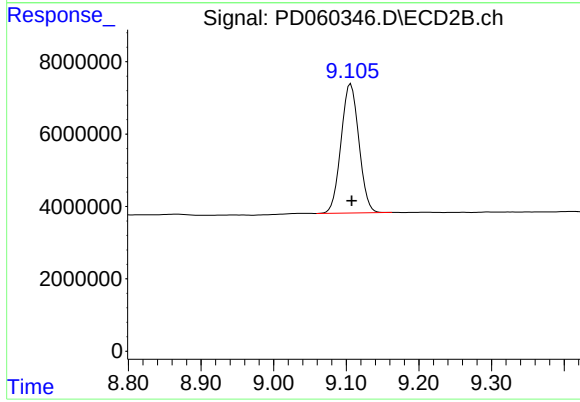

#27 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: -0.001 min
Response: 60956261
Conc: 21.54 ng/ml