

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
 Data File : PD060348.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2020 16:29
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 01:36:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:35:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.022	22508827	73588047	20.000	20.000
27)	SA Decachlor...	8.293	9.107	53037028	113.2E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.944	4.413	31967648	107.8E6	20.000	20.000
3)	MA gamma-BHC...	4.230	4.699	30323711	98284322	20.000	20.000
4)	MA Heptachlor	4.536	5.210	30523270	95817166	20.000	20.000
9)	A Endosulfan I	5.575	6.261	26948658	77346423	20.000	20.000
13)	MA Dieldrin	5.820	6.519	59414481	167.6E6	40.000	40.000
14)	MA Endrin	6.079	6.738	48509953	136.1E6	40.000	40.000
16)	A 4,4'-DDD	6.203	6.856	47488243	131.2E6	40.000	40.000
17)	MA 4,4'-DDT	6.446	7.156	47716704	128.7E6	40.000	40.000
20)	A Methoxychlor	6.993	7.613	117.3E6	324.3E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
Data File : PD060348.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2020 16:29
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 01:36:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:35:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

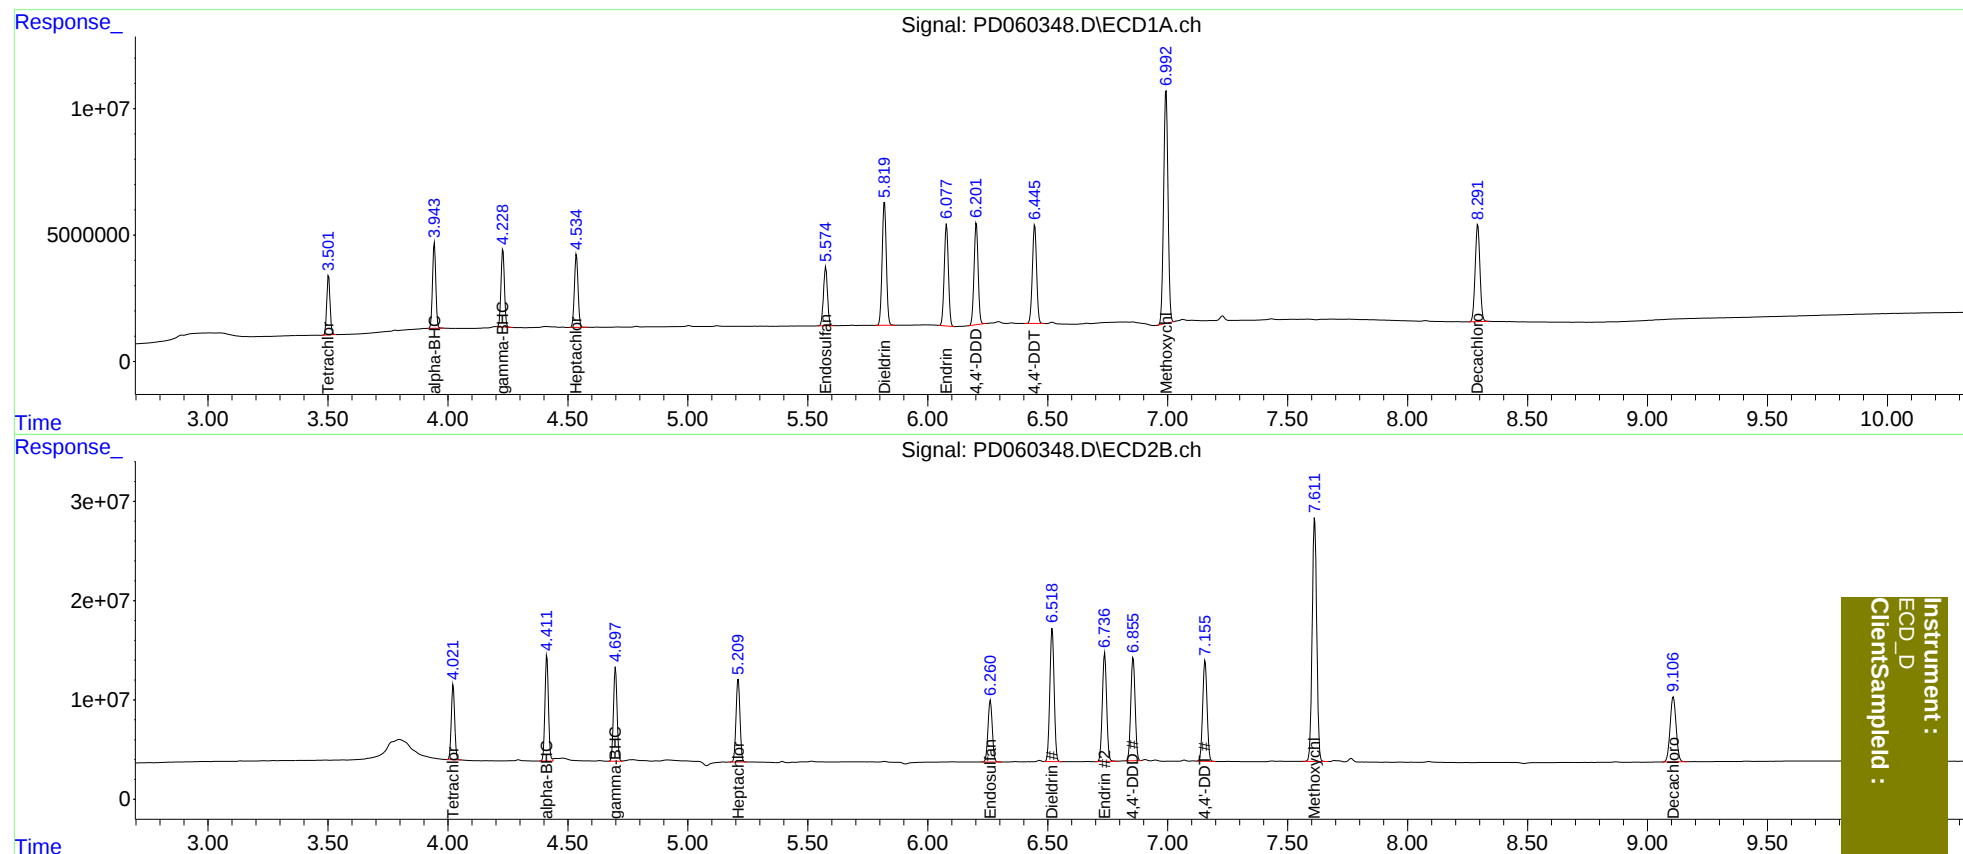


Instrument :
ECD_D
ClientSampled :

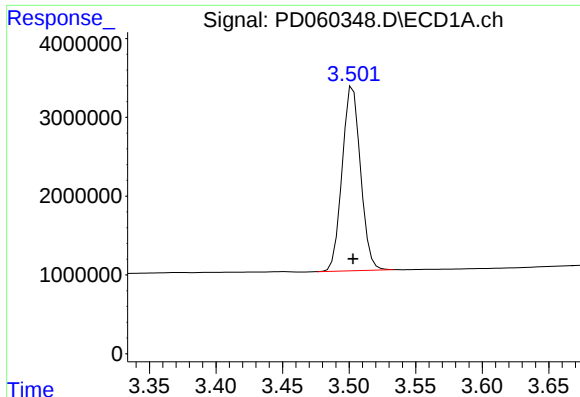

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 22508827
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

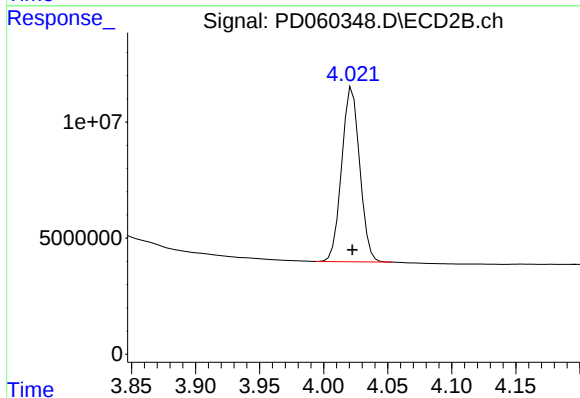


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 73588047
Conc: 20.00 ng/ml

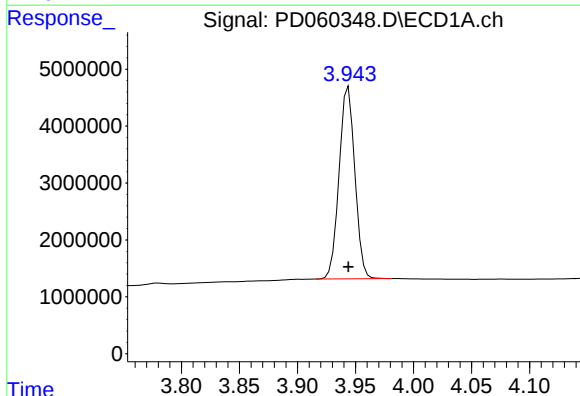


#2 alpha-BHC

R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 31967648
Conc: 20.00 ng/ml

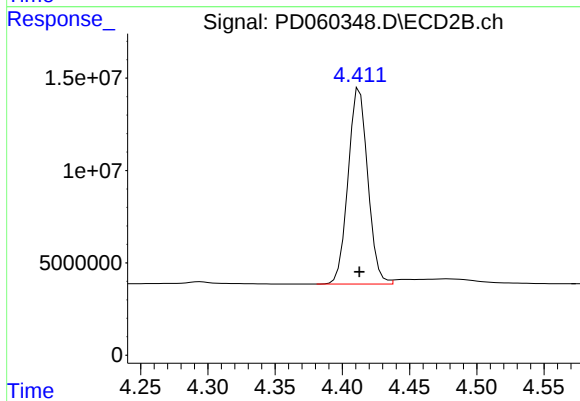

#2 alpha-BHC


R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 107768586
Conc: 20.00 ng/ml

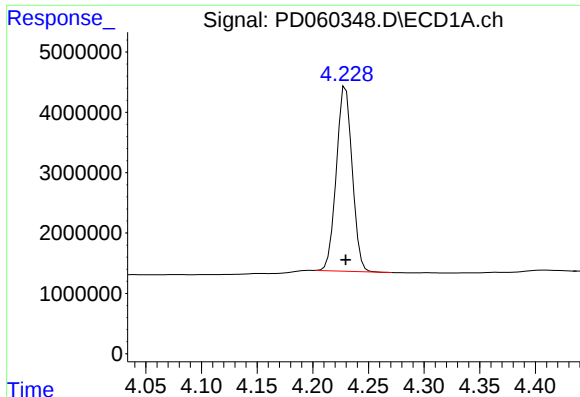

#3 gamma-BHC (Lindane)


R.T.: 4.230 min
Delta R.T.: 0.000 min
Response: 30323711
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

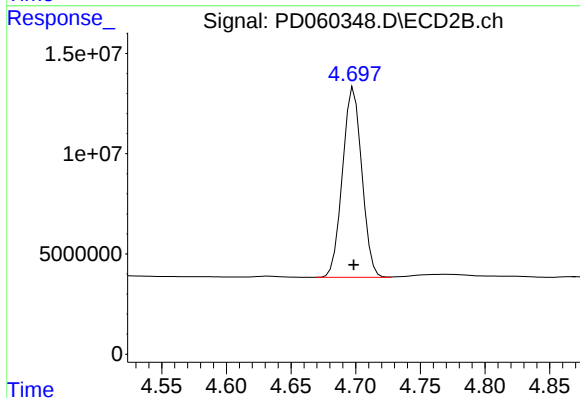


#3 gamma-BHC (Lindane)

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 98284322
Conc: 20.00 ng/ml

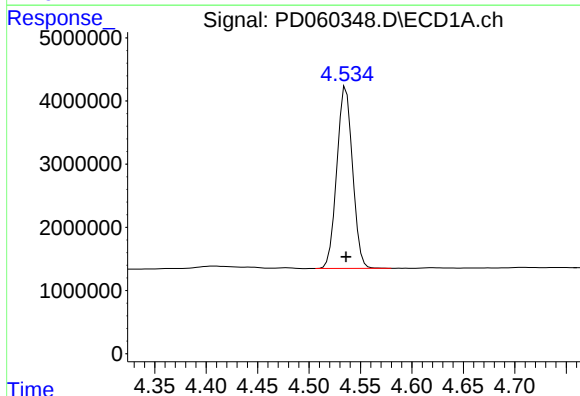


#4 Heptachlor

R.T.: 4.536 min
Delta R.T.: 0.000 min
Response: 30523270
Conc: 20.00 ng/ml

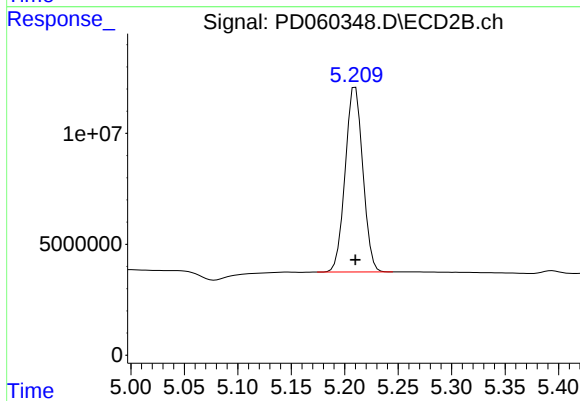

#4 Heptachlor


R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 95817166
Conc: 20.00 ng/ml

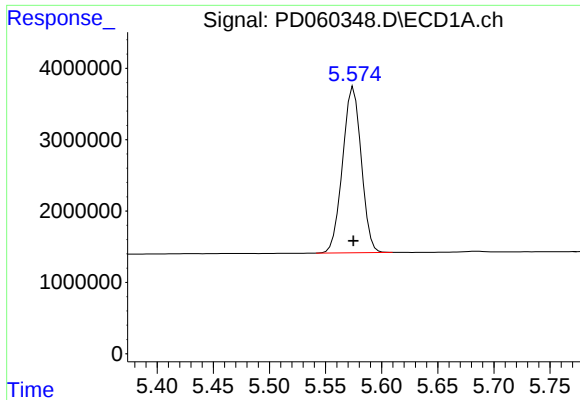

#9 Endosulfan I


R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 26948658
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

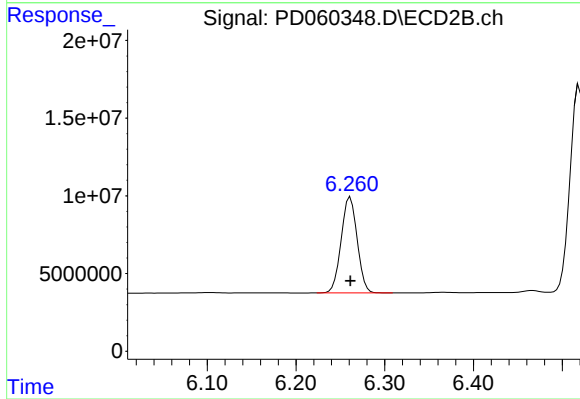


#9 Endosulfan I

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 77346423
Conc: 20.00 ng/ml

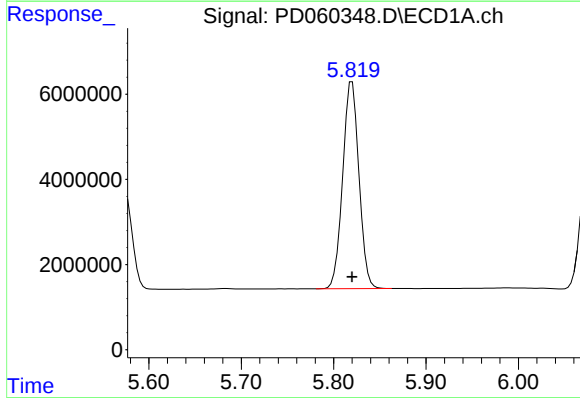


#13 Dieldrin

R.T.: 5.820 min
Delta R.T.: 0.000 min
Response: 59414481
Conc: 40.00 ng/ml

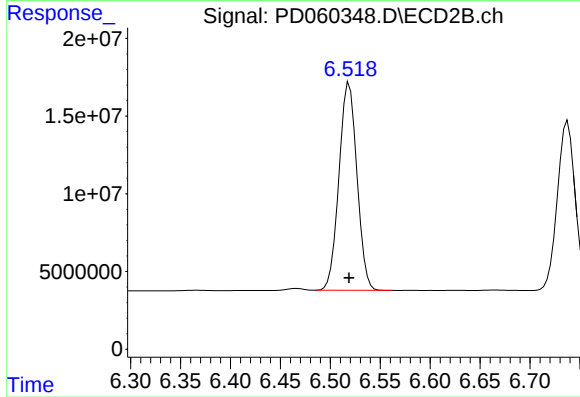

#13 Dieldrin


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 167610744
Conc: 40.00 ng/ml

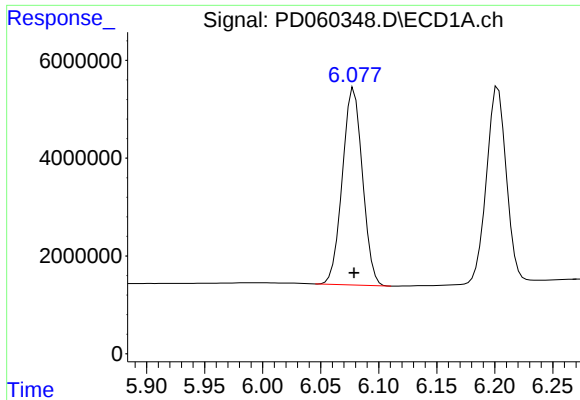

#14 Endrin


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 48509953
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

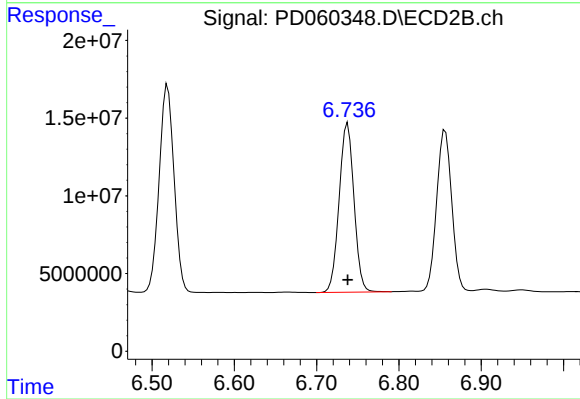


#14 Endrin

R.T.: 6.738 min
Delta R.T.: 0.000 min
Response: 136099681
Conc: 40.00 ng/ml

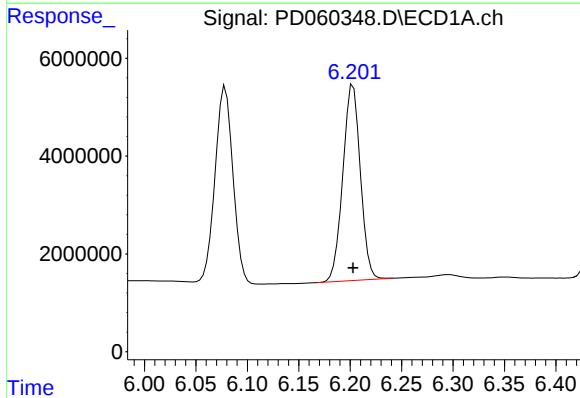


#16 4,4'-DDD

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 47488243
Conc: 40.00 ng/ml

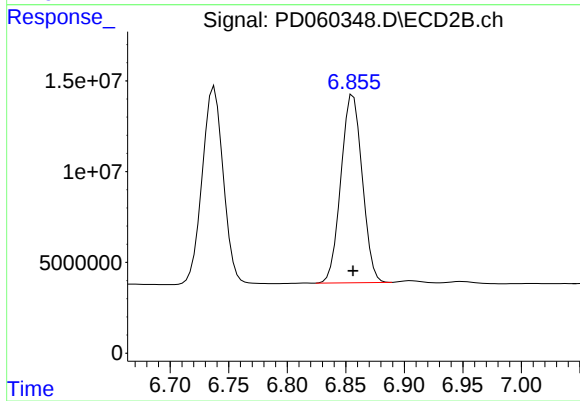

#16 4,4'-DDD


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 131223598
Conc: 40.00 ng/ml

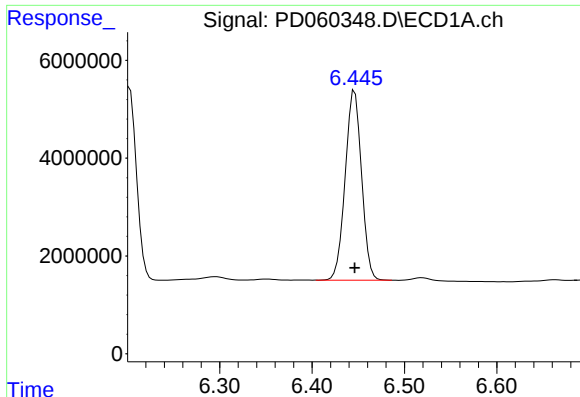

#17 4,4'-DDT


R.T.: 6.446 min
Delta R.T.: 0.000 min
Response: 47716704
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

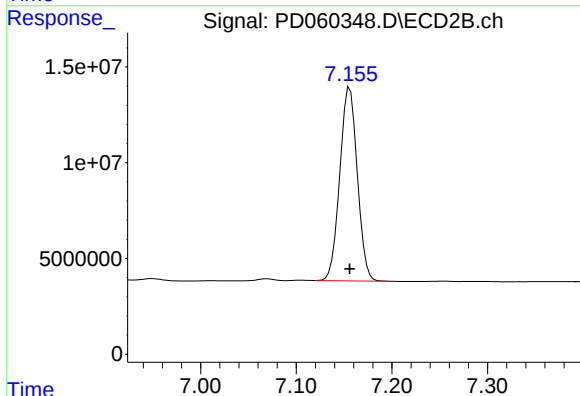


#17 4,4'-DDT

R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 128739539
Conc: 40.00 ng/ml

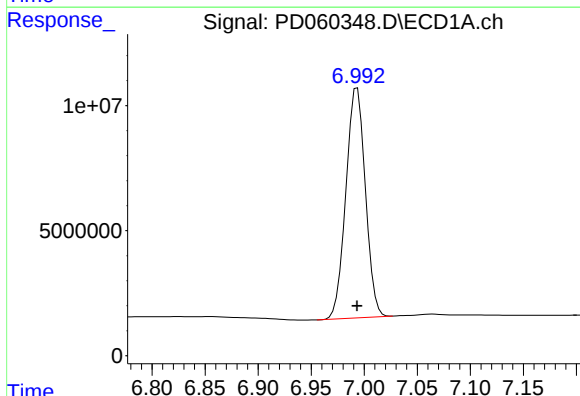


#20 Methoxychlor

R.T.: 6.993 min
Delta R.T.: 0.000 min
Response: 117259076
Conc: 200.00 ng/ml

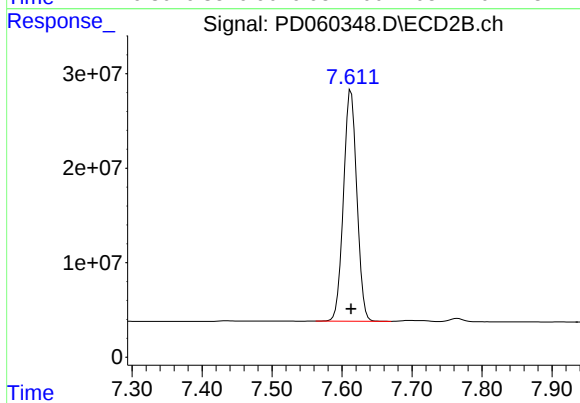

#20 Methoxychlor


R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 324283007
Conc: 200.00 ng/ml

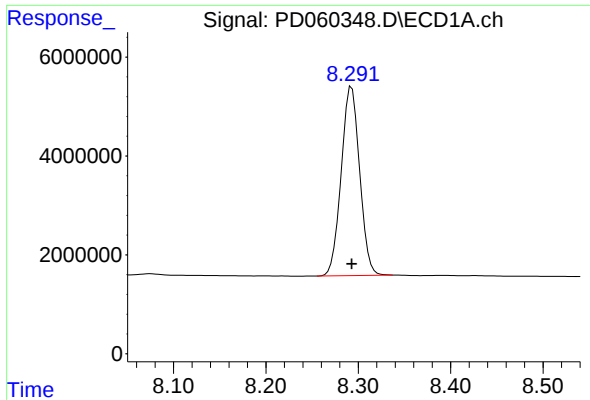

#27 Decachlorobiphenyl

R.T.: 8.293 min
Delta R.T.: 0.000 min
Response: 53037028
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

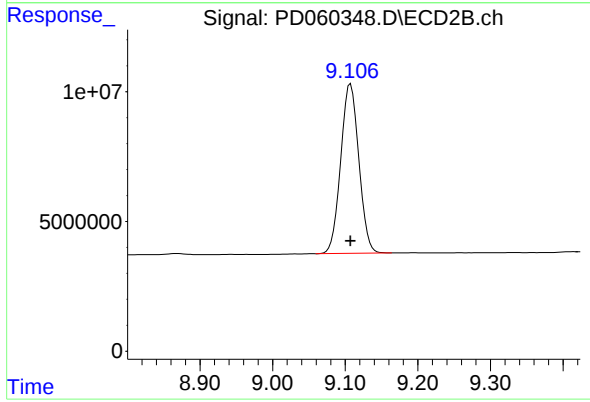

#27 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 113217573
Conc: 40.00 ng/ml