

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
 Data File : PD060350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2020 16:57
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 01:37:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:35:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.023	43450838	144.9E6	38.608	39.376
27)	SA Decachlor...	8.294	9.107	102.9E6	221.8E6	77.636	78.356
Target Compounds							
2)	A alpha-BHC	3.944	4.413	64961441	221.5E6	40.642	41.115
3)	MA gamma-BHC...	4.230	4.699	60962404	198.8E6	40.208	40.447
4)	MA Heptachlor	4.537	5.211	61023364	191.9E6	39.985	40.054
9)	A Endosulfan I	5.575	6.262	53567169	154.1E6	39.755	39.858
13)	MA Dieldrin	5.821	6.519	121.4E6	339.1E6	81.722	80.937
14)	MA Endrin	6.079	6.738	97416188	274.2E6	80.327	80.591
16)	A 4,4'-DDD	6.203	6.856	96000390	266.3E6	80.862	81.185
17)	MA 4,4'-DDT	6.446	7.156	98761790	265.0E6	82.790	82.340
20)	A Methoxychlor	6.994	7.613	233.4E6	632.1E6	398.035	389.843

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
Data File : PD060350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2020 16:57
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 01:37:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:35:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

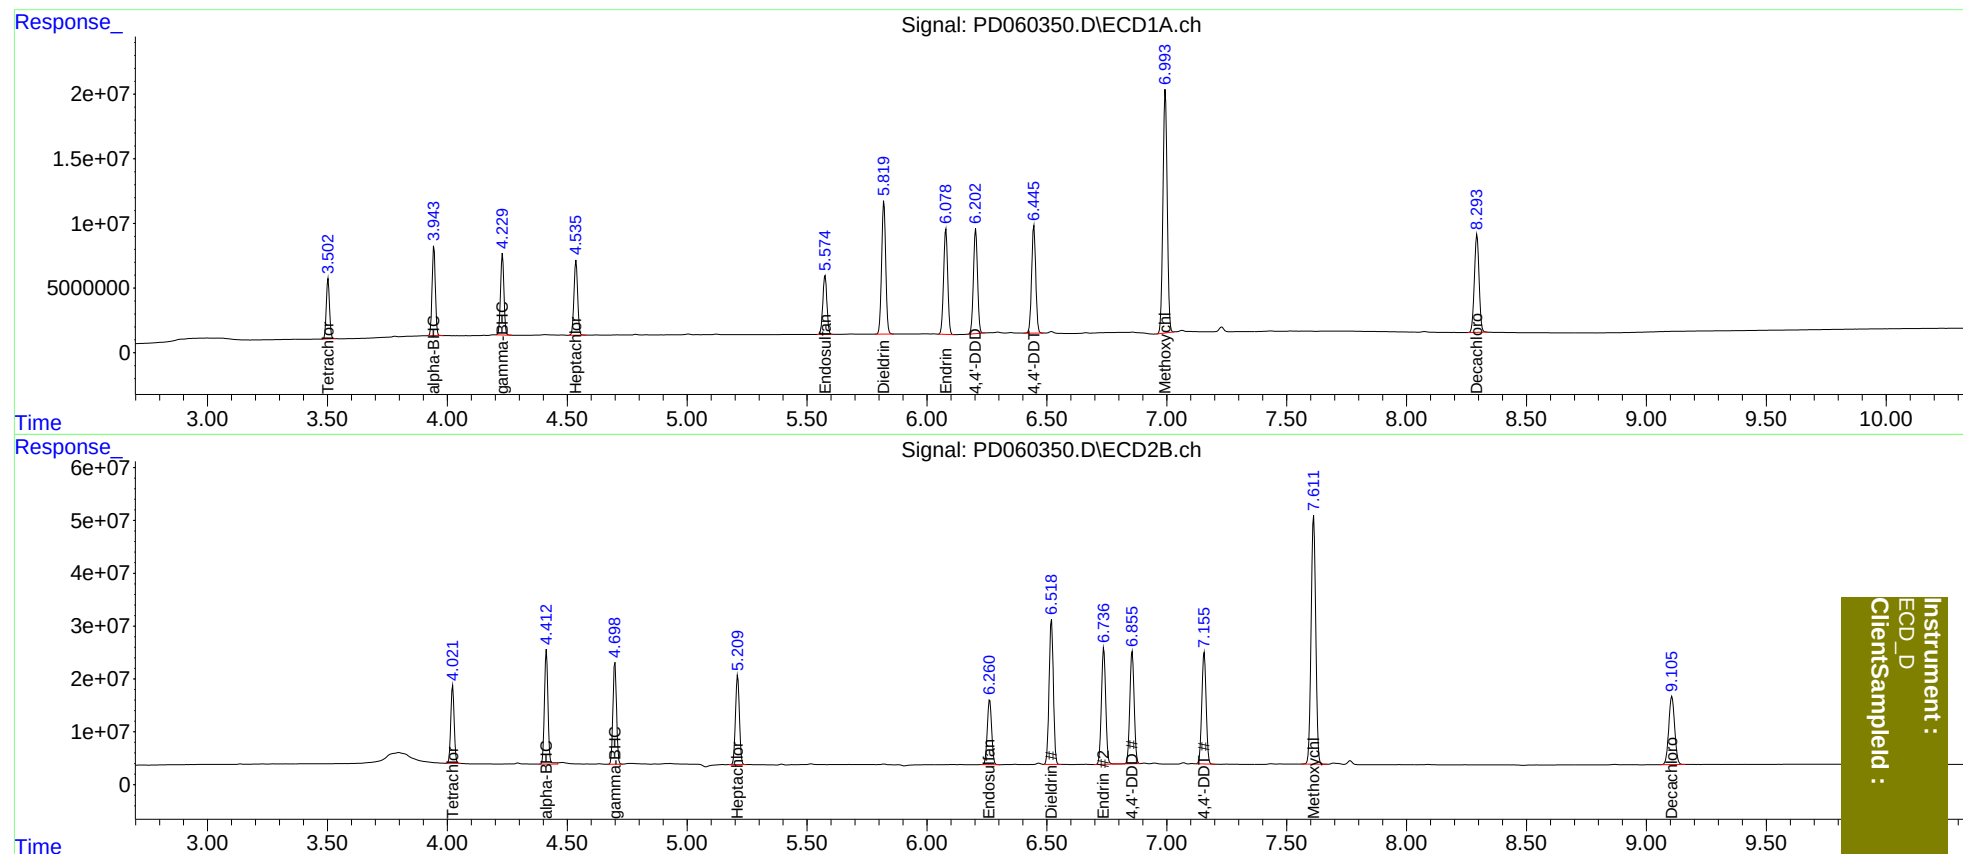


Instrument :
ECD_D
ClientSampled :

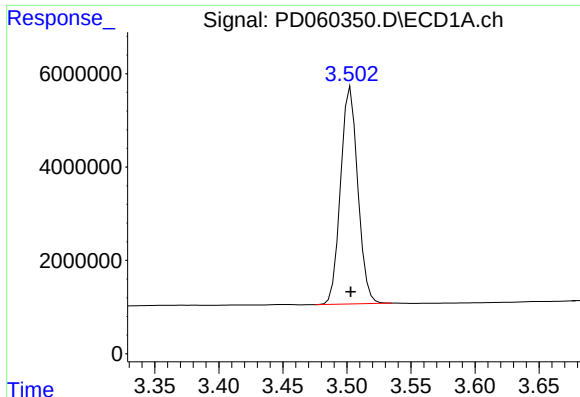

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 43450838
Conc: 38.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

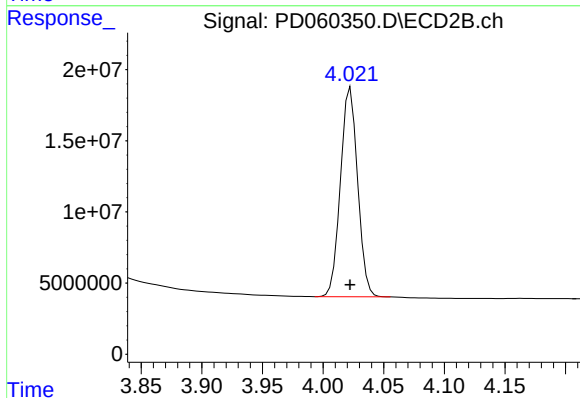


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 144880873
Conc: 39.38 ng/ml

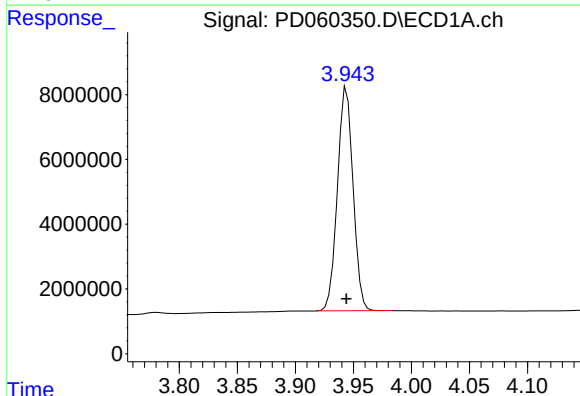


#2 alpha-BHC

R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 64961441
Conc: 40.64 ng/ml

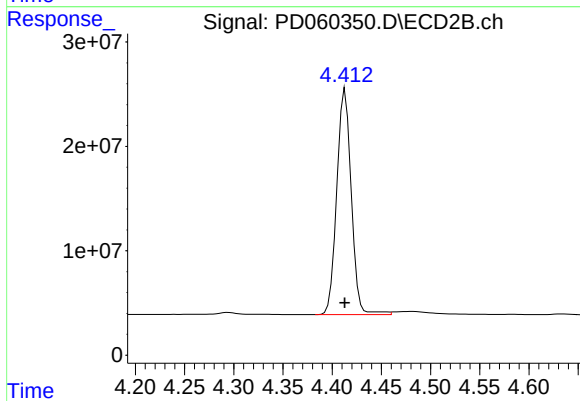

#2 alpha-BHC


R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 221544281
Conc: 41.11 ng/ml

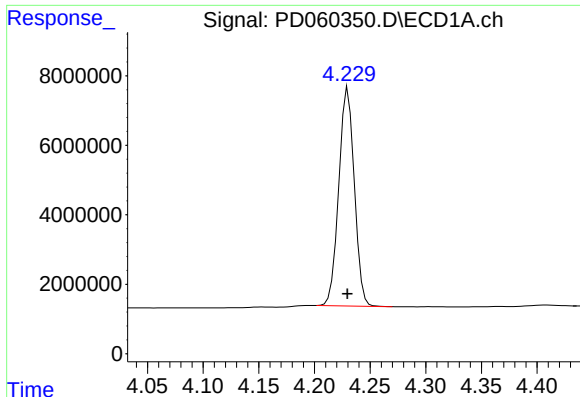

#3 gamma-BHC (Lindane)


R.T.: 4.230 min
Delta R.T.: 0.000 min
Response: 60962404
Conc: 40.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

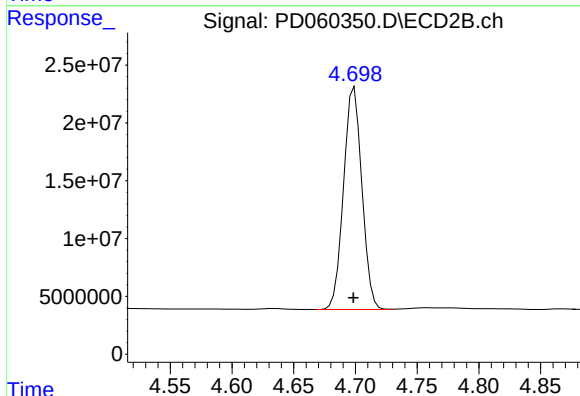


#3 gamma-BHC (Lindane)

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 198765193
Conc: 40.45 ng/ml

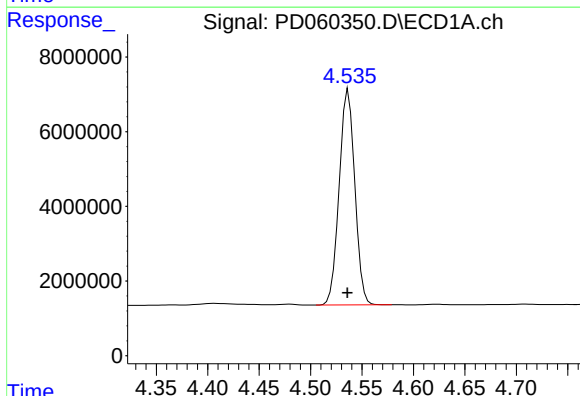


#4 Heptachlor

R.T.: 4.537 min
Delta R.T.: 0.000 min
Response: 61023364
Conc: 39.98 ng/ml

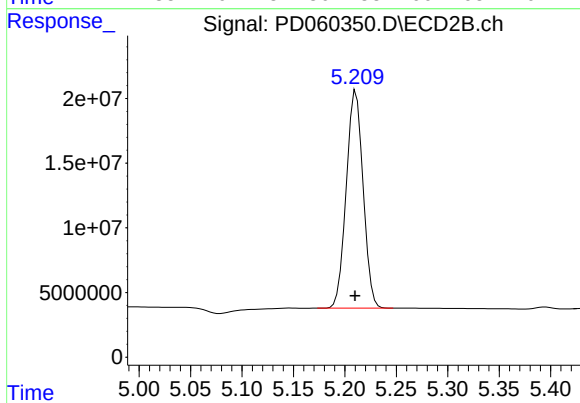

#4 Heptachlor


R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 191890906
Conc: 40.05 ng/ml

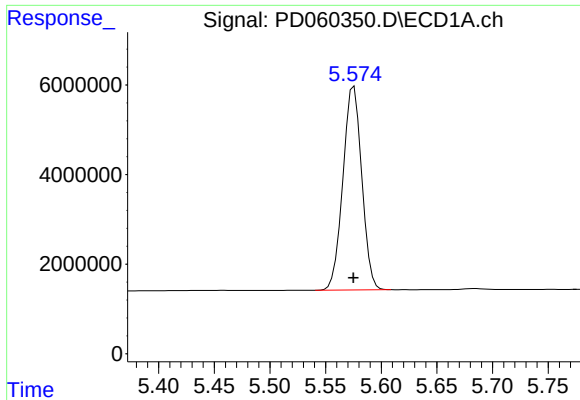

#9 Endosulfan I


R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 53567169
Conc: 39.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

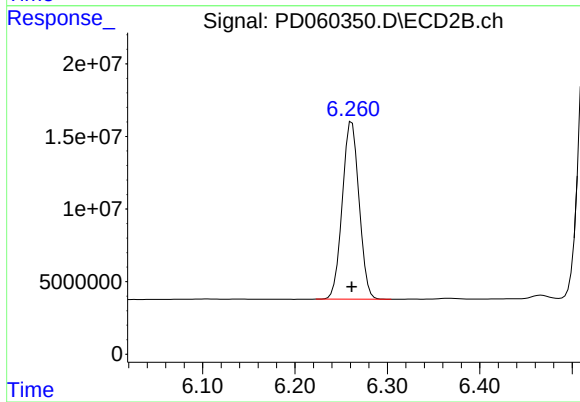


#9 Endosulfan I

R.T.: 6.262 min
Delta R.T.: 0.000 min
Response: 154142890
Conc: 39.86 ng/ml

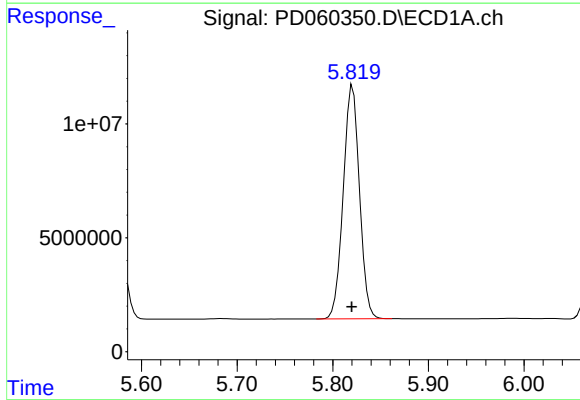


#13 Dieldrin

R.T.: 5.821 min
Delta R.T.: 0.000 min
Response: 121387183
Conc: 81.72 ng/ml

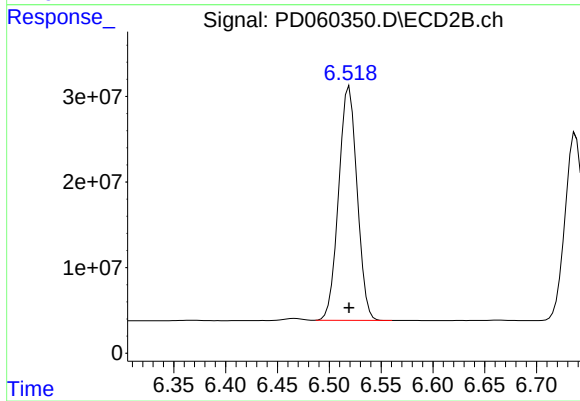

#13 Dieldrin


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 339146515
Conc: 80.94 ng/ml

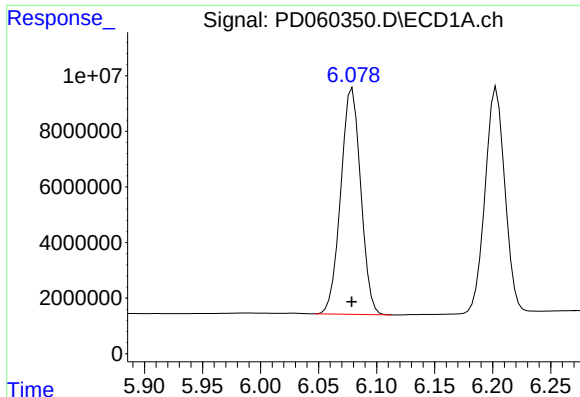

#14 Endrin


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 97416188
Conc: 80.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

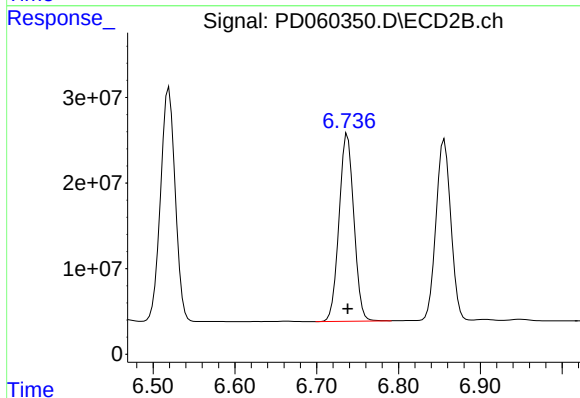


#14 Endrin

R.T.: 6.738 min
Delta R.T.: 0.000 min
Response: 274209003
Conc: 80.59 ng/ml

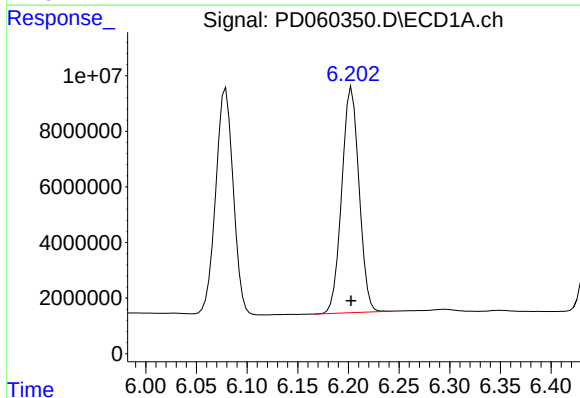


#16 4,4'-DDD

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 96000390
Conc: 80.86 ng/ml

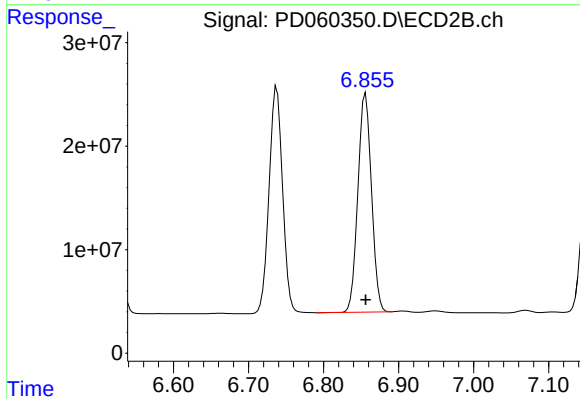

#16 4,4'-DDD


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 266333107
Conc: 81.18 ng/ml

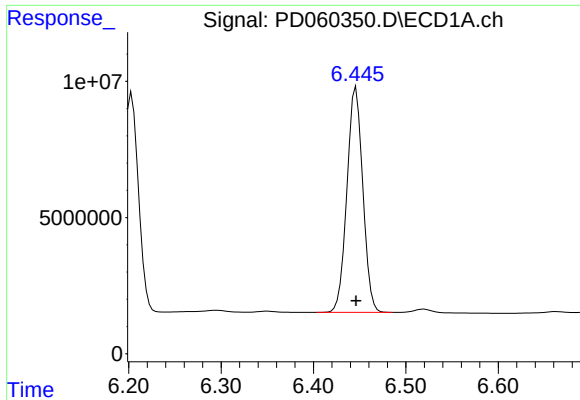

#17 4,4'-DDT


R.T.: 6.446 min
Delta R.T.: 0.000 min
Response: 98761790
Conc: 82.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

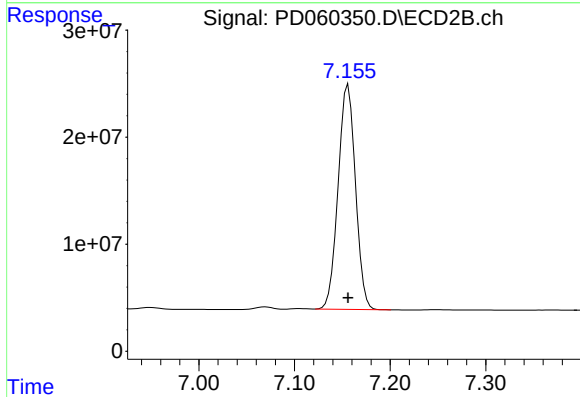


#17 4,4'-DDT

R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 265009084
Conc: 82.34 ng/ml

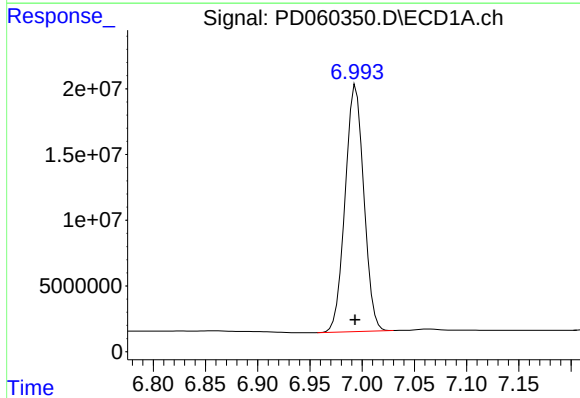


#20 Methoxychlor

R.T.: 6.994 min
Delta R.T.: 0.000 min
Response: 233365947
Conc: 398.03 ng/ml

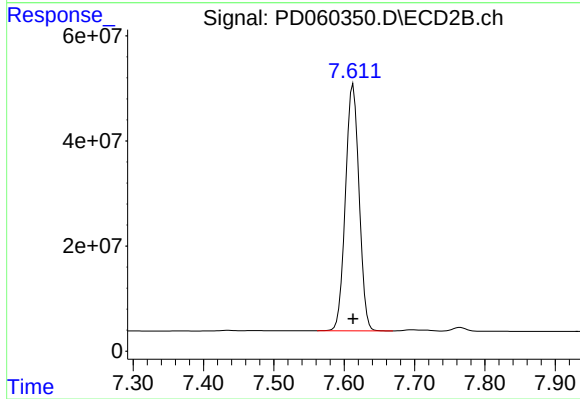

#20 Methoxychlor


R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 632096508
Conc: 389.84 ng/ml

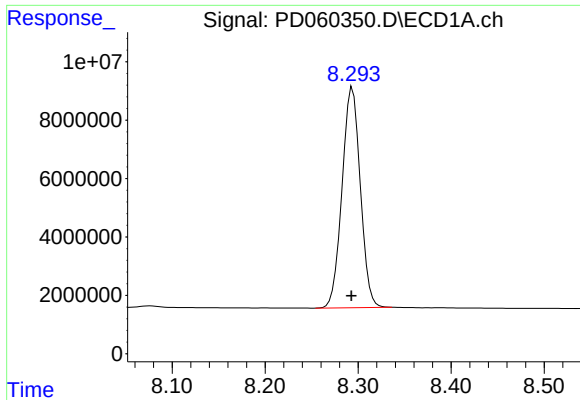

#27 Decachlorobiphenyl

R.T.: 8.294 min
Delta R.T.: 0.001 min
Response: 102939509
Conc: 77.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

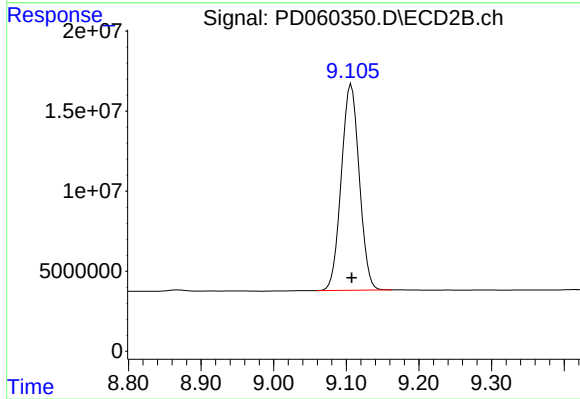

#27 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 221781708
Conc: 78.36 ng/ml