

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
 Data File : PD060352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2020 17:25
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 01:37:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:35:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.023	85362574	285.7E6	75.848	77.661
27)	SA Decachlor...	8.293	9.107	198.8E6	422.3E6	149.933	149.211
Target Compounds							
2)	A alpha-BHC	3.944	4.413	133.3E6	438.5E6	83.398	81.382
3)	MA gamma-BHC...	4.230	4.699	123.2E6	397.7E6	81.285	80.936
4)	MA Heptachlor	4.537	5.210	122.5E6	379.8E6	80.271	79.281
9)	A Endosulfan I	5.575	6.261	106.2E6	302.0E6	78.791	78.084
13)	MA Dieldrin	5.820	6.519	245.8E6	666.1E6	165.449	158.975
14)	MA Endrin	6.079	6.737	193.8E6	538.2E6	159.788	158.177
16)	A 4,4'-DDD	6.203	6.857	193.2E6	524.8E6	162.734	159.976
17)	MA 4,4'-DDT	6.446	7.156	202.1E6	529.0E6	169.452	164.364
20)	A Methoxychlor	6.994	7.614	453.4E6	1180.4E6	773.347	728.025

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
Data File : PD060352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2020 17:25
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 01:37:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:35:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

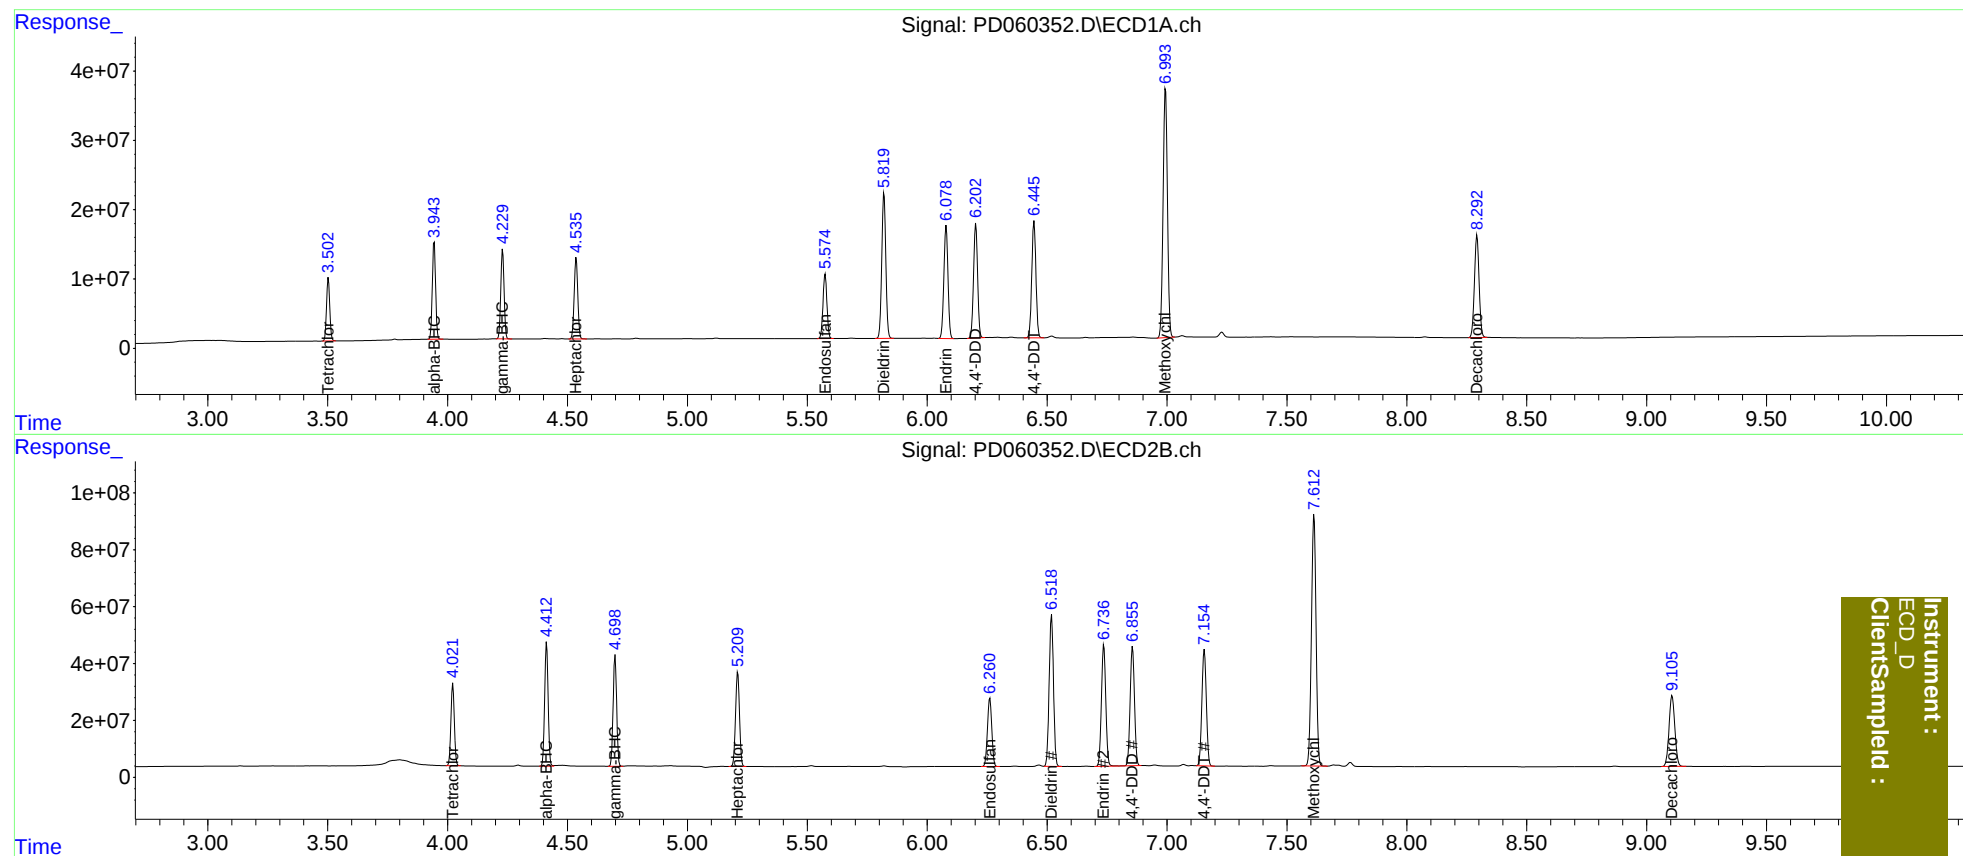


Instrument :
ECD_D
ClientSampled :

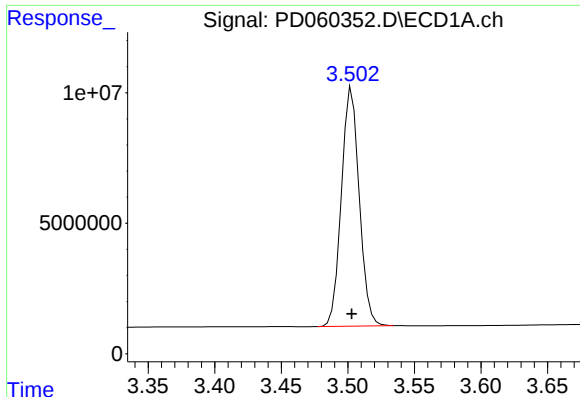

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 85362574
Conc: 75.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

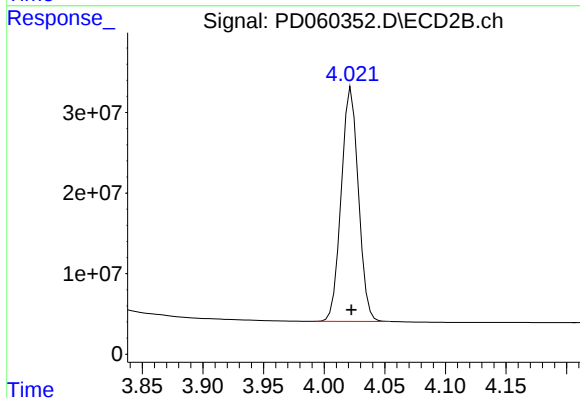


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 285745801
Conc: 77.66 ng/ml

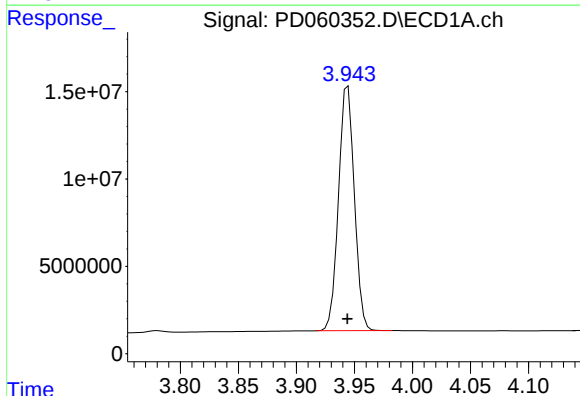


#2 alpha-BHC

R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 133301164
Conc: 83.40 ng/ml

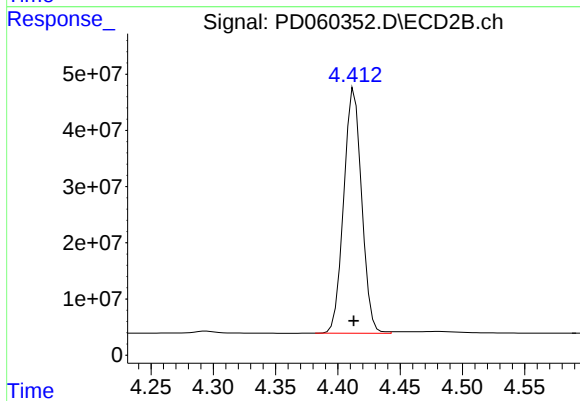

#2 alpha-BHC


R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 438519968
Conc: 81.38 ng/ml

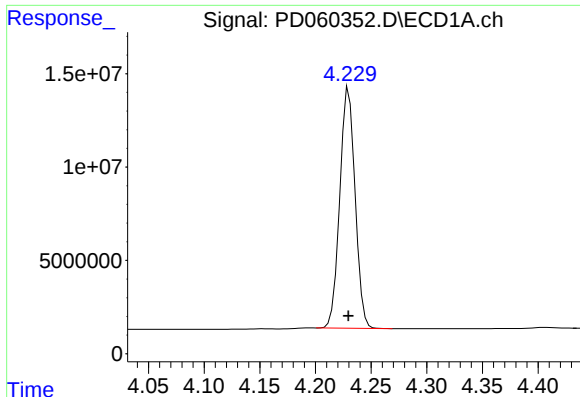

#3 gamma-BHC (Lindane)


R.T.: 4.230 min
Delta R.T.: 0.000 min
Response: 123243886
Conc: 81.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

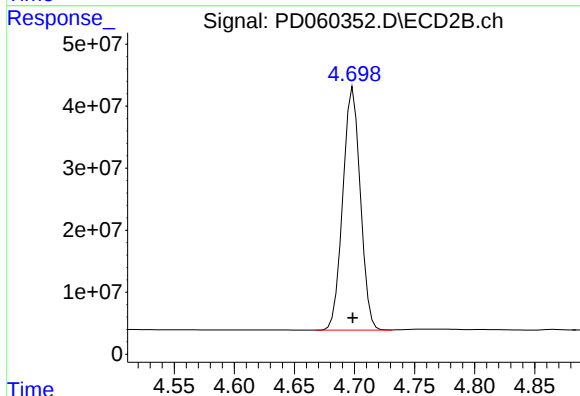


#3 gamma-BHC (Lindane)

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 397737304
Conc: 80.94 ng/ml

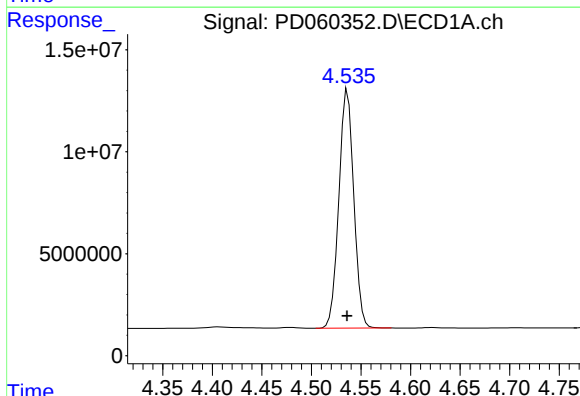


#4 Heptachlor

R.T.: 4.537 min
Delta R.T.: 0.000 min
Response: 122506121
Conc: 80.27 ng/ml

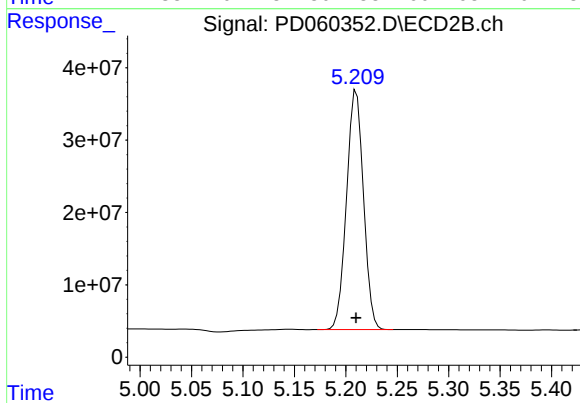

#4 Heptachlor


R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 379824843
Conc: 79.28 ng/ml

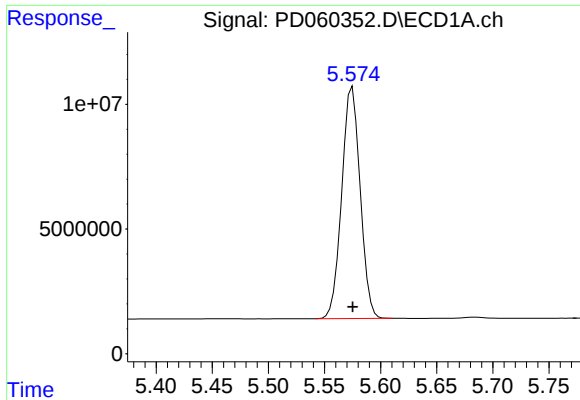

#9 Endosulfan I


R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 106166035
Conc: 78.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

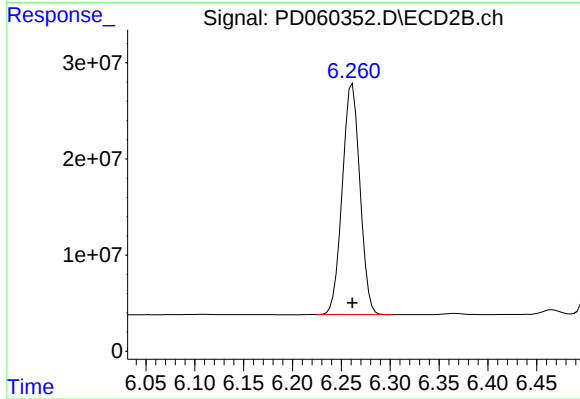


#9 Endosulfan I

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 301974096
Conc: 78.08 ng/ml

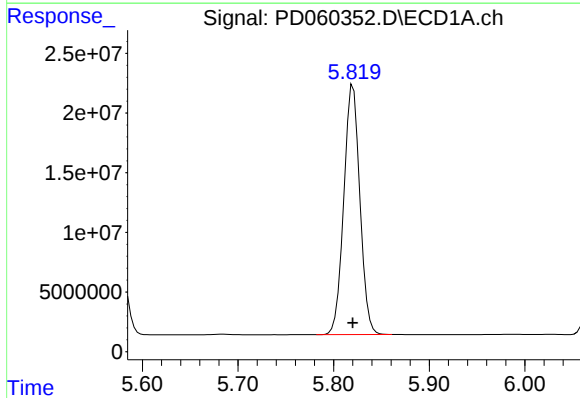


#13 Dieldrin

R.T.: 5.820 min
Delta R.T.: 0.000 min
Response: 245751912
Conc: 165.45 ng/ml

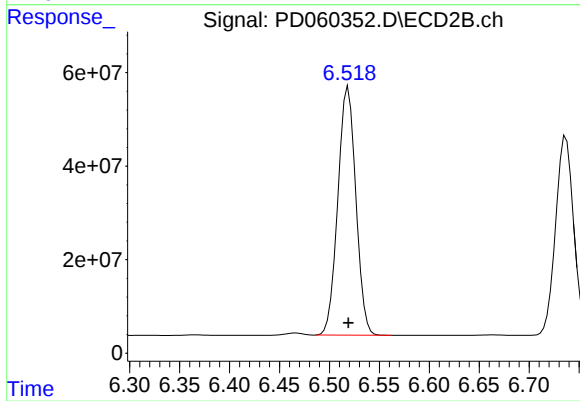

#13 Dieldrin


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 666146243
Conc: 158.97 ng/ml

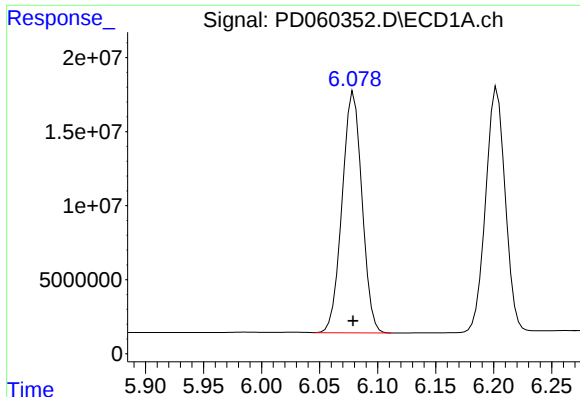

#14 Endrin


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 193782717
Conc: 159.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

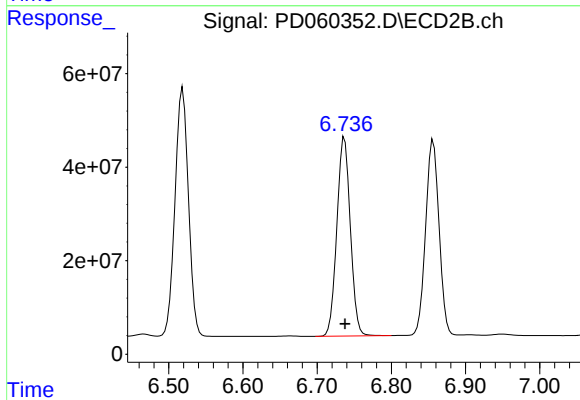


#14 Endrin

R.T.: 6.737 min
Delta R.T.: 0.000 min
Response: 538196163
Conc: 158.18 ng/ml

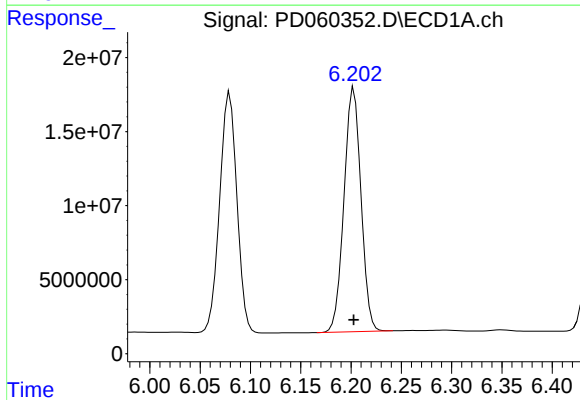


#16 4,4'-DDD

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 193199386
Conc: 162.73 ng/ml

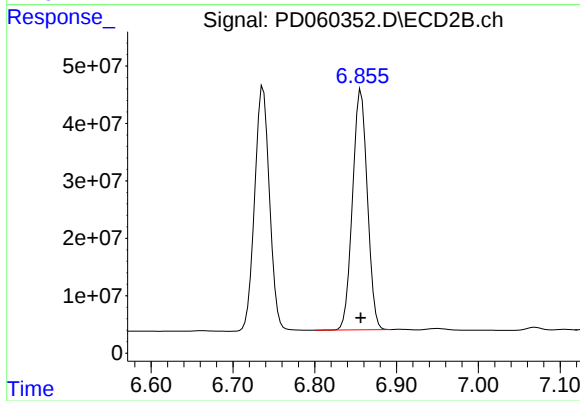

#16 4,4'-DDD


R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 524816413
Conc: 159.98 ng/ml

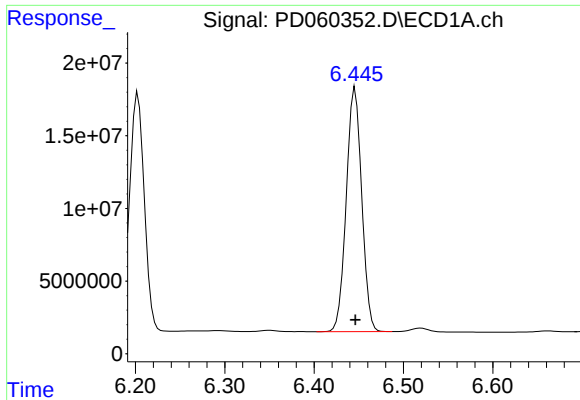

#17 4,4'-DDT


R.T.: 6.446 min
Delta R.T.: 0.000 min
Response: 202142866
Conc: 169.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

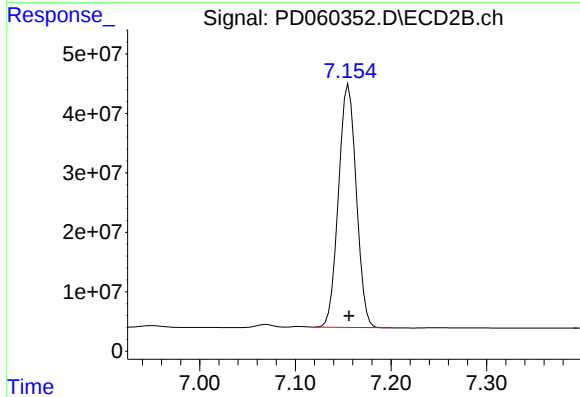


#17 4,4'-DDT

R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 529002740
Conc: 164.36 ng/ml

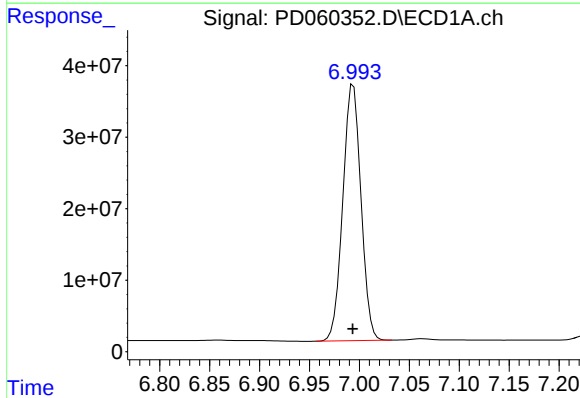


#20 Methoxychlor

R.T.: 6.994 min
Delta R.T.: 0.000 min
Response: 453409489
Conc: 773.35 ng/ml

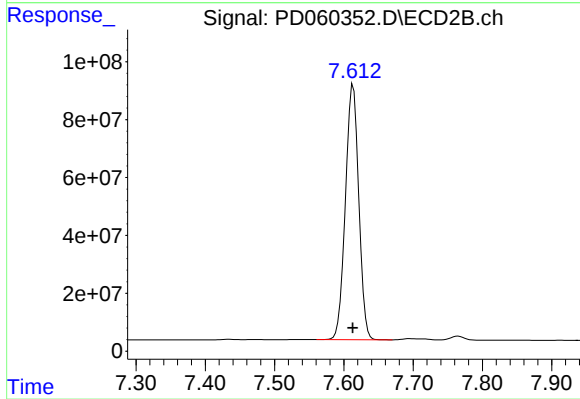

#20 Methoxychlor

R.T.: 7.614 min
Delta R.T.: 0.000 min
Response: 1180430611
Conc: 728.02 ng/ml

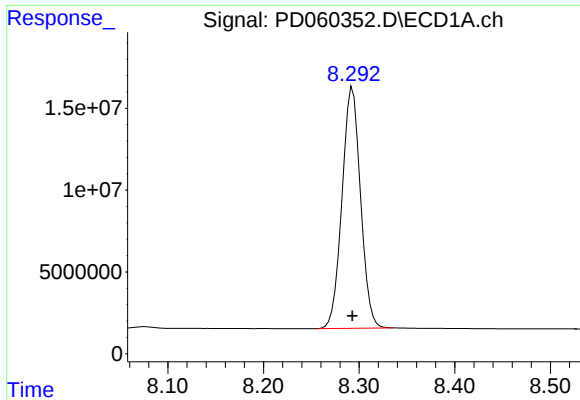

#27 Decachlorobiphenyl


R.T.: 8.293 min

Delta R.T.: 0.000 min

Response: 198800582

Conc: 149.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

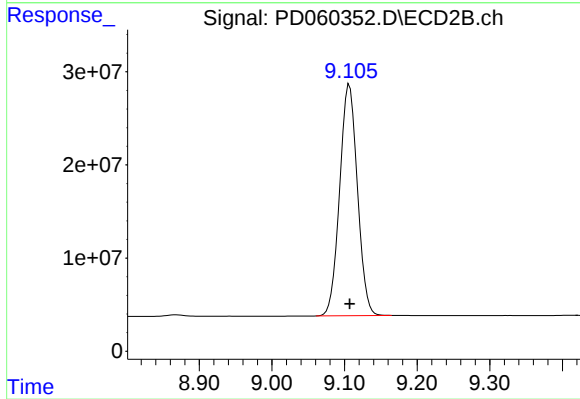

#27 Decachlorobiphenyl

R.T.: 9.107 min

Delta R.T.: 0.000 min

Response: 422332504

Conc: 149.21 ng/ml