

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
 Data File : PD060388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2020 06:23
 Operator : DD\AJ
 Sample : INDA324
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA324

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 06:48:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.022	21589710	71238960	18.959	19.377
27)	SA Decachlor...	8.293	9.106	48663879	103.0E6	35.936	35.523
Target Compounds							
2)	A alpha-BHC	3.944	4.413	30387275	103.9E6	18.528	19.053
3)	MA gamma-BHC...	4.230	4.698	28820113	94720664	18.509	19.133
4)	MA Heptachlor	4.536	5.210	28729856	89969127	18.402	18.570
9)	A Endosulfan I	5.575	6.261	25859366	73304389	18.779	18.740
13)	MA Dieldrin	5.821	6.518	56898796	157.5E6	37.383	37.132
14)	MA Endrin	6.080	6.737	44698215	114.0E6	35.909	32.859
16)	A 4,4'-DDD	6.203	6.856	50680754	137.5E6	41.663	41.496
17)	MA 4,4'-DDT	6.447	7.156	35241687	91565906	28.851	27.891
20)	A Methoxychlor	6.994	7.613	99129126	250.7E6	165.947	152.962

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
Data File : PD060388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2020 06:23
Operator : DD\AJ
Sample : INDA324
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 06:48:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

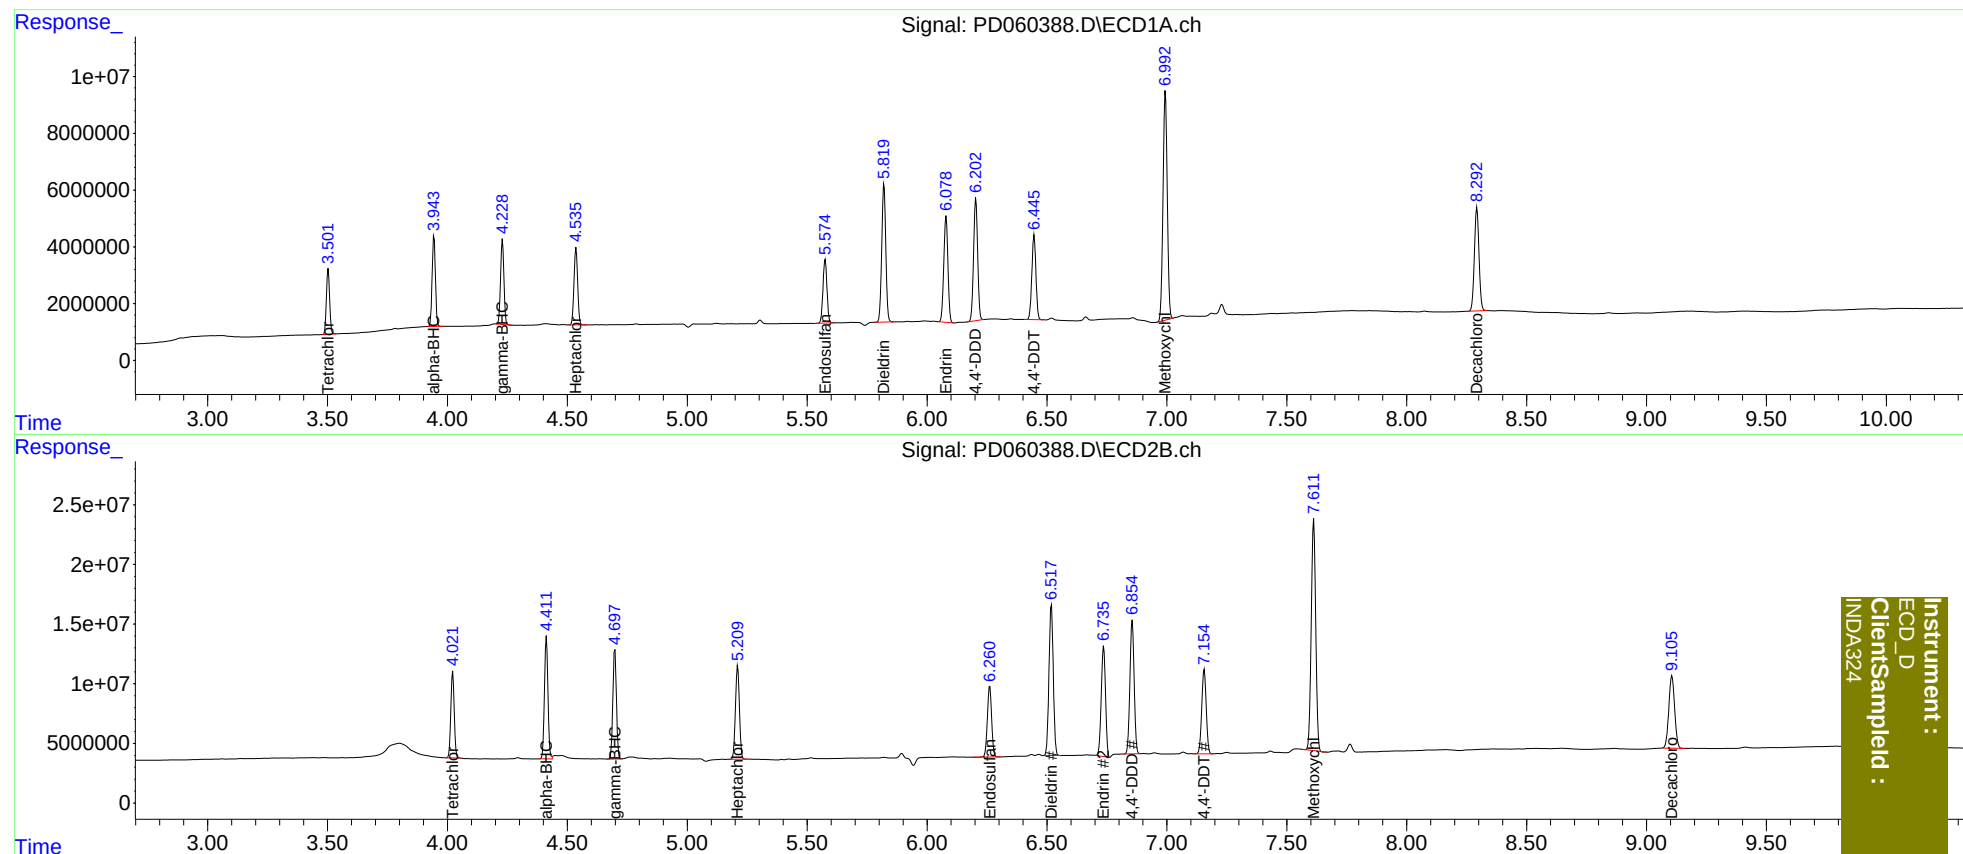

Instrument :
ECD_D
ClientSample :
INDA324