

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
 Data File : PD060337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2020 13:55
 Operator : DD\AJ
 Sample : RESC09
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC09

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 03:09:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.023	20919386	69236883	18.371	18.833
27)	SA Decachlor...	8.293	9.107	49196656	108.7E6	36.329	37.514
Target Compounds							
2)	A alpha-BHC	3.945	4.414	14598082	48582806	8.901	8.911
3)	MA gamma-BHC...	4.230	4.699	13782755	44586815	8.852	9.006
4)	MA Heptachlor	4.537	5.211	14156340	43033765	9.067	8.882
5)	MB Aldrin	4.787	5.518	15118836	44044238	9.897	9.849
6)	B beta-BHC	4.480	4.868	7305054	23637884	10.404	10.857
7)	B delta-BHC	4.688	5.087	14730106	32789527	9.760	8.477
8)	B Heptachlo...	5.233	5.904	14175847	33773086	9.938	9.037
9)	A Endosulfan I	5.575	6.262	12528313	35477748	9.098	9.070
10)	B trans-Chl...	5.462	6.138	14784344	41418973	9.865	9.780
11)	B cis-Chlor...	5.521	6.212	14569423	40859888	9.883	9.911
12)	B 4,4'-DDE	5.685	6.366	27552339	77451574	19.279	19.494
13)	MA Dieldrin	5.821	6.519	26658114	75236241	17.515	17.737
14)	MA Endrin	6.080	6.738	22805049	64175907	18.321	18.499
15)	B Endosulfa...	6.353	6.946	22854482	62510168	19.229	19.565
16)	A 4,4'-DDD	6.204	6.856	21206660	58751593	17.433	17.734
17)	MA 4,4'-DDT	6.447	7.157	21150239	59119172	17.315	18.008
18)	B Endrin al...	6.522	7.070	19792492	54329051	19.798	20.117
19)	B Endosulfa...	6.736	7.293	22126767	63241234	19.532	20.095
20)	A Methoxychlor	6.995	7.613	54227957	157.0E6	90.780	95.755
21)	B Endrin ke...	7.231	7.765	26894819	68472688	19.905	20.338

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
Data File : PD060337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2020 13:55
Operator : DD\AJ
Sample : RESC09
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 03:09:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

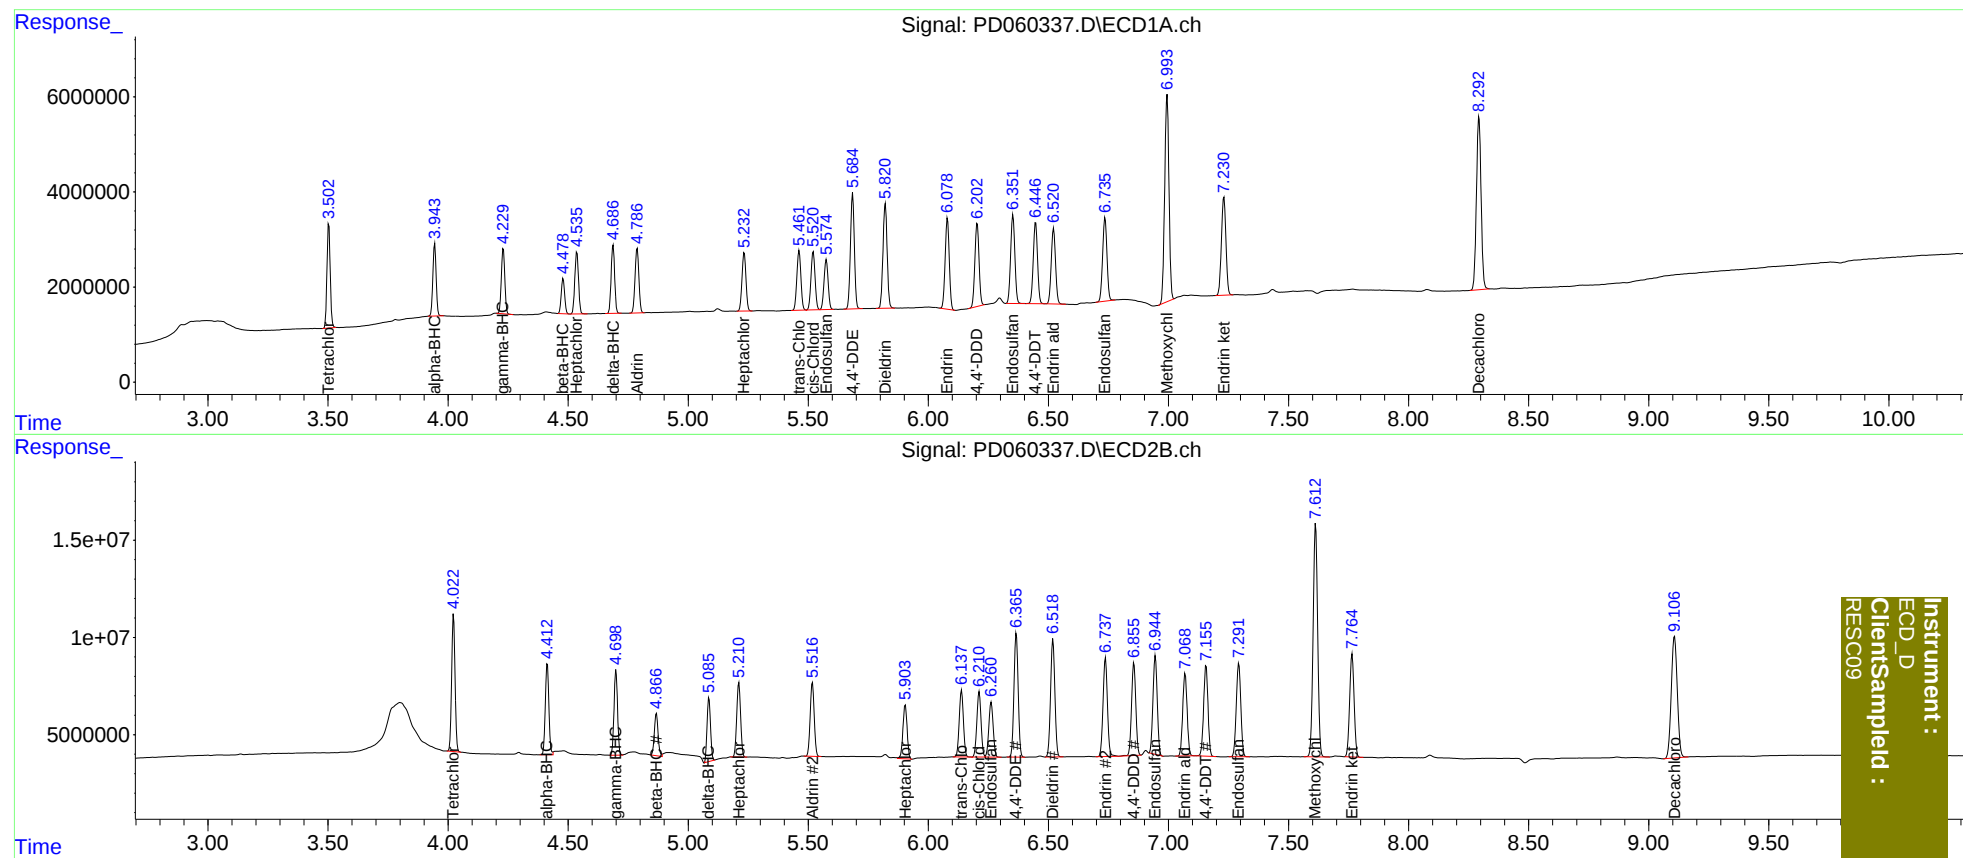

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
Data File : PD060337.D
Acq On : 27 Nov 2020 13:55
Operator : DD\AJ
Sample : RESC09
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC09

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Title : GC Extractables
Last Update : Sat Nov 28 01:50:00 2020
Integrator: ChemStation

RT#1	RT#2	Resolution
3.503	3.945	100.00%
3.945	4.230	100.00%
4.230	4.480	100.00%
4.480	4.537	100.00%
4.537	4.688	100.00%
4.688	4.787	100.00%
4.787	5.233	100.00%
5.233	5.462	100.00%
5.462	5.521	100.00%
5.521	5.575	100.00%
5.575	5.685	100.00%
5.685	5.821	100.00%
5.821	6.080	100.00%
6.080	6.204	100.00%
6.204	6.353	100.00%
6.353	6.447	100.00%
6.447	6.522	100.00%
6.522	6.736	100.00%
6.736	6.995	100.00%
6.995	7.231	100.00%
7.231	8.293	100.00%

Signal #2


4.023	4.414	100.00%
4.414	4.700	100.00%
4.700	4.868	100.00%
4.868	5.087	100.00%
5.087	5.211	100.00%
5.211	5.518	100.00%
5.518	5.904	100.00%
5.904	6.138	100.00%
6.138	6.212	100.00%
6.212	6.262	98.85%
6.262	6.366	100.00%
6.366	6.519	100.00%
6.519	6.738	100.00%
6.738	6.856	100.00%
6.856	6.946	100.00%
6.946	7.070	100.00%
7.070	7.157	100.00%
7.157	7.293	100.00%
7.293	7.613	100.00%
7.613	7.765	100.00%
7.765	9.107	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112720\
Data File : PD060337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2020 13:55
Operator : DD\AJ
Sample : RESC09
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC09

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 03:09:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

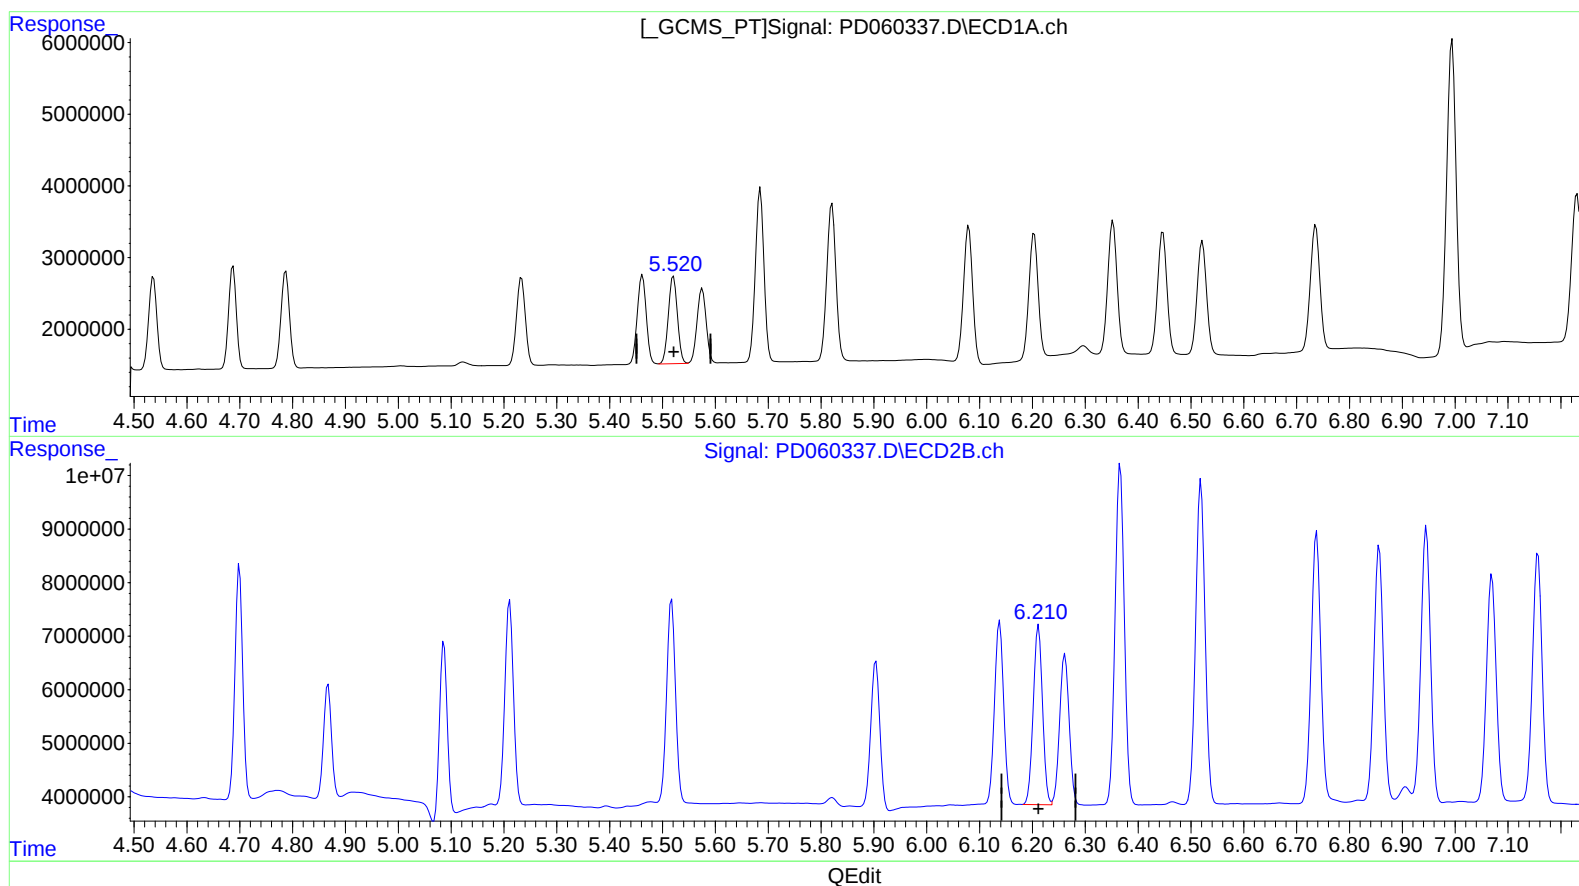

(11) cis-Chlordane (B)

5.521min 9.883 ng/ml

response 14569423

(11) cis-Chlordane #2 (B)

6.212min 9.911 ng/ml

response 40859888