

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112723\
 Data File : PD079841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2023 13:07
 Operator : AR\AJ
 Sample : 05473-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 20:14:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.802	34254933	52183771	23.456	22.815
27)	SA Decachlor...	9.118	7.947	24132321	31088962	13.599	13.022
Target Compounds							
2)	A alpha-BHC	0.000	3.327	0	313930	N.D.	<MDL
4)	MA Heptachlor	4.937	0.000	1880130	0	0.751	N.D. #
5)	MB Aldrin	0.000	4.279	0	5894378	N.D.	1.812
6)	B beta-BHC	0.000	3.892f	0	5523629	N.D.	3.373
7)	B delta-BHC	4.794	0.000	31121304	0	12.489	N.D. #
11)	B cis-Chlor...	0.000	5.092	0	532303	N.D.	0.175
14)	MA Endrin	0.000	5.685	0	263053	N.D.	<MDL
15)	B Endosulfa...	0.000	5.896f	0	101498	N.D.	<MDL
20)	A Methoxychlor	0.000	6.645	0	232113	N.D.	0.181
22)	Toxaphene-1	0.000	5.092f	0	532303	N.D.	31.835
24)	Toxaphene-3	0.000	6.645	0	232113	N.D.	4.031


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112723\
Data File : PD079841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2023 13:07
Operator : AR\AJ
Sample : 05473-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 20:14:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

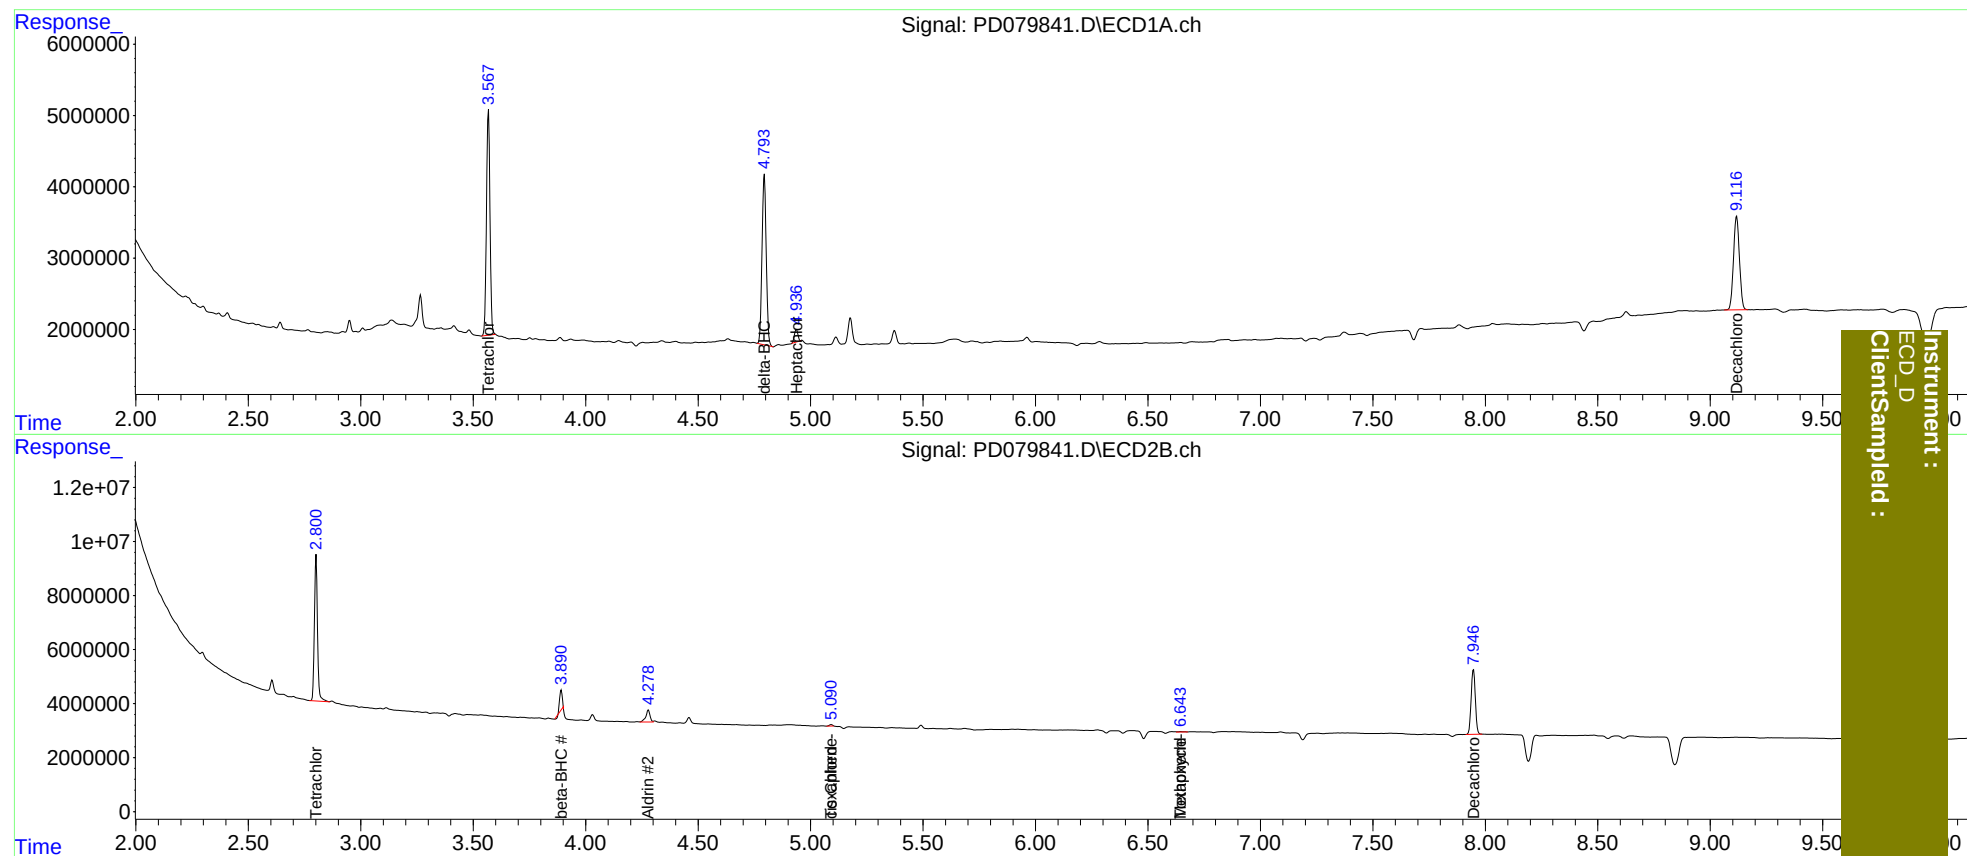


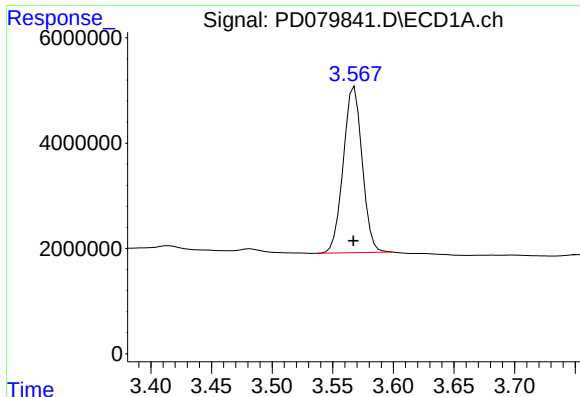

#1 Tetrachloro-m-xylene


R.T.: 3.568 min
Delta R.T.: 0.000 min
Response: 34254933
Conc: 23.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

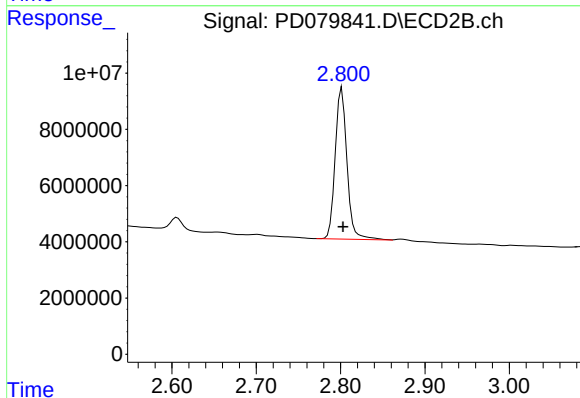


#1 Tetrachloro-m-xylene

R.T.: 2.802 min
Delta R.T.: -0.001 min
Response: 52183771
Conc: 22.81 ng/ml

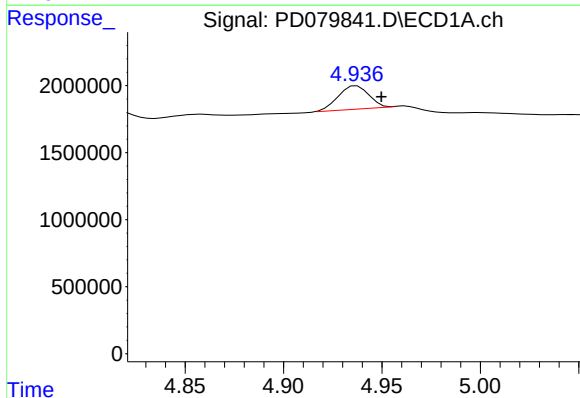


#4 Heptachlor

R.T.: 4.937 min
Delta R.T.: -0.013 min
Response: 1880130
Conc: 0.75 ng/ml

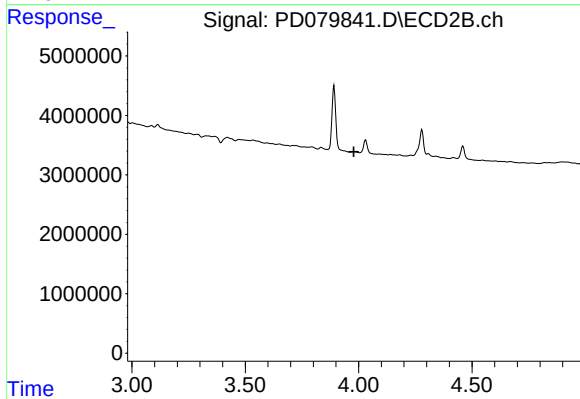

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.978 min
Response: 0
Conc: N.D.

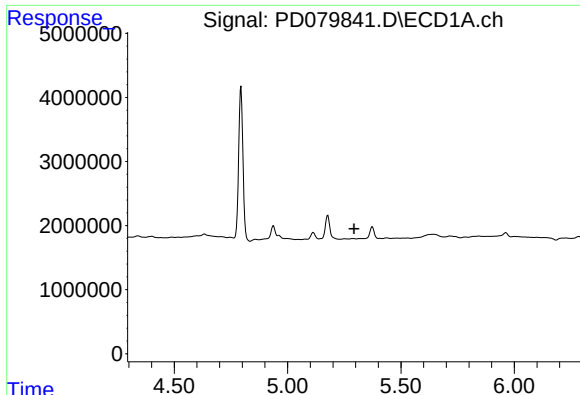

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

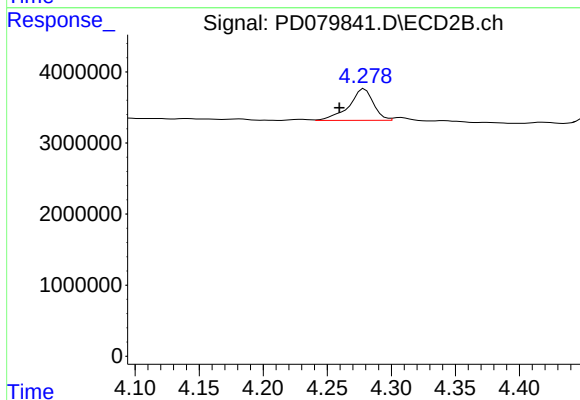


#5 Aldrin

R.T.: 4.279 min
Delta R.T.: 0.020 min
Response: 5894378
Conc: 1.81 ng/ml

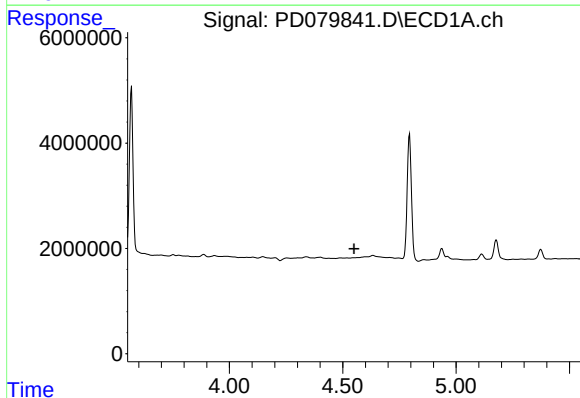


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.551 min
Response: 0
Conc: N.D.

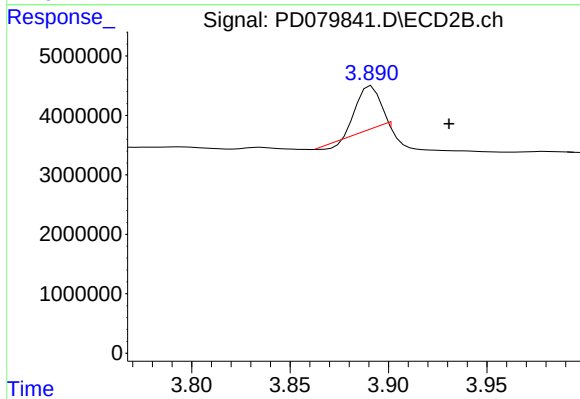

#6 beta-BHC


R.T.: 3.892 min
Delta R.T.: -0.039 min
Response: 5523629
Conc: 3.37 ng/ml

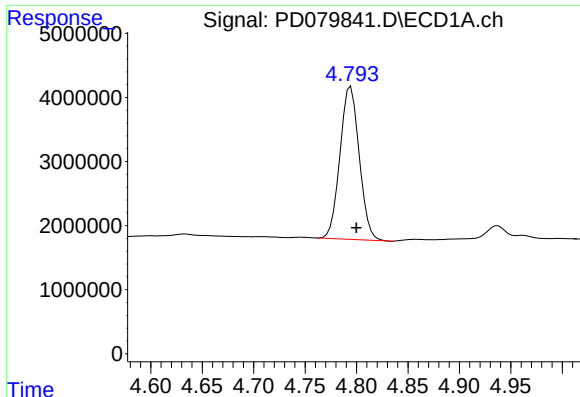

#7 delta-BHC


R.T.: 4.794 min
Delta R.T.: -0.005 min
Response: 31121304
Conc: 12.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

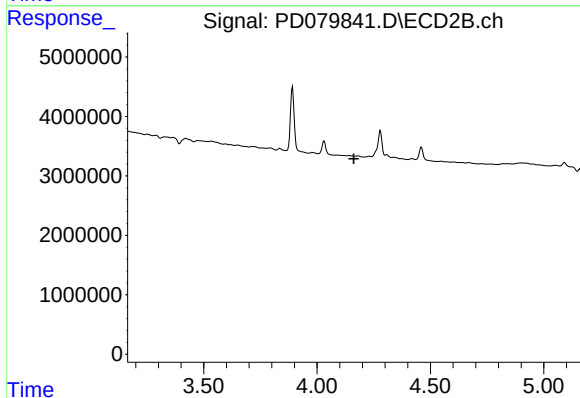


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.162 min
Response: 0
Conc: N.D.

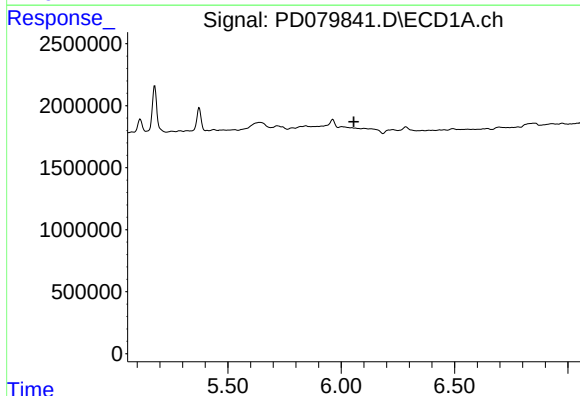


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

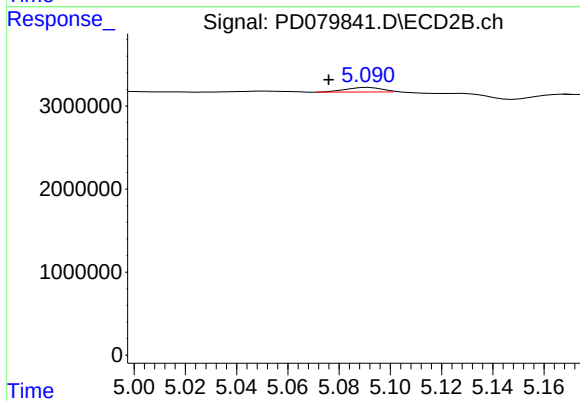

#11 cis-Chlordane


R.T.: 5.092 min
Delta R.T.: 0.016 min
Response: 532303
Conc: 0.18 ng/ml

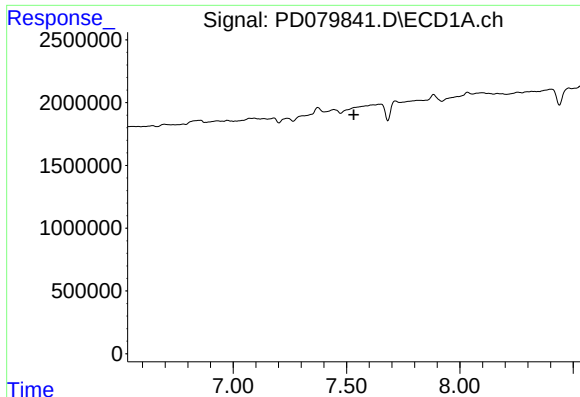

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

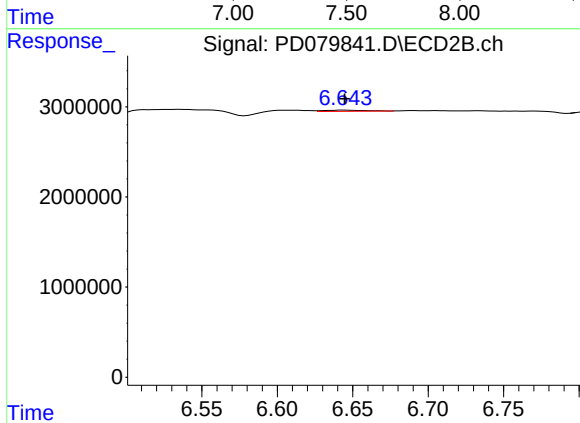


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 232113
Conc: 0.18 ng/ml

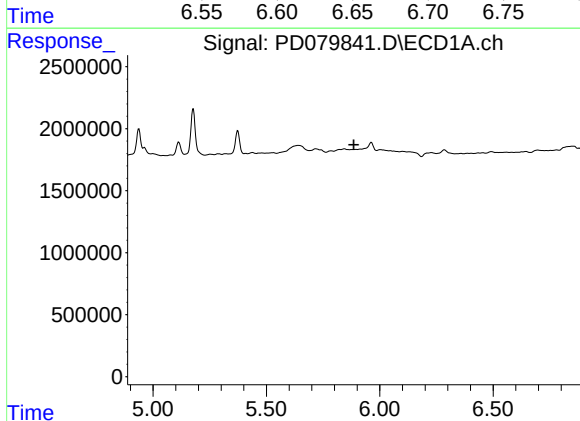


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 5.886 min
Response: 0
Conc: N.D.

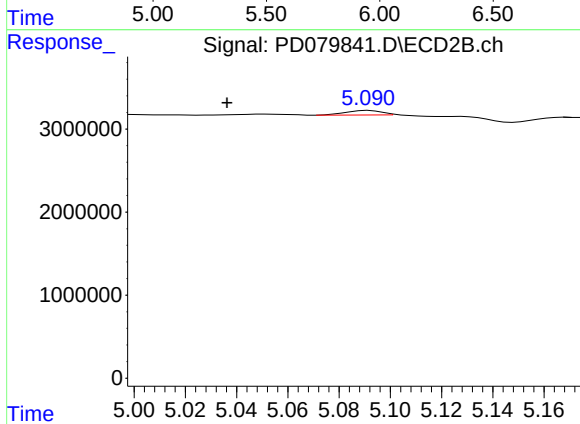

#22 Toxaphene-1


R.T.: 5.092 min
Delta R.T.: 0.055 min
Response: 532303
Conc: 31.83 ng/ml

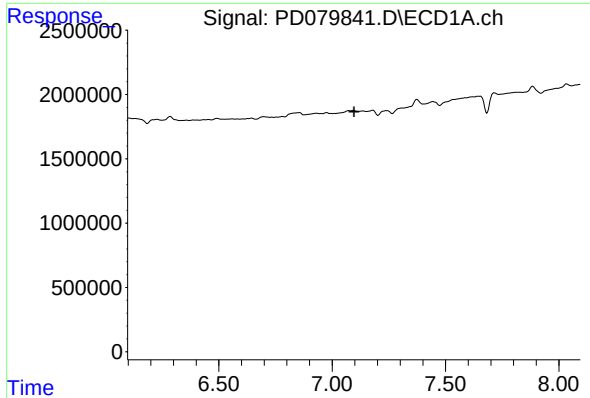

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 7.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

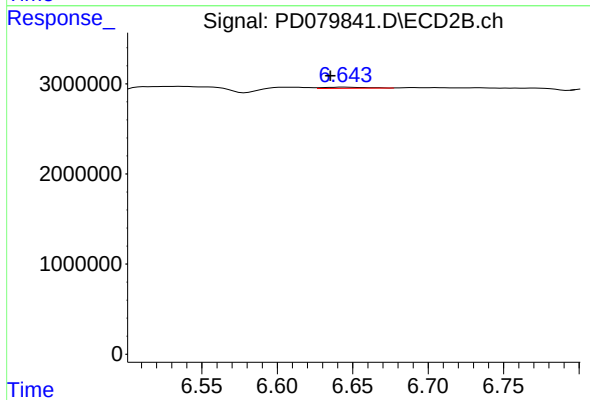


#24 Toxaphene-3

R.T.: 6.645 min
Delta R.T.: 0.010 min
Response: 232113
Conc: 4.03 ng/ml

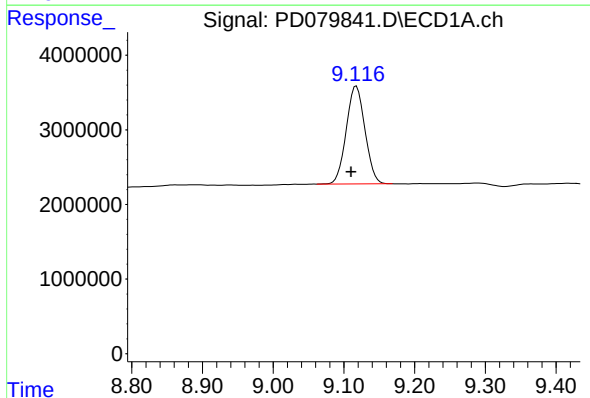

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.007 min
Response: 24132321
Conc: 13.60 ng/ml

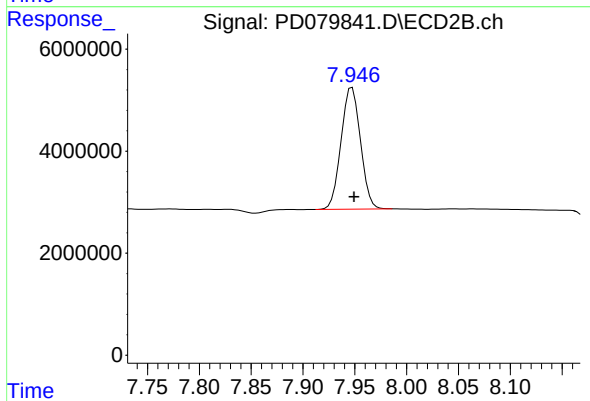

#27 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: -0.002 min
Response: 31088962
Conc: 13.02 ng/ml