

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112723\
 Data File : PD079840.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2023 12:54
 Operator : AR\AJ
 Sample : 05473-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AE7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :Ankita Jodhani 11/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 20:13:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.801	29070857	48112843	19.906	21.035
2)	SA Decachlor...	9.120	7.948	33695151	43330134	18.988	18.149
Target Compounds							
9)	A Endosulfan I	6.118	5.140	1405123	4166106	0.680m	1.503m#
10)	B trans-Chl...	5.957	5.039	3837673	4483044	1.804	1.510m
16)	A 4,4'-DDD	6.737	5.815	1998841	6674522	1.234	2.835 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112723\
Data File : PD079840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2023 12:54
Operator : AR\AJ
Sample : 05473-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 20:13:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

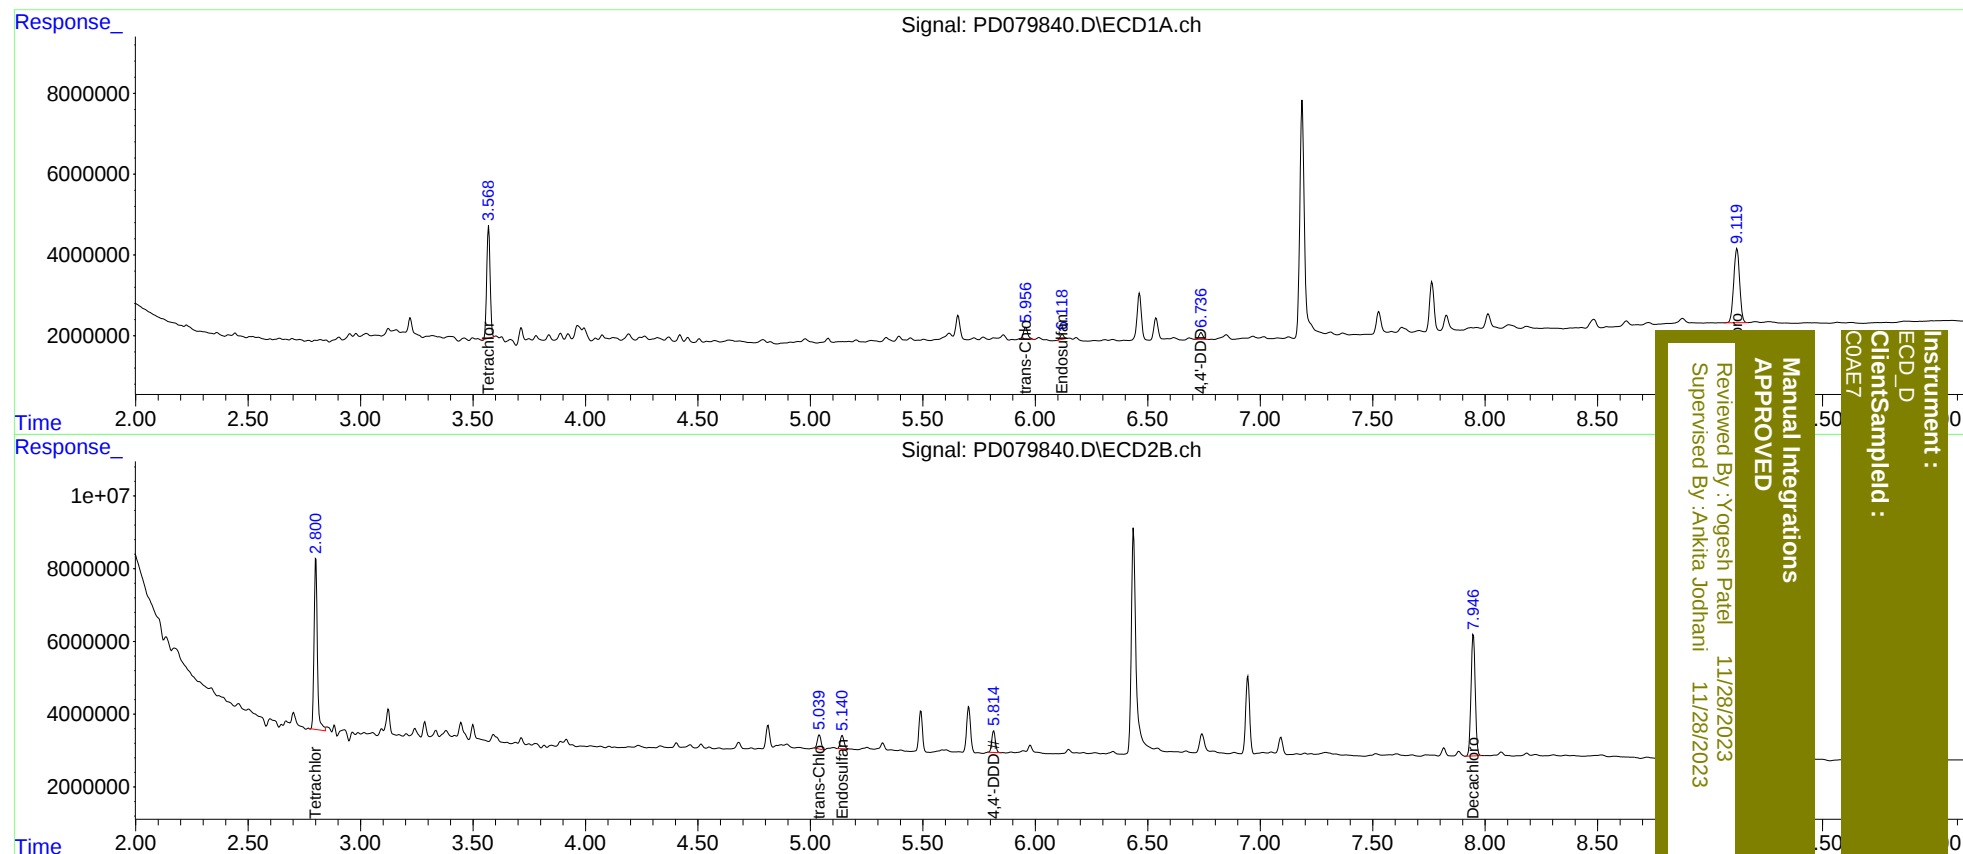

Instrument :
ECD_D
ClientSampled :
COA E7

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/28/2023
Supervised By : Ankita Jodhani 11/28/2023