

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
 Data File : PD086953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2024 12:52
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 13:24:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 13:19:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.883	151.0E6	1007.0E6	75.525	75.265
28)	SA Decachlor...	9.089	8.087	229.6E6	992.7E6	75.168	74.950
Target Compounds							
23)	Chlordane-1	4.724	3.912	99887109	383.6E6	755.135	750.716
24)	Chlordane-2	5.250	4.495	106.2E6	400.8E6	752.662	749.217
25)	Chlordane-3	5.956	5.134	438.3E6	1221.5E6	757.810	754.691
26)	Chlordane-4	6.042	5.199	522.6E6	1019.3E6	756.741	747.797
27)	Chlordane-5	6.881	6.100	90210217	467.5E6	754.732	748.550



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
Data File : PD086953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2024 12:52
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 13:24:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 13:19:46 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

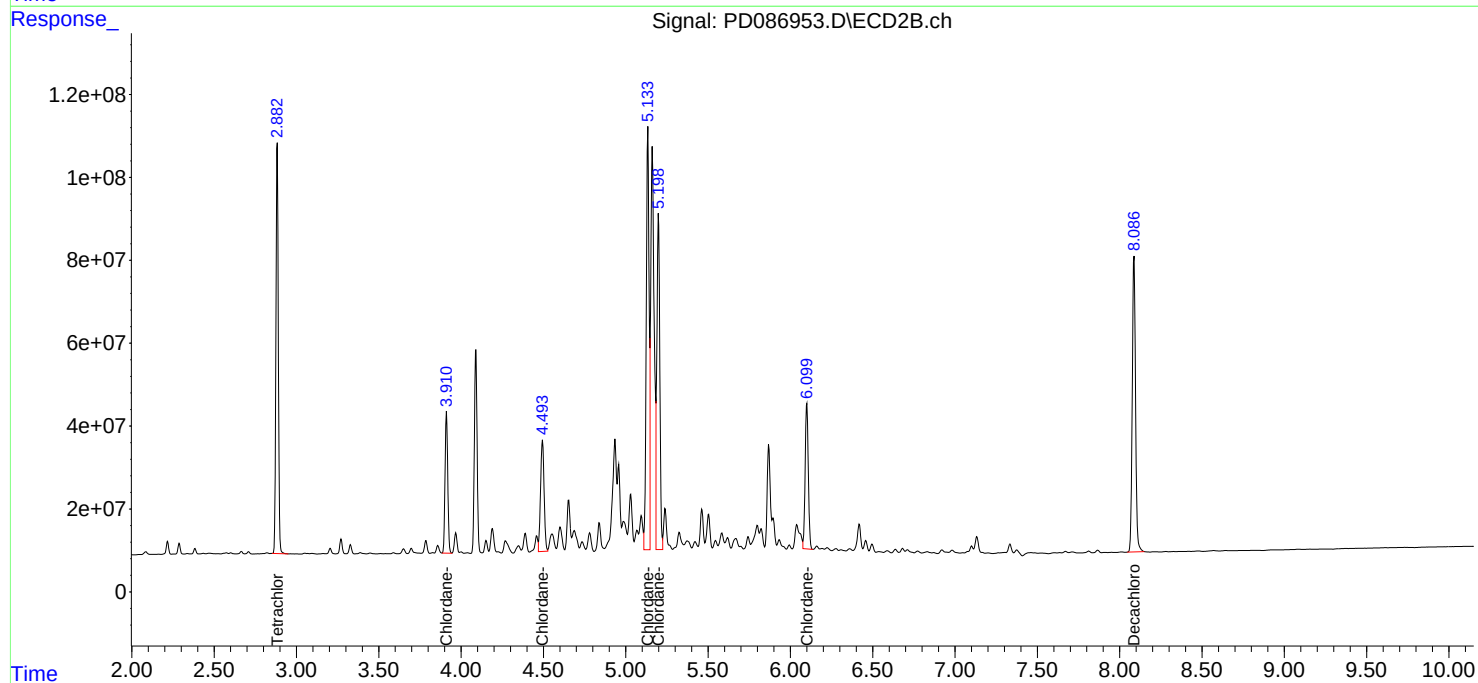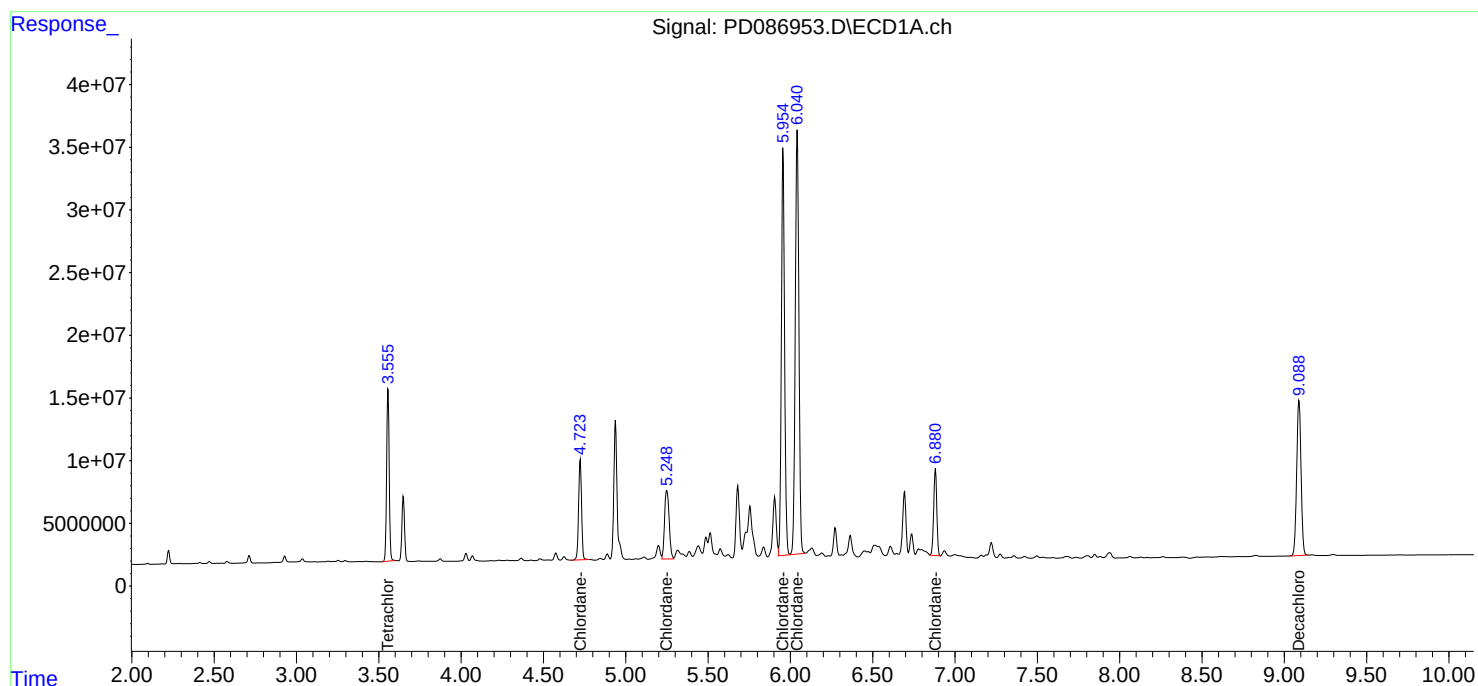


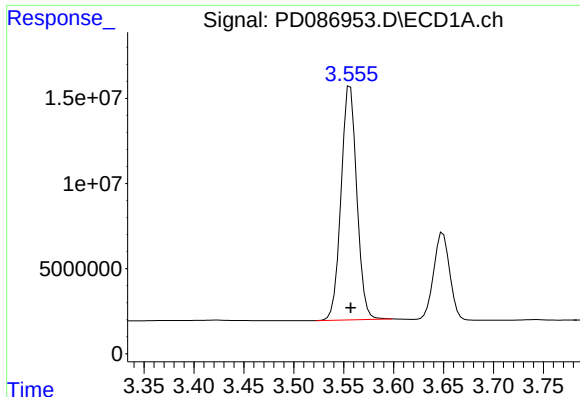

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 150982784
Conc: 75.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

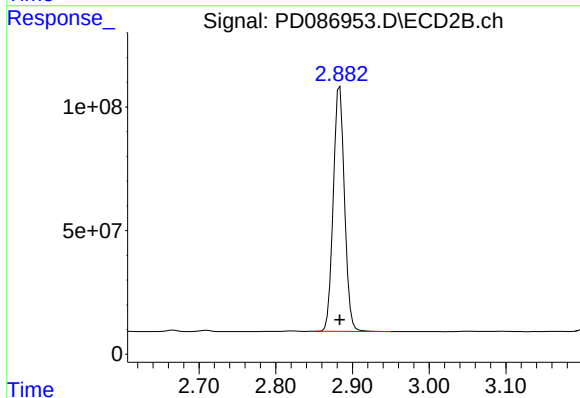


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 1007025130
Conc: 75.27 ng/ml

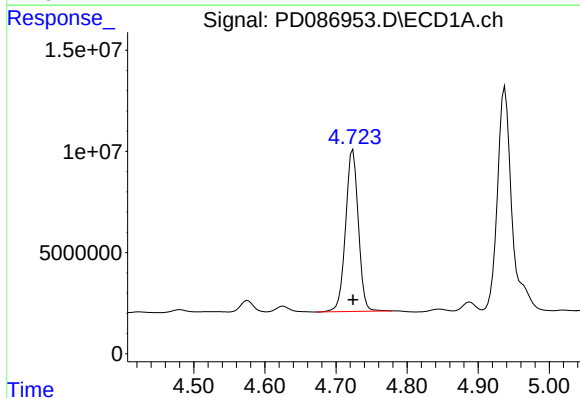


#23 Chlordane-1

R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 99887109
Conc: 755.13 ng/ml

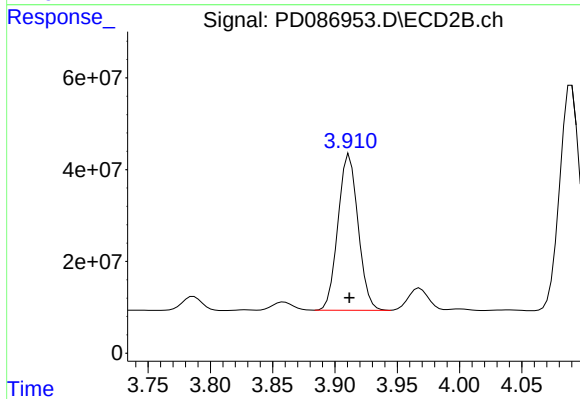

#23 Chlordane-1


R.T.: 3.912 min
Delta R.T.: 0.000 min
Response: 383569091
Conc: 750.72 ng/ml

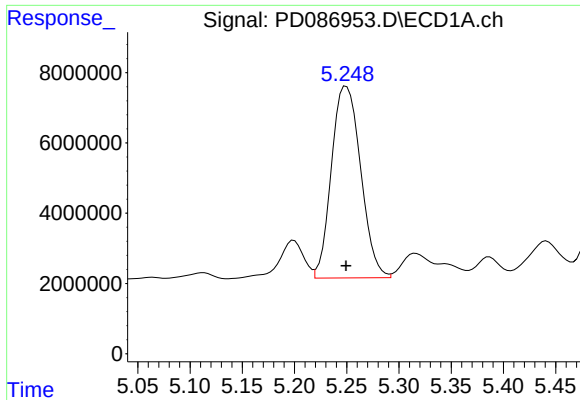

#24 Chlordane-2


R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 106153880
Conc: 752.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

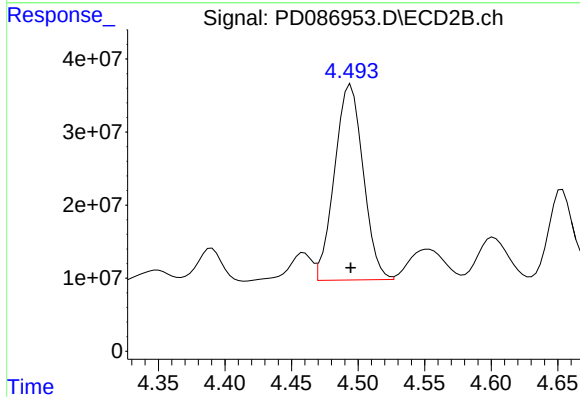


#24 Chlordane-2

R.T.: 4.495 min
Delta R.T.: 0.000 min
Response: 400800633
Conc: 749.22 ng/ml

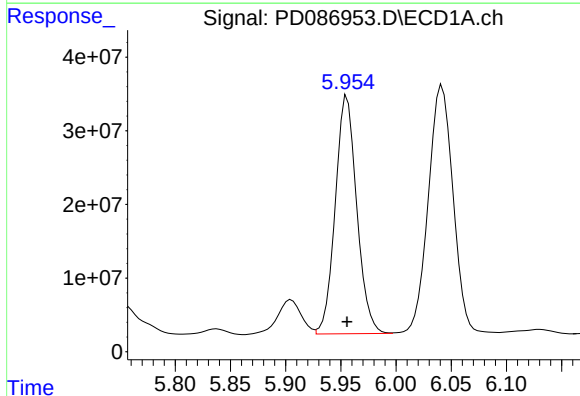


#25 Chlordane-3

R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 438302459
Conc: 757.81 ng/ml

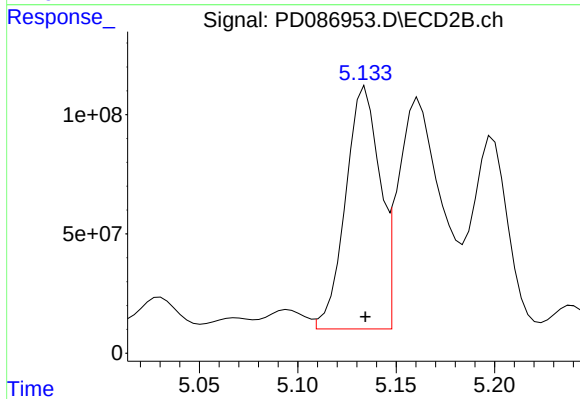

#25 Chlordane-3


R.T.: 5.134 min
Delta R.T.: 0.000 min
Response: 1221510063
Conc: 754.69 ng/ml

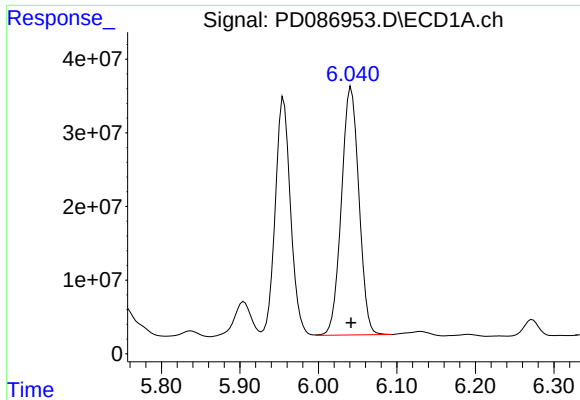

#26 Chlordane-4


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 522593506
Conc: 756.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

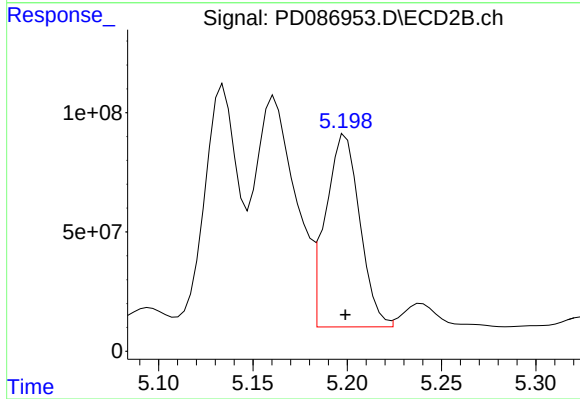


#26 Chlordane-4

R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 1019267291
Conc: 747.80 ng/ml

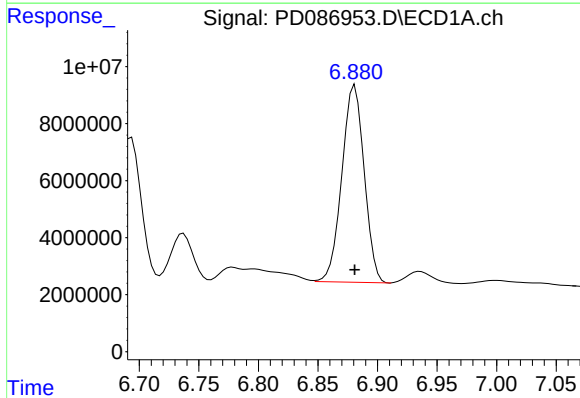


#27 Chlordane-5

R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 90210217
Conc: 754.73 ng/ml

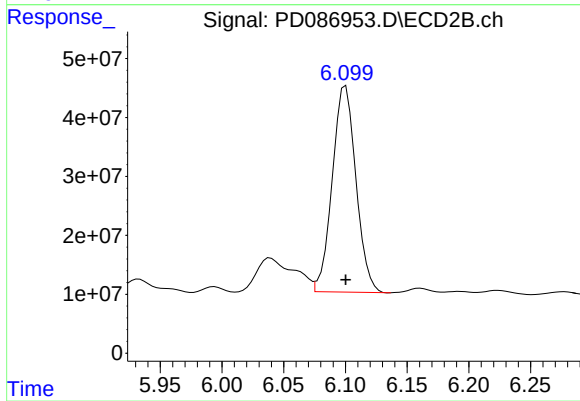

#27 Chlordane-5


R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 467542624
Conc: 748.55 ng/ml

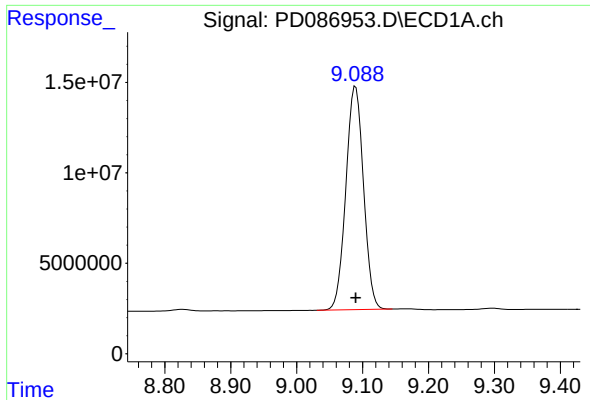

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 229628736
Conc: 75.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

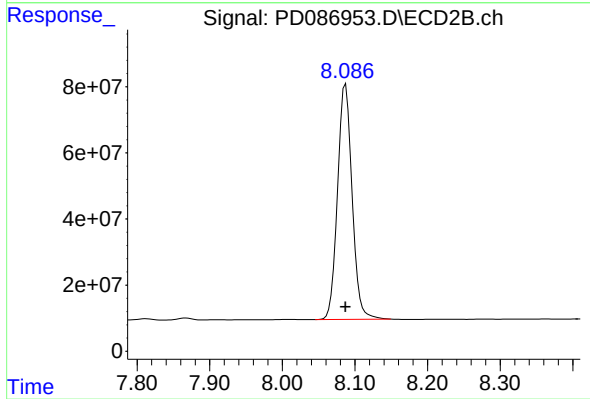

#28 Decachlorobiphenyl

R.T.: 8.087 min
Delta R.T.: 0.000 min
Response: 992743213
Conc: 74.95 ng/ml