

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
 Data File : PD086955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2024 13:20
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 13:30:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 13:30:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.884	50404869	360.7E6	25.160	26.441
28)	SA Decachlor...	9.090	8.088	82203188	369.2E6	26.405	27.094
Target Compounds							
23)	Chlordane-1	4.724	3.912	32699588	139.9E6	247.898	267.378
24)	Chlordane-2	5.250	4.495	37801467	151.0E6	263.278	273.447
25)	Chlordane-3	5.956	5.135	136.8E6	440.3E6	239.811	266.151
26)	Chlordane-4	6.042	5.200	166.8E6	371.9E6	243.571	266.744
27)	Chlordane-5	6.881	6.100	29919977	171.1E6	250.241	267.551



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
Data File : PD086955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2024 13:20
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 13:30:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 13:30:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

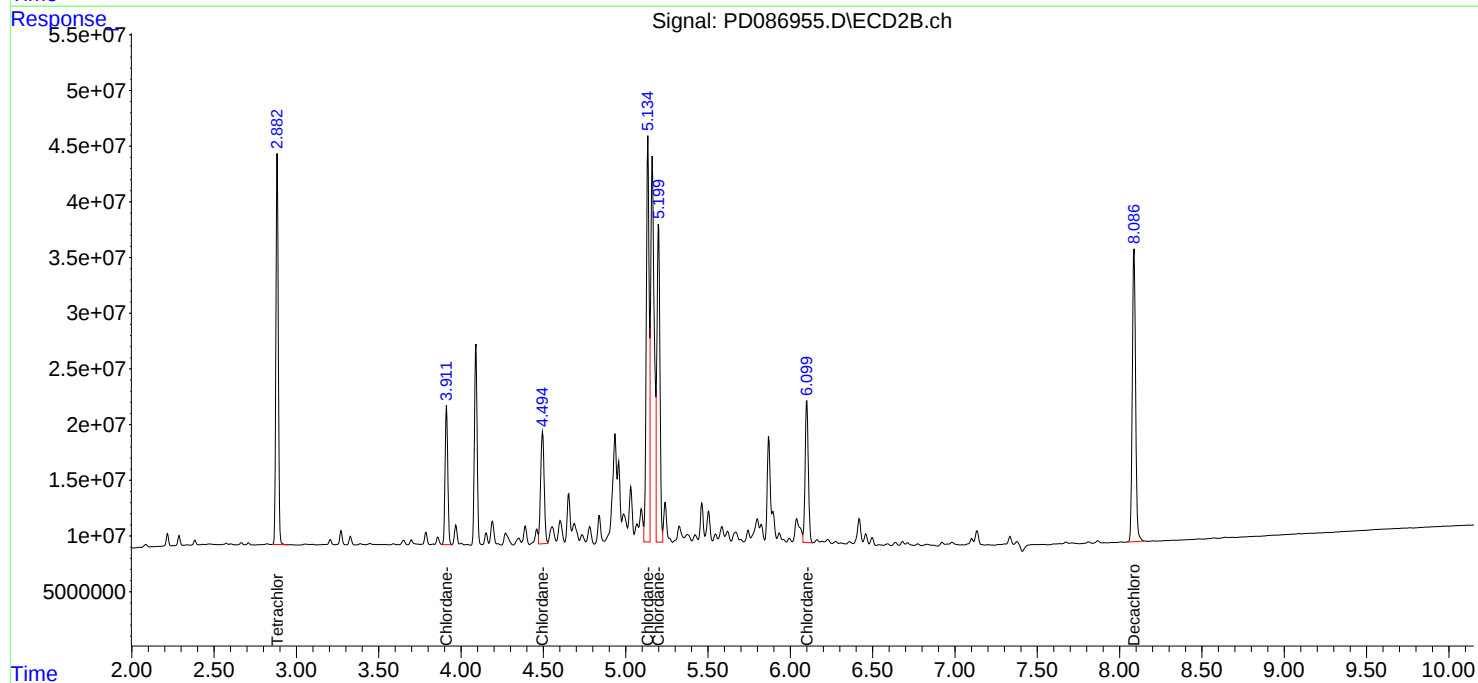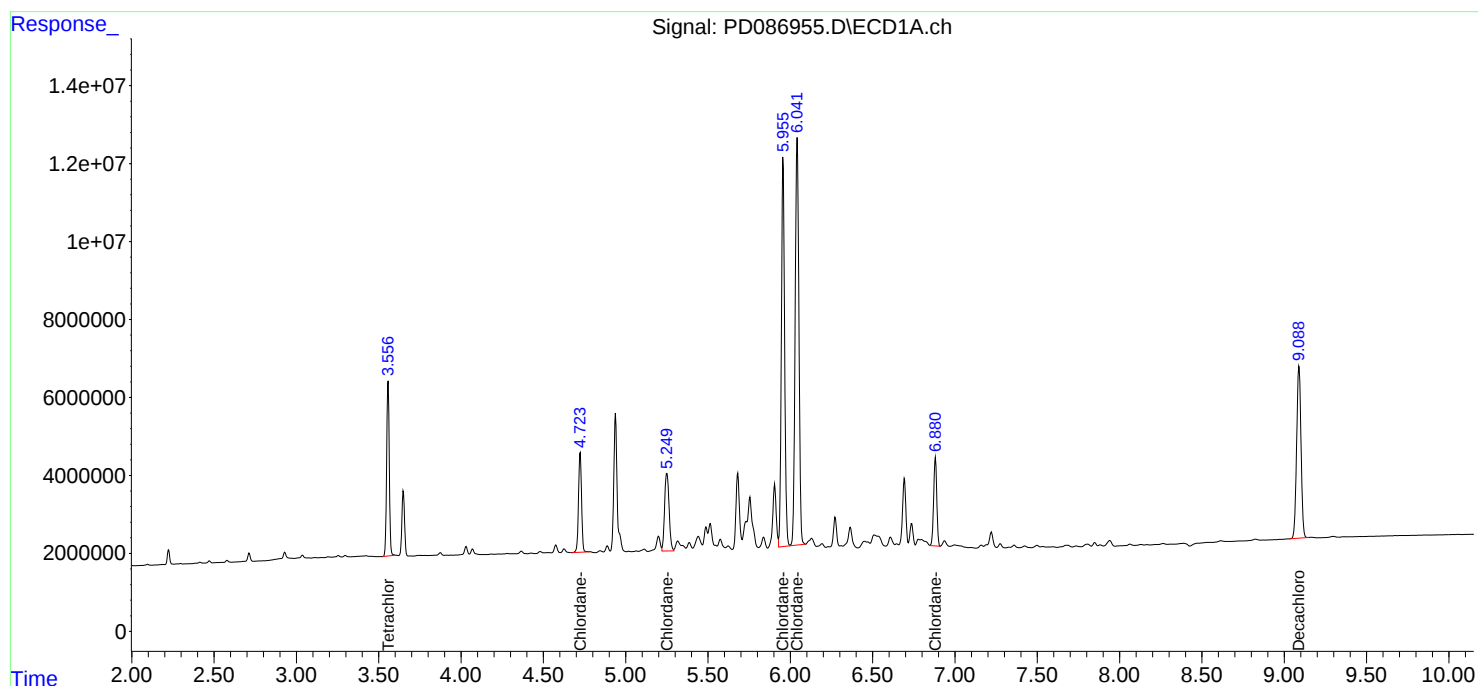


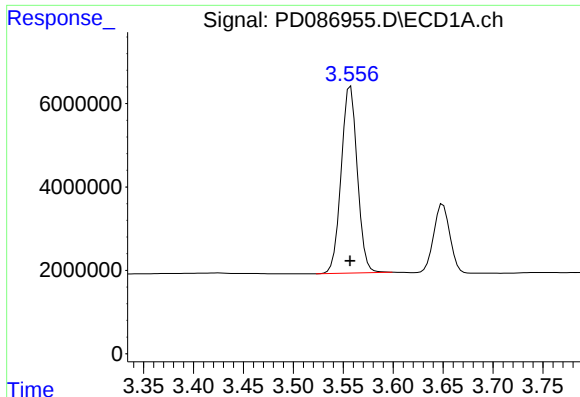

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 50404869
Conc: 25.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

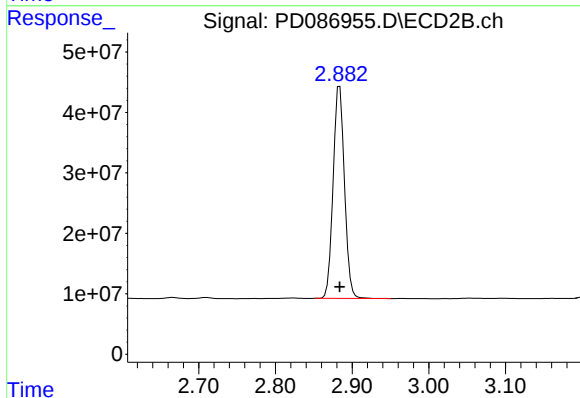


#1 Tetrachloro-m-xylene

R.T.: 2.884 min
Delta R.T.: 0.000 min
Response: 360707695
Conc: 26.44 ng/ml

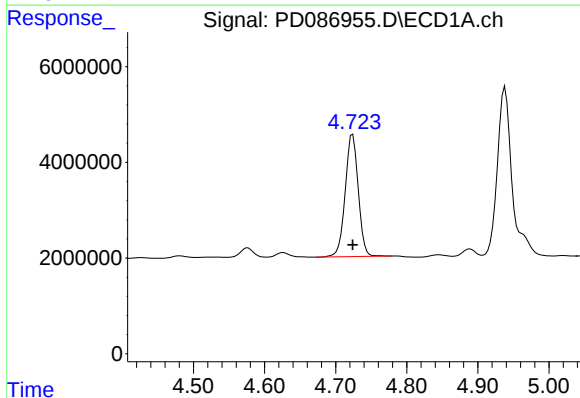


#23 Chlordane-1

R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 32699588
Conc: 247.90 ng/ml

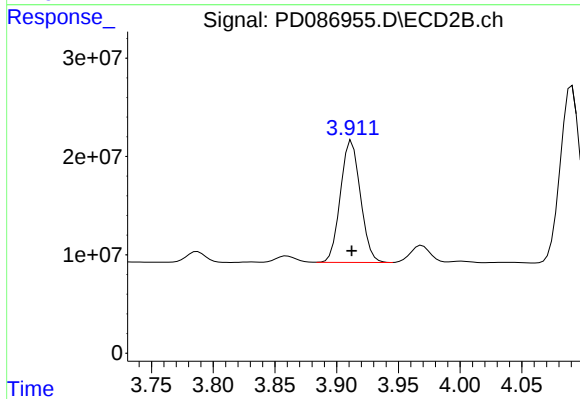

#23 Chlordane-1


R.T.: 3.912 min
Delta R.T.: 0.000 min
Response: 139854064
Conc: 267.38 ng/ml

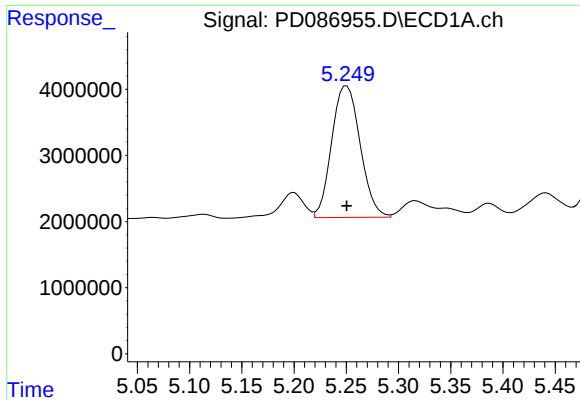

#24 Chlordane-2


R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 37801467
Conc: 263.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

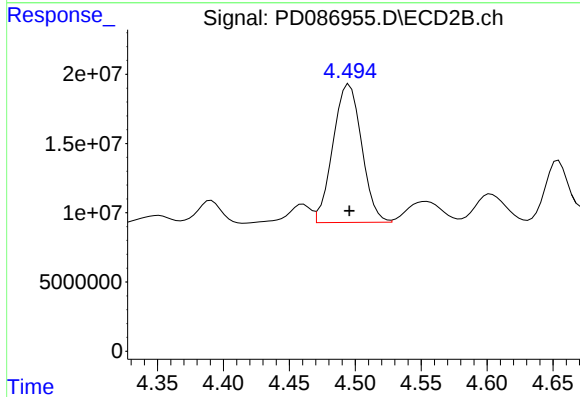


#24 Chlordane-2

R.T.: 4.495 min
Delta R.T.: 0.000 min
Response: 151004038
Conc: 273.45 ng/ml

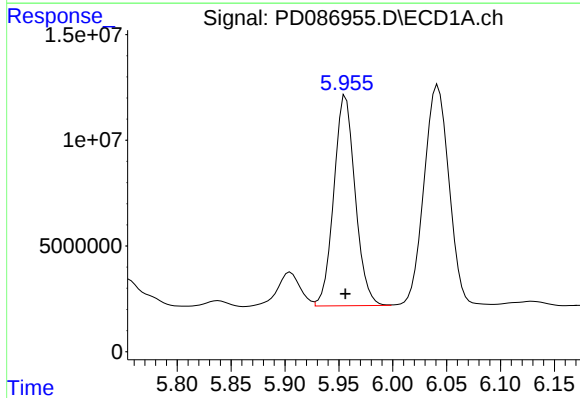


#25 Chlordane-3

R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 136842851
Conc: 239.81 ng/ml

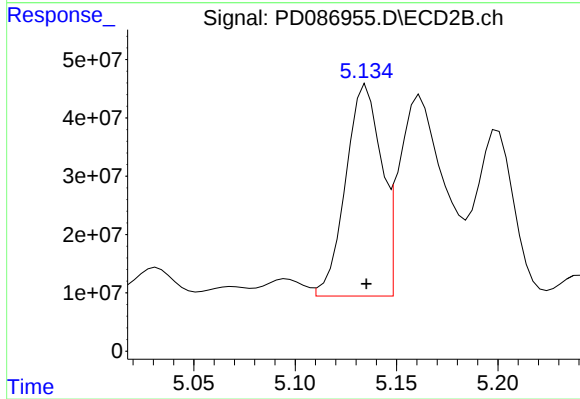

#25 Chlordane-3


R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 440261096
Conc: 266.15 ng/ml

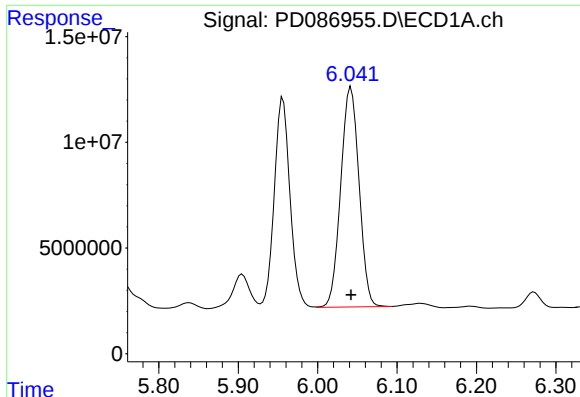

#26 Chlordane-4


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 166776657
Conc: 243.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

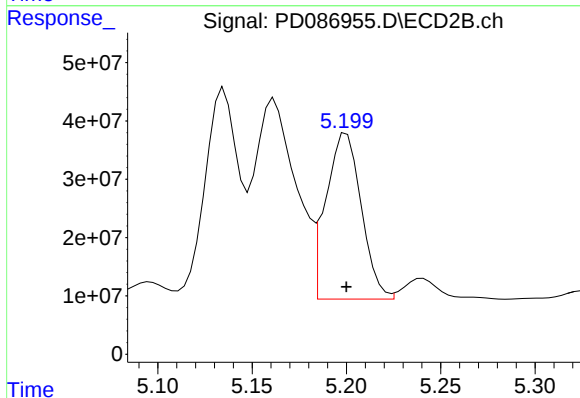


#26 Chlordane-4

R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 371881394
Conc: 266.74 ng/ml

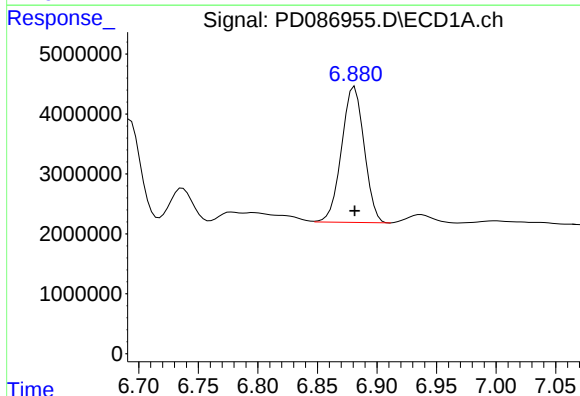


#27 Chlordane-5

R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 29919977
Conc: 250.24 ng/ml

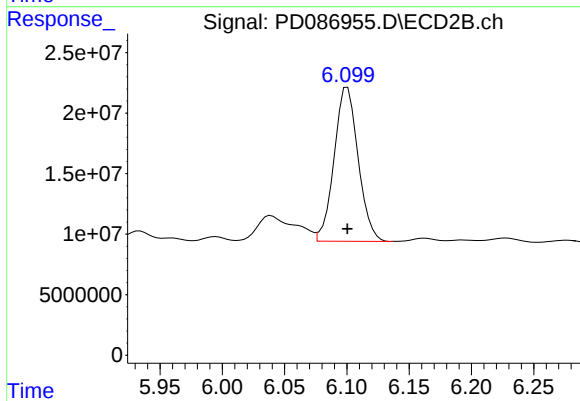

#27 Chlordane-5


R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 171116502
Conc: 267.55 ng/ml

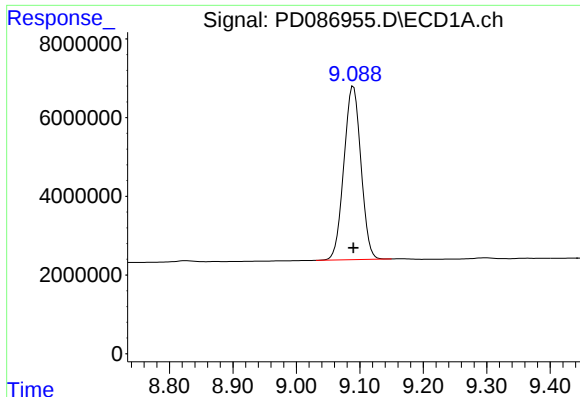

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 82203188
Conc: 26.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

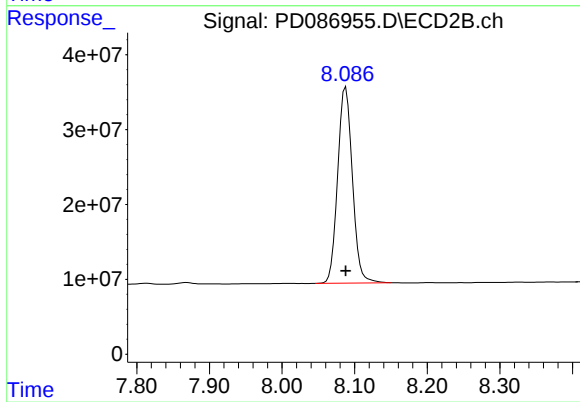

#28 Decachlorobiphenyl

R.T.: 8.088 min
Delta R.T.: 0.000 min
Response: 369172973
Conc: 27.09 ng/ml