

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
 Data File : PD086952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2024 12:38
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 13:22:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 13:19:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.884	197.2E6	1285.2E6	99.000	96.228
28)	SA Decachlor...	9.089	8.088	293.8E6	1264.9E6	96.297	95.463
Target Compounds							
23)	Chlordane-1	4.725	3.912	131.4E6	490.1E6	996.840	959.761
24)	Chlordane-2	5.251	4.495	136.3E6	507.4E6	967.826	948.024
25)	Chlordane-3	5.956	5.135	577.4E6	1556.7E6	1003.462	964.809
26)	Chlordane-4	6.042	5.200	686.8E6	1307.2E6	998.982	957.625
27)	Chlordane-5	6.882	6.100	118.2E6	601.5E6	991.733	962.065



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
Data File : PD086952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2024 12:38
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 13:22:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 13:19:46 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

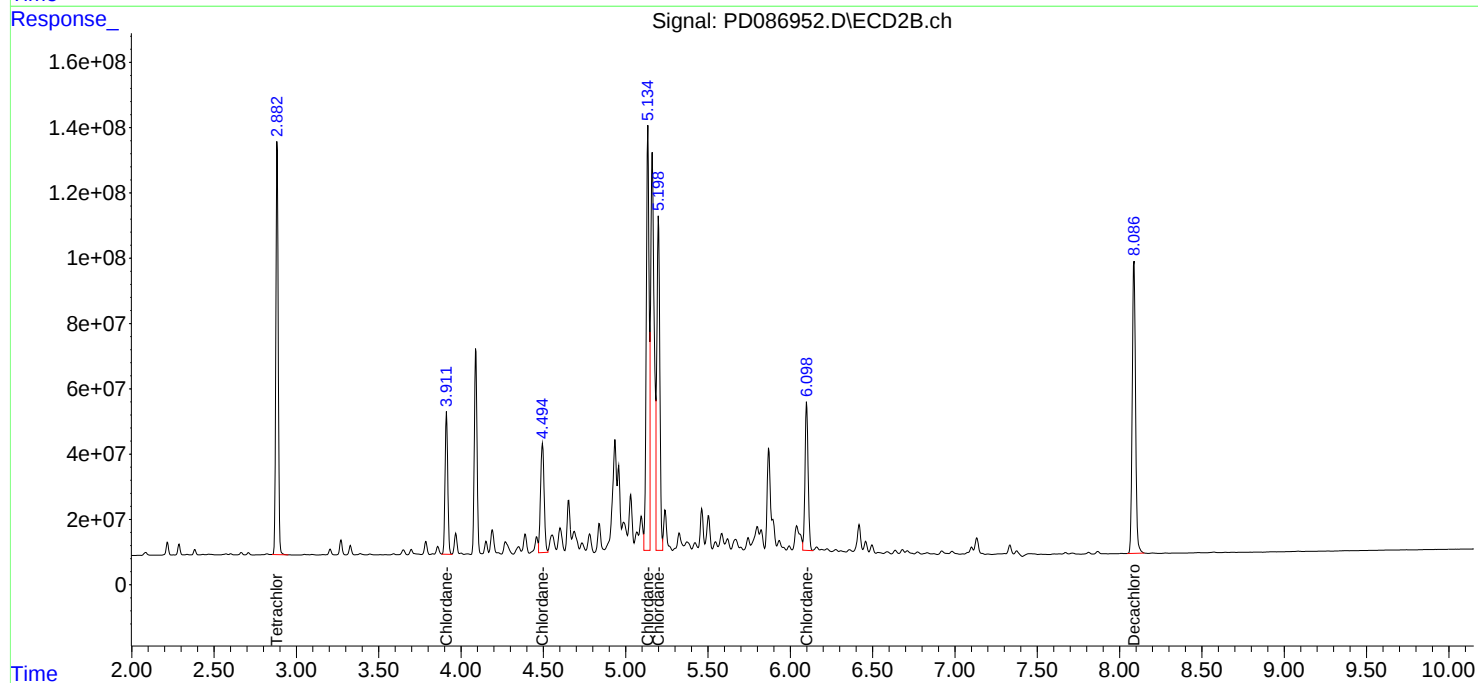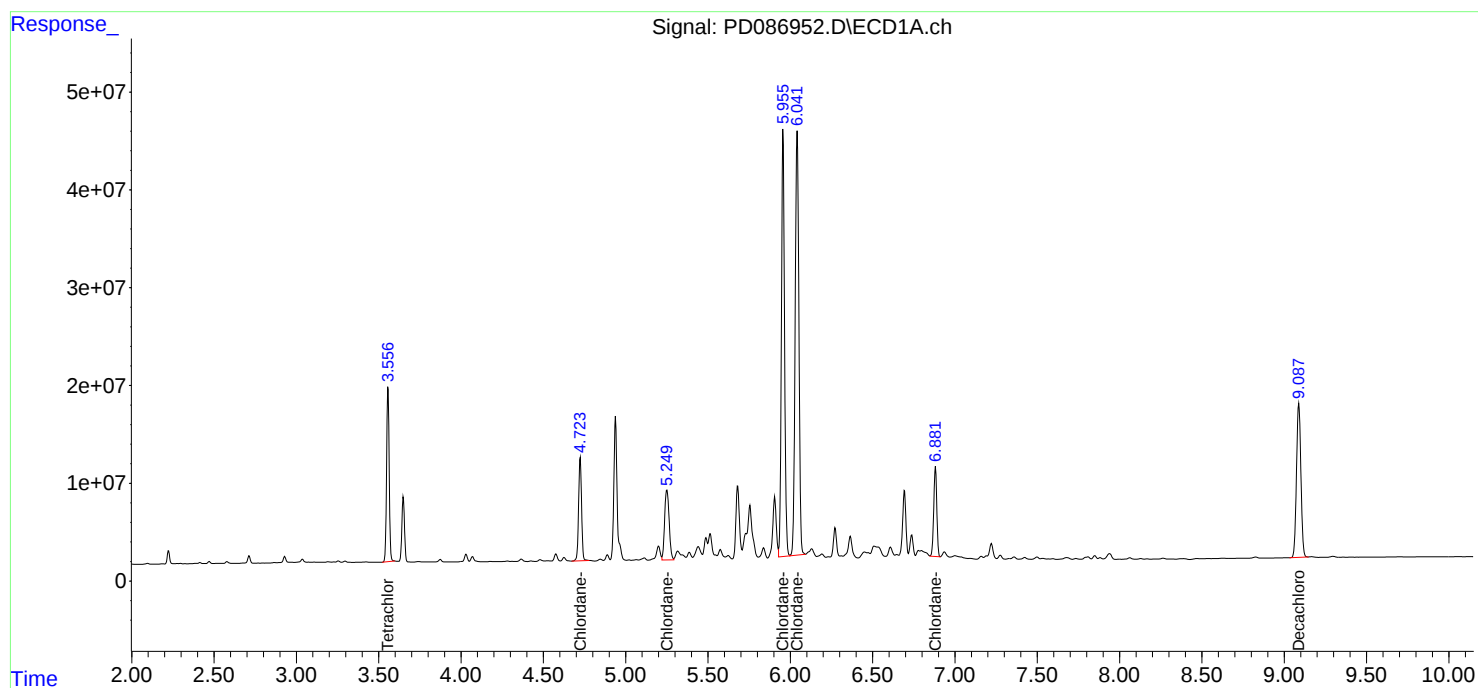


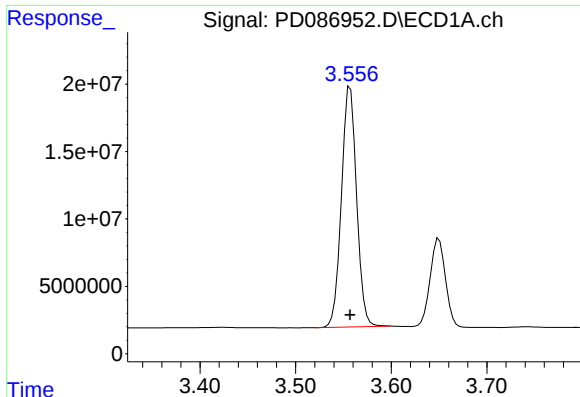

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 197218276
Conc: 99.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

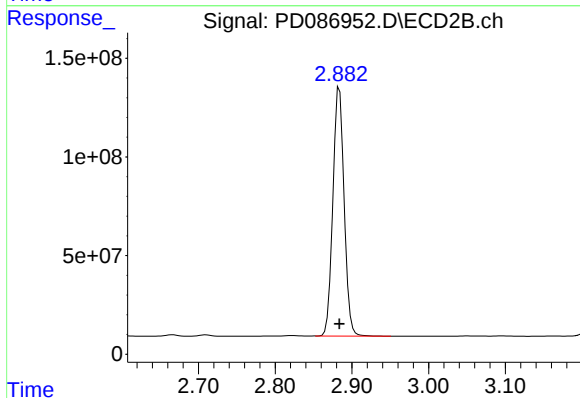


#1 Tetrachloro-m-xylene

R.T.: 2.884 min
Delta R.T.: 0.000 min
Response: 1285229054
Conc: 96.23 ng/ml

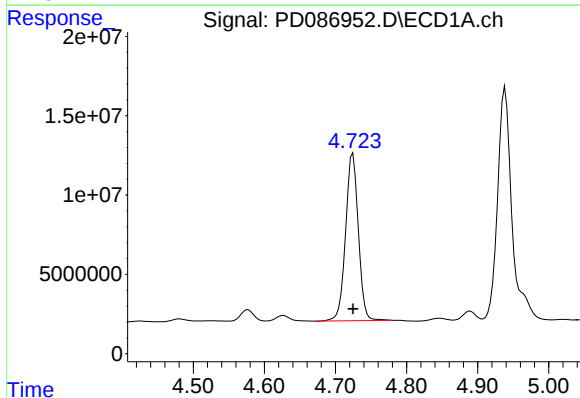


#23 Chlordane-1

R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 131407914
Conc: 996.84 ng/ml

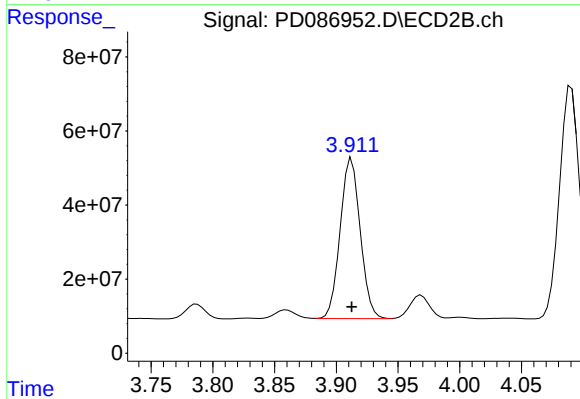

#23 Chlordane-1


R.T.: 3.912 min
Delta R.T.: 0.000 min
Response: 490143883
Conc: 959.76 ng/ml

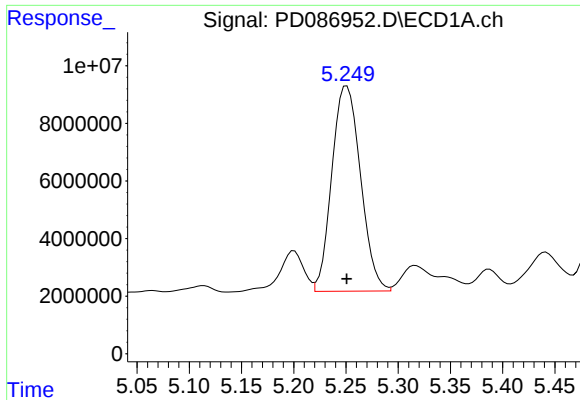

#24 Chlordane-2


R.T.: 5.251 min
Delta R.T.: 0.000 min
Response: 136257874
Conc: 967.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

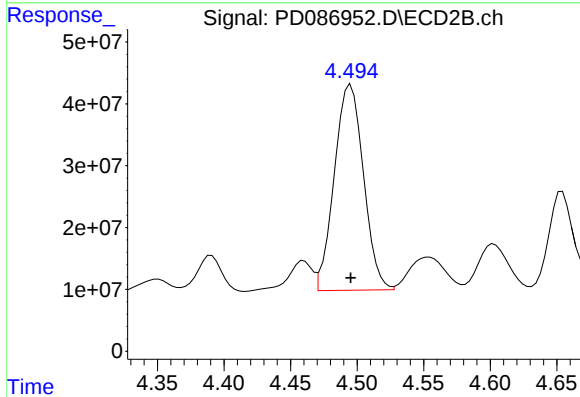


#24 Chlordane-2

R.T.: 4.495 min
Delta R.T.: 0.000 min
Response: 507419355
Conc: 948.02 ng/ml

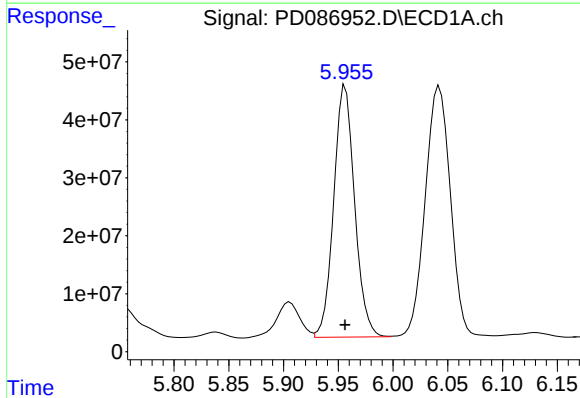


#25 Chlordane-3

R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 577361205
Conc: 1003.46 ng/ml

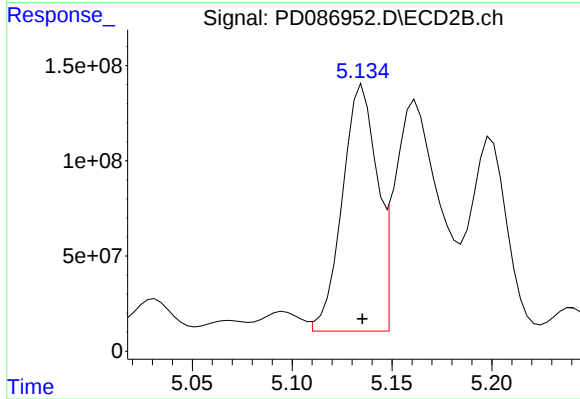

#25 Chlordane-3


R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 1556715482
Conc: 964.81 ng/ml

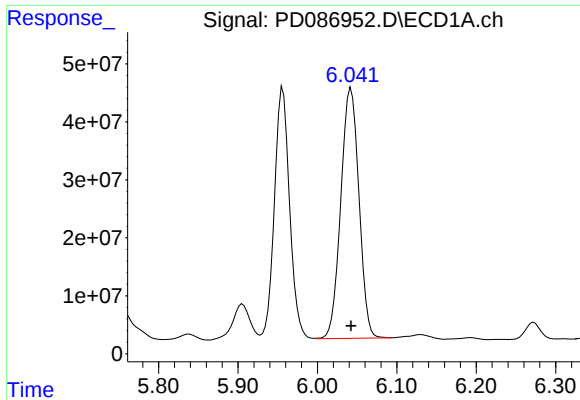

#26 Chlordane-4


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 686780634
Conc: 998.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

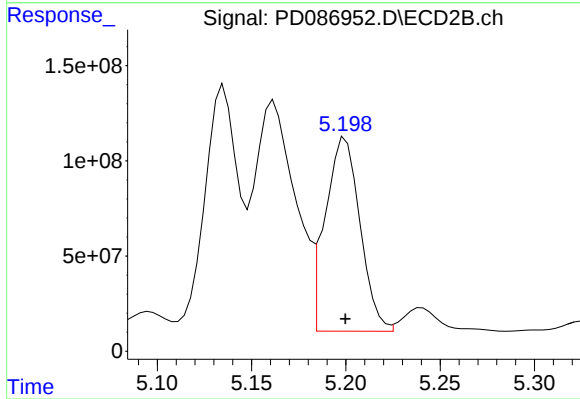


#26 Chlordane-4

R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 1307185010
Conc: 957.62 ng/ml

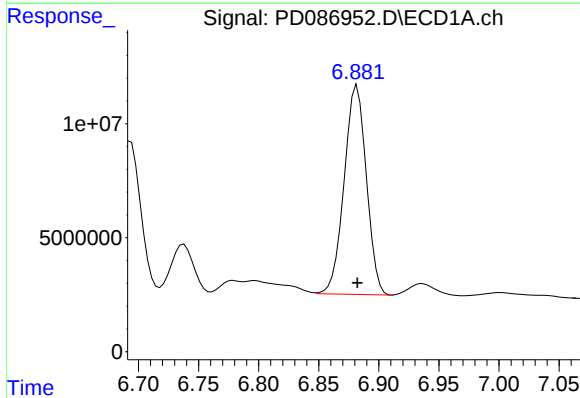


#27 Chlordane-5

R.T.: 6.882 min
Delta R.T.: 0.000 min
Response: 118164021
Conc: 991.73 ng/ml

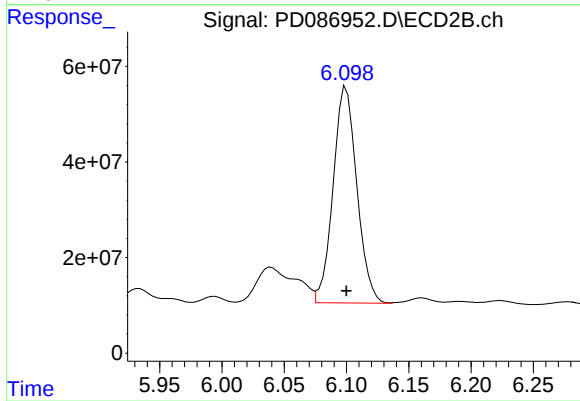

#27 Chlordane-5


R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 601485145
Conc: 962.07 ng/ml

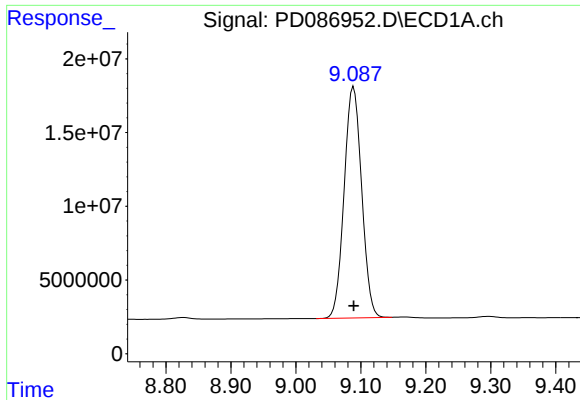

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 293846382
Conc: 96.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

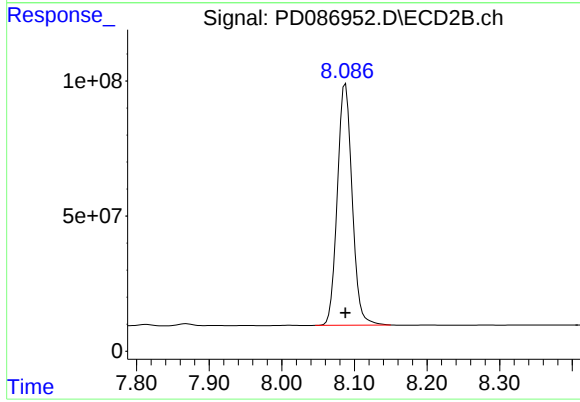

#28 Decachlorobiphenyl

R.T.: 8.088 min
Delta R.T.: 0.000 min
Response: 1264876085
Conc: 95.46 ng/ml