

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
 Data File : PD086954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2024 13:06
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 13:20:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 13:19:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.884	100.6E6	693.0E6	50.000	50.000
28)	SA Decachlor...	9.090	8.088	158.2E6	692.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.724	3.912	66120490	265.6E6	500.000	500.000
24)	Chlordane-2	5.250	4.495	72658609	281.5E6	500.000	500.000
25)	Chlordane-3	5.956	5.135	286.7E6	835.1E6	500.000	500.000
26)	Chlordane-4	6.042	5.200	344.1E6	711.4E6	500.000	500.000
27)	Chlordane-5	6.882	6.100	60067018	324.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
Data File : PD086954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2024 13:06
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 13:20:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 13:19:46 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

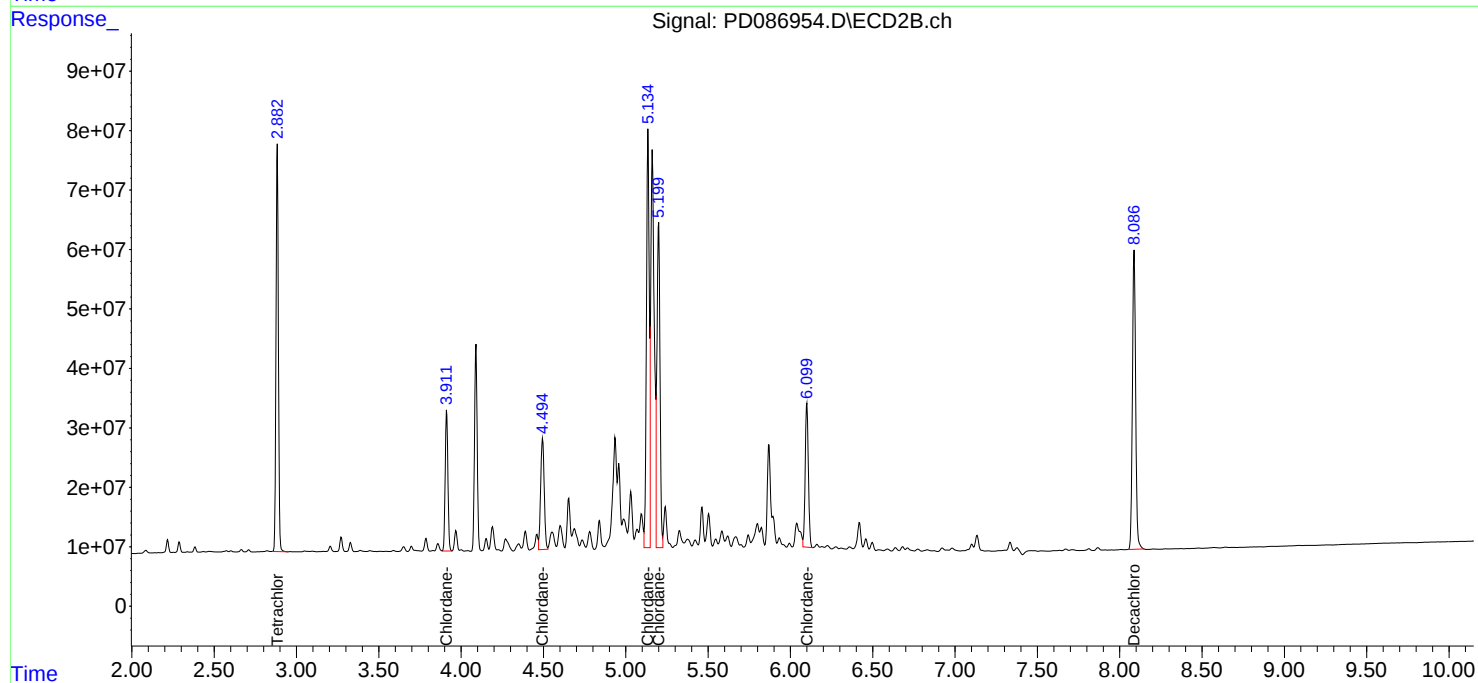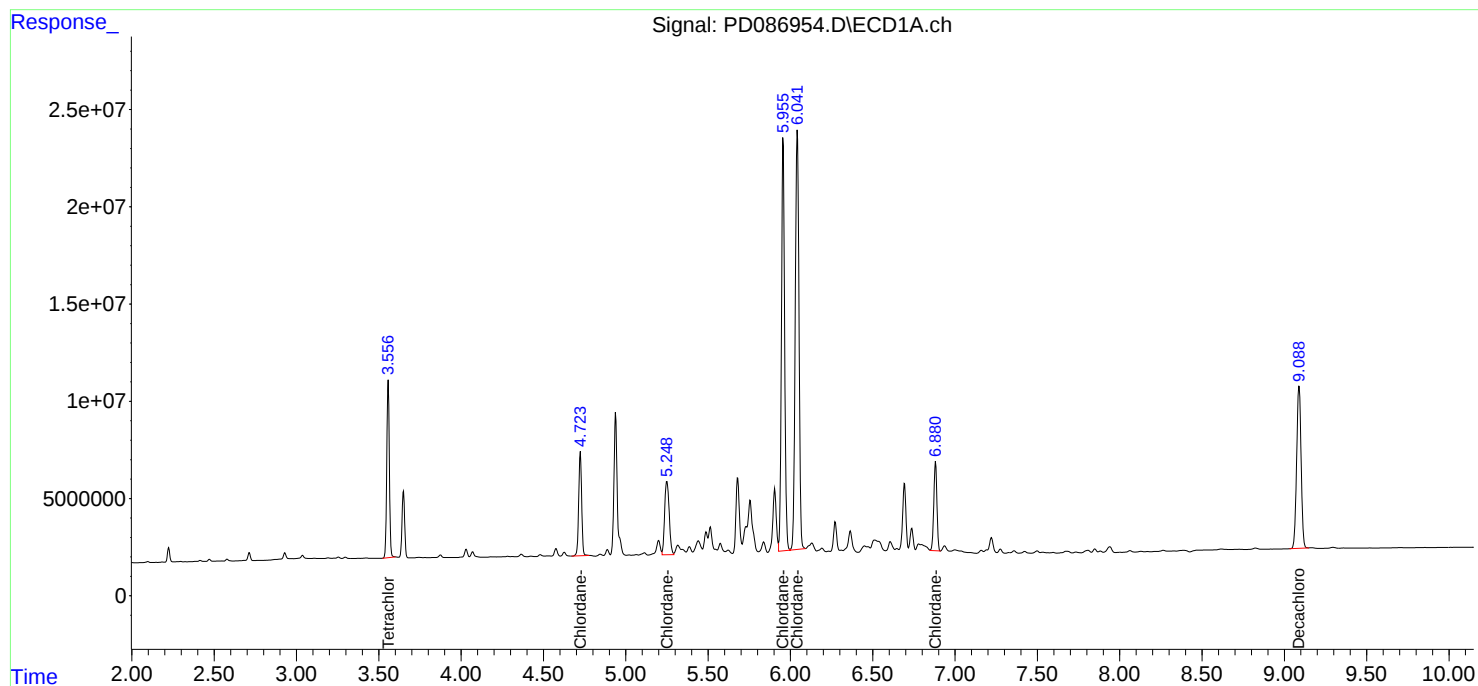


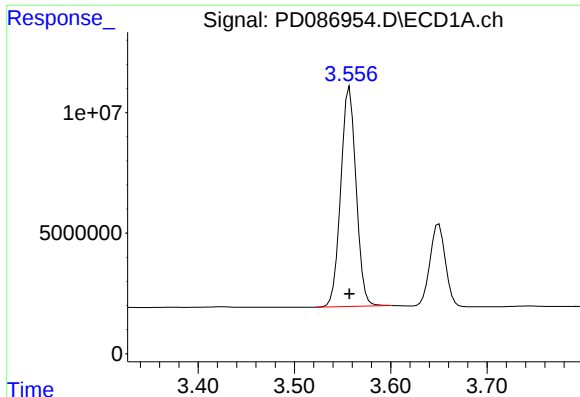

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 100600368
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

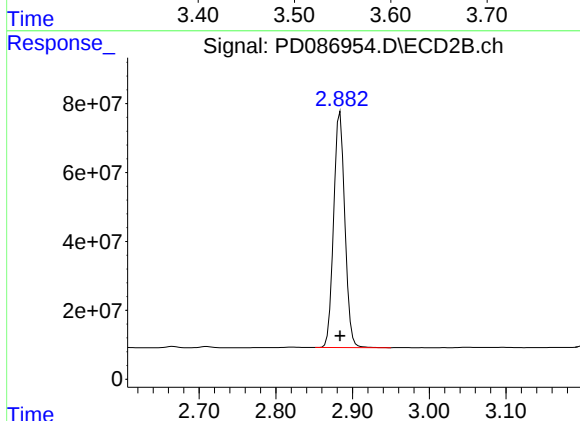


#1 Tetrachloro-m-xylene

R.T.: 2.884 min
Delta R.T.: 0.000 min
Response: 692991347
Conc: 50.00 ng/ml

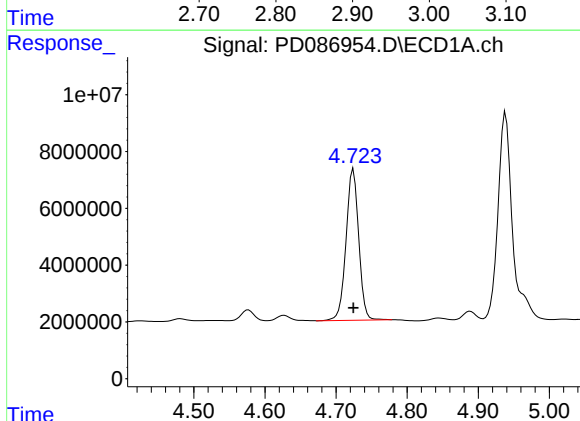


#23 Chlordane-1

R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 66120490
Conc: 500.00 ng/ml

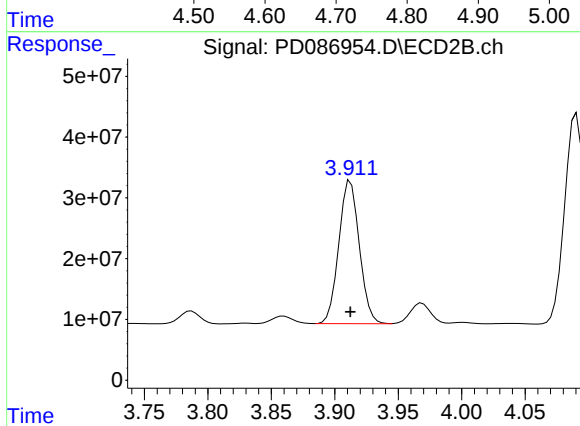

#23 Chlordane-1


R.T.: 3.912 min
Delta R.T.: 0.000 min
Response: 265621877
Conc: 500.00 ng/ml

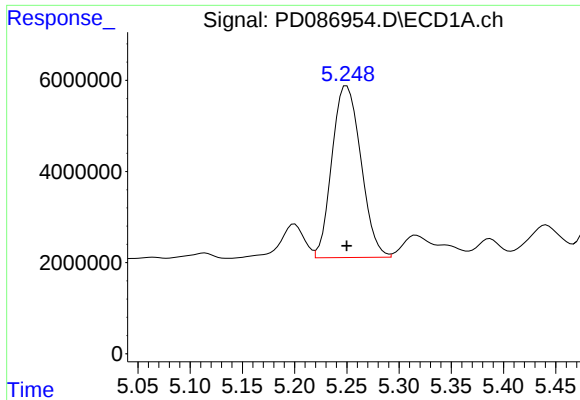

#24 Chlordane-2


R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 72658609
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

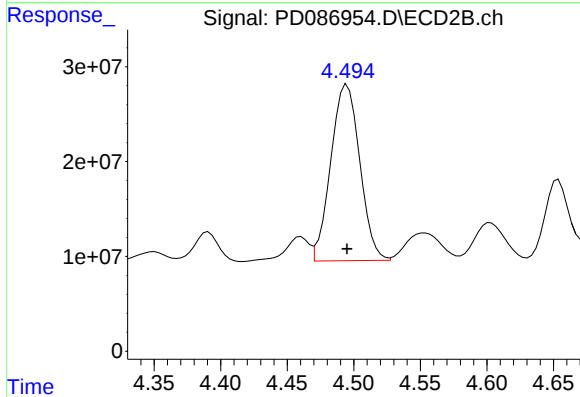


#24 Chlordane-2

R.T.: 4.495 min
Delta R.T.: 0.000 min
Response: 281529144
Conc: 500.00 ng/ml

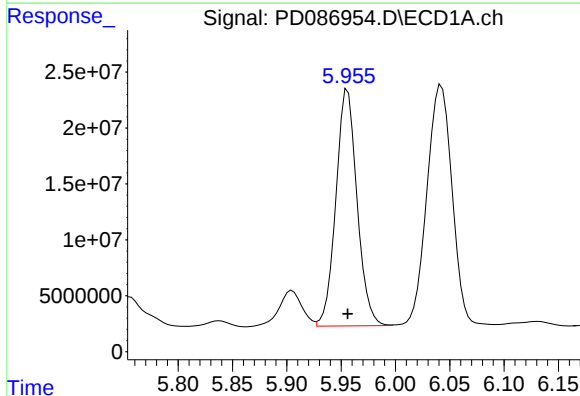


#25 Chlordane-3

R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 286688942
Conc: 500.00 ng/ml

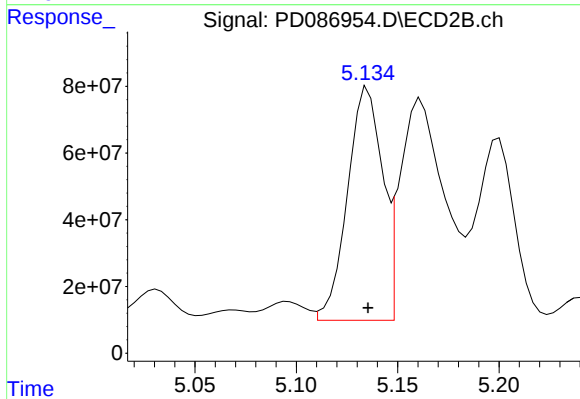

#25 Chlordane-3


R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 835137656
Conc: 500.00 ng/ml

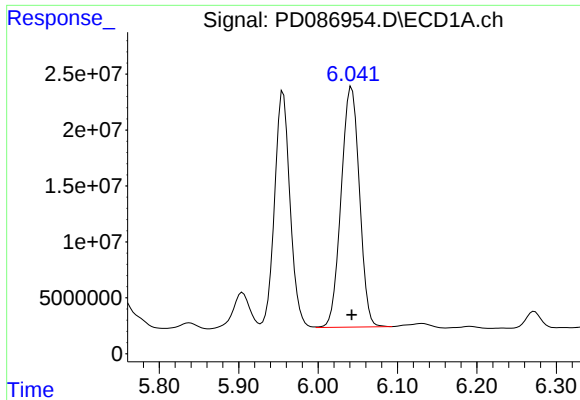

#26 Chlordane-4


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 344090010
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

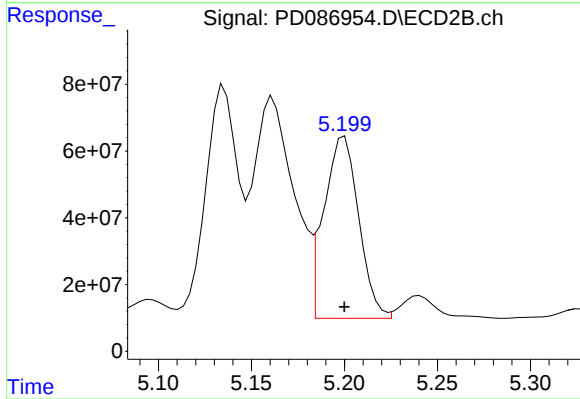


#26 Chlordane-4

R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 711436005
Conc: 500.00 ng/ml

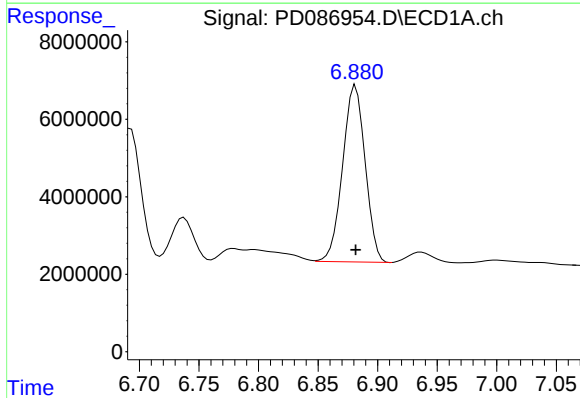


#27 Chlordane-5

R.T.: 6.882 min
Delta R.T.: 0.000 min
Response: 60067018
Conc: 500.00 ng/ml

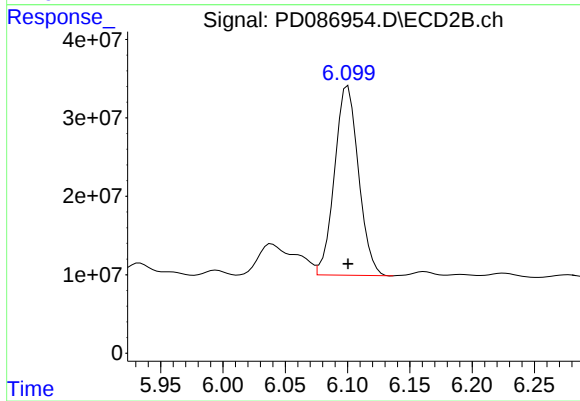

#27 Chlordane-5


R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 324459433
Conc: 500.00 ng/ml

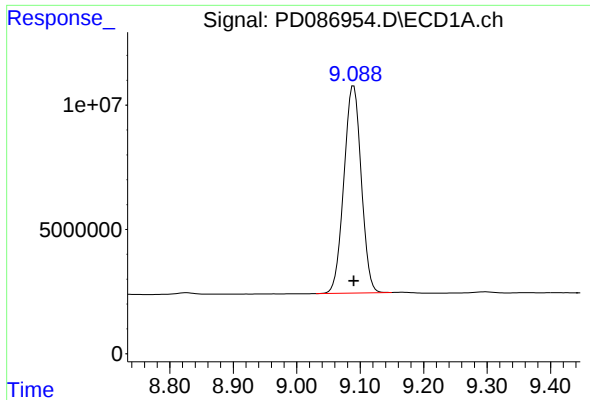

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 158222687
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

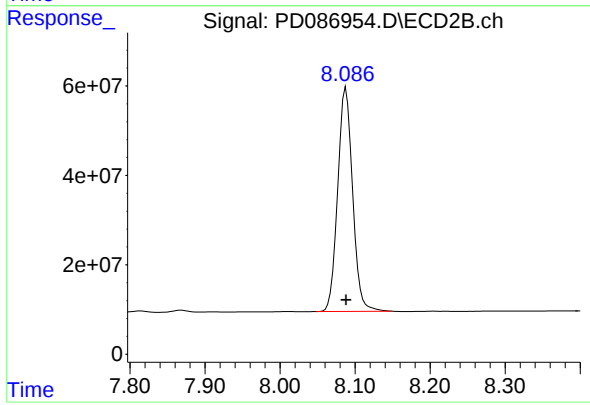

#28 Decachlorobiphenyl

R.T.: 8.088 min
Delta R.T.: 0.000 min
Response: 692547159
Conc: 50.00 ng/ml