

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
 Data File : PD086956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2024 13:34
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 13:44:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 13:44:07 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.884	8896799	66676997	4.542	4.910
28)	SA Decachlor...	9.089	8.088	15210384	72619775	4.908	5.260
Target Compounds							
23)	Chlordane-1	4.724	3.913	5548737	25495411	43.444	48.989
24)	Chlordane-2	5.250	4.496	6854882	28862249	48.178	51.796
25)	Chlordane-3	5.956	5.135	22281520	82678620	40.836	49.985
26)	Chlordane-4	6.042	5.199	27989668	71699146	42.426	51.136
27)	Chlordane-5	6.882	6.100	5409827	32276895	46.123	50.373



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
Data File : PD086956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2024 13:34
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 13:44:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 13:44:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

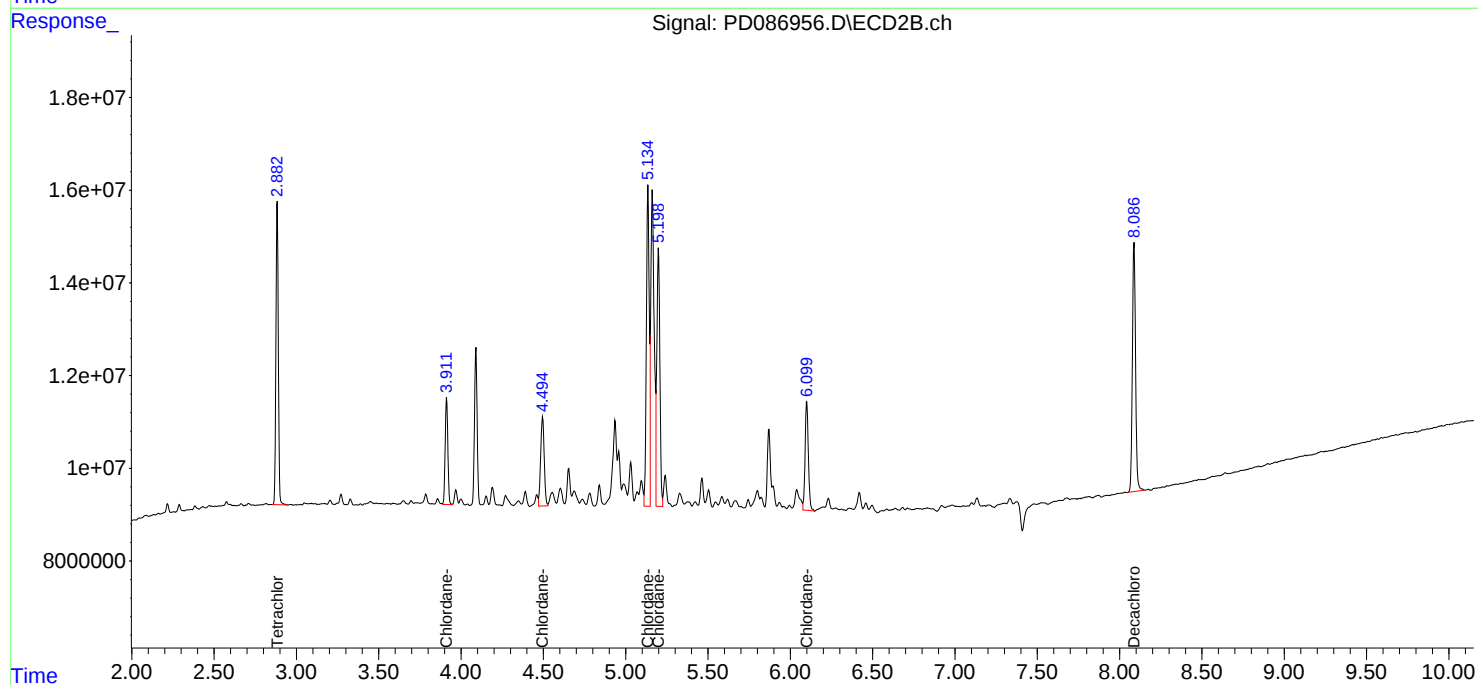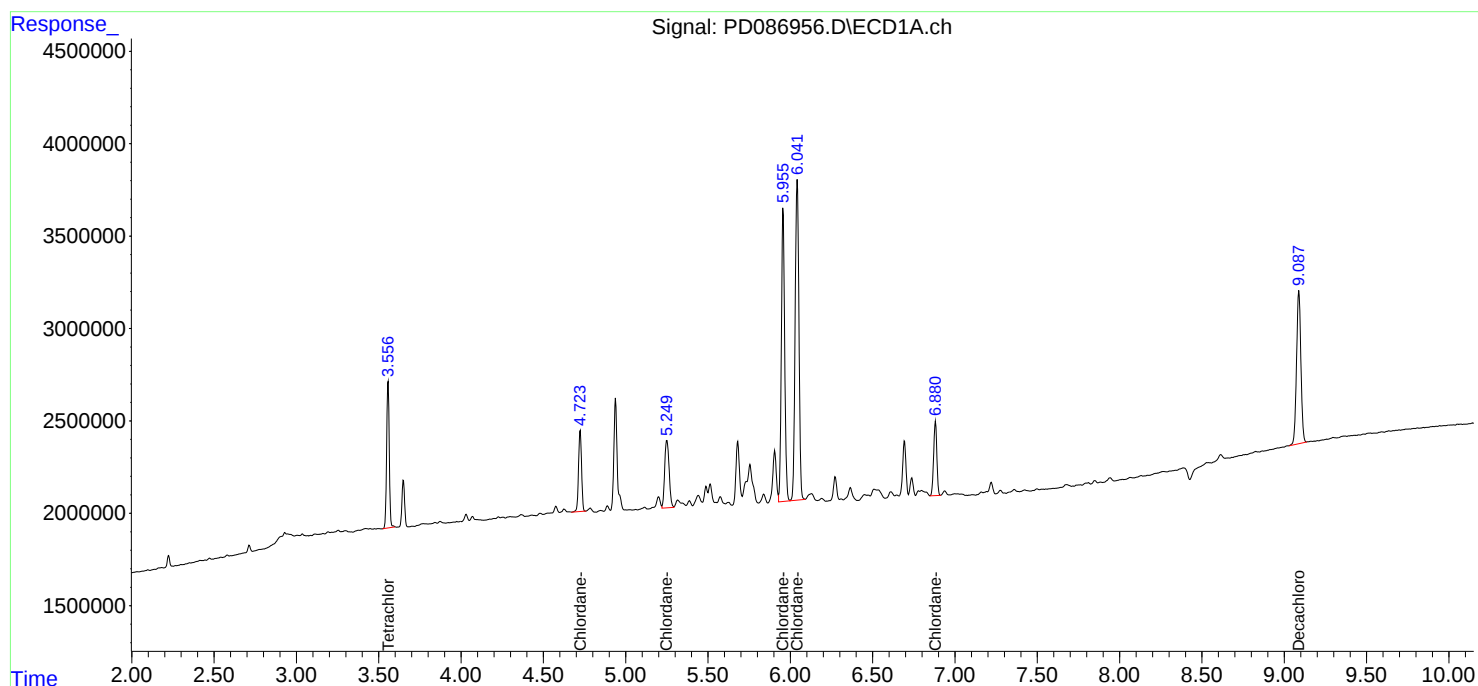


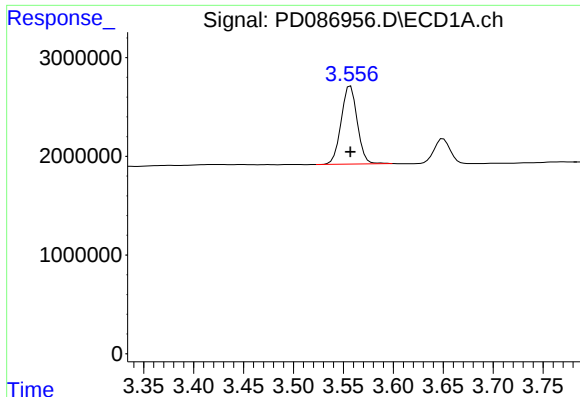

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 8896799
Conc: 4.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

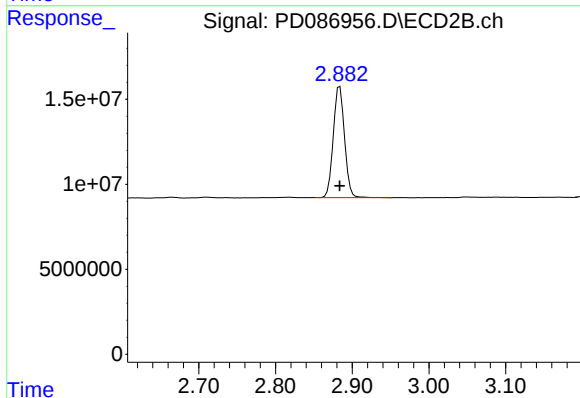


#1 Tetrachloro-m-xylene

R.T.: 2.884 min
Delta R.T.: 0.000 min
Response: 66676997
Conc: 4.91 ng/ml

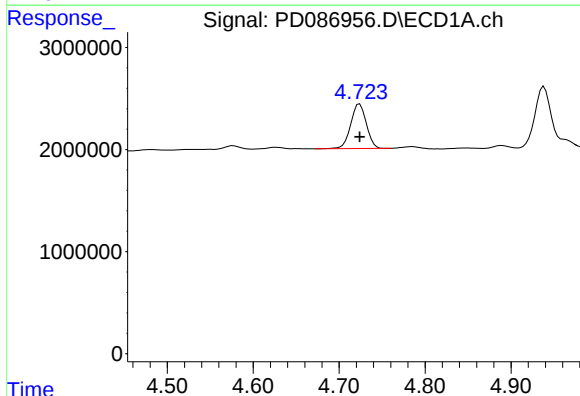


#23 Chlordane-1

R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 5548737
Conc: 43.44 ng/ml

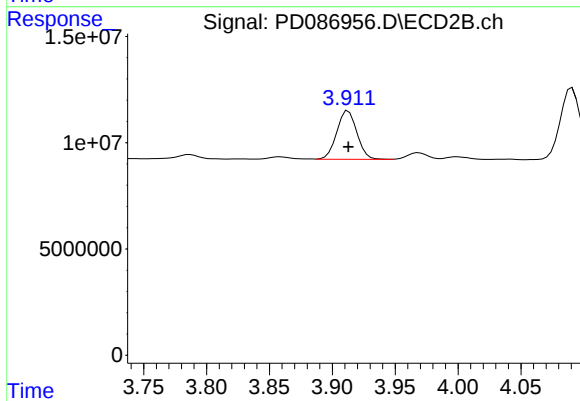

#23 Chlordane-1


R.T.: 3.913 min
Delta R.T.: 0.000 min
Response: 25495411
Conc: 48.99 ng/ml

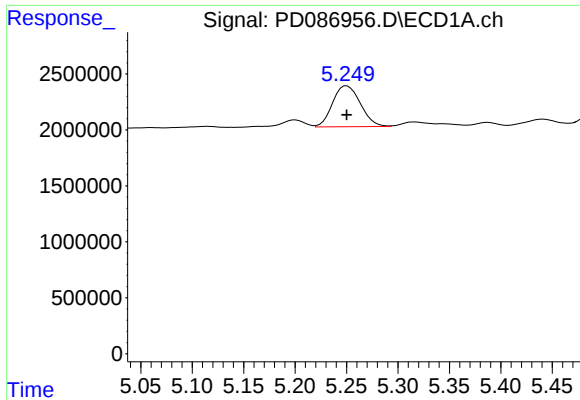

#24 Chlordane-2


R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 6854882
Conc: 48.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

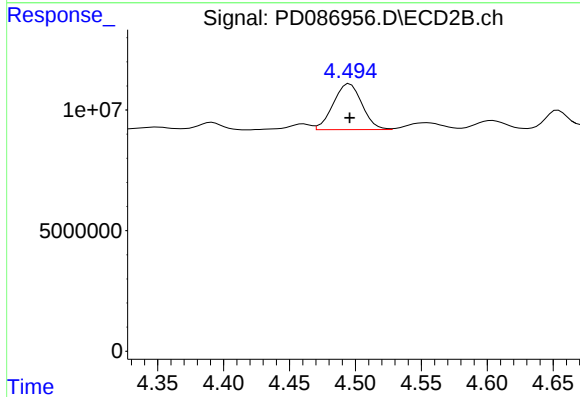


#24 Chlordane-2

R.T.: 4.496 min
Delta R.T.: 0.000 min
Response: 28862249
Conc: 51.80 ng/ml

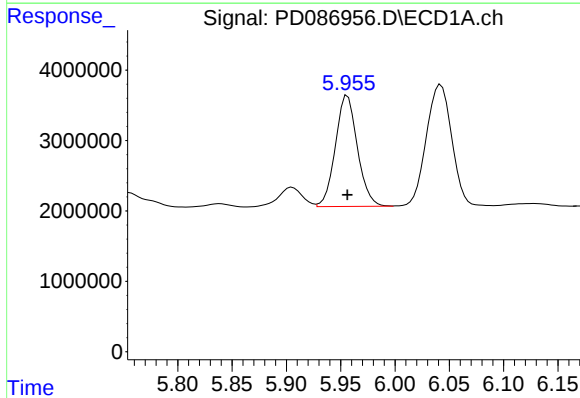


#25 Chlordane-3

R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 22281520
Conc: 40.84 ng/ml

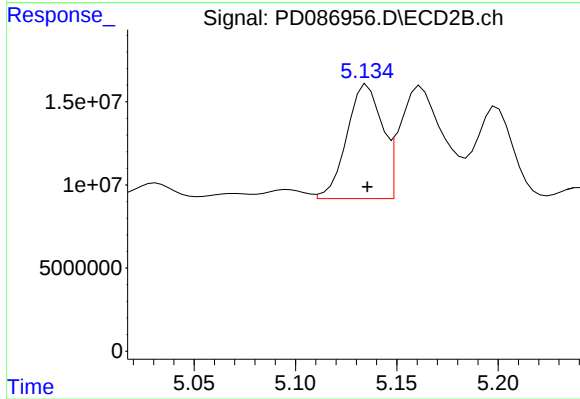

#25 Chlordane-3


R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 82678620
Conc: 49.99 ng/ml

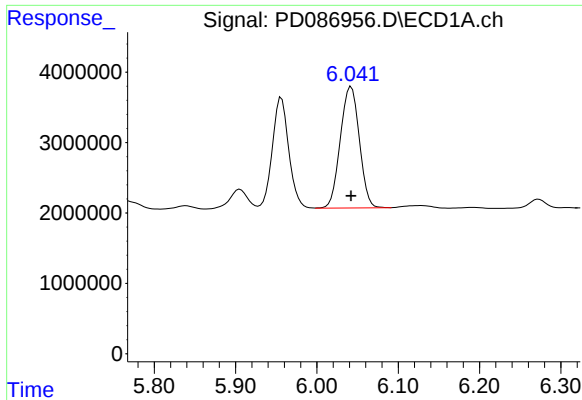

#26 Chlordane-4


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 27989668
Conc: 42.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

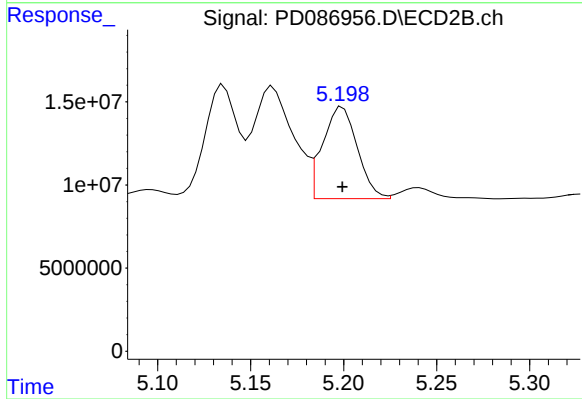


#26 Chlordane-4

R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 71699146
Conc: 51.14 ng/ml

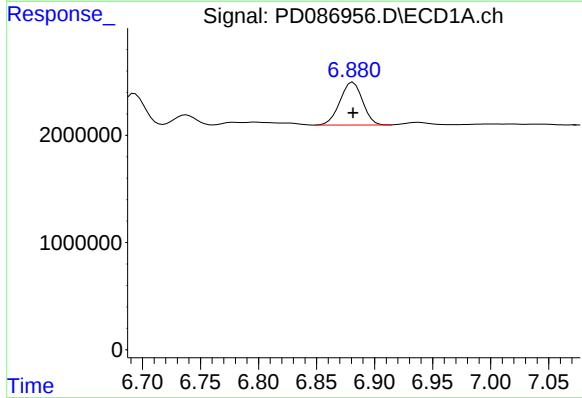


#27 Chlordane-5

R.T.: 6.882 min
Delta R.T.: 0.000 min
Response: 5409827
Conc: 46.12 ng/ml

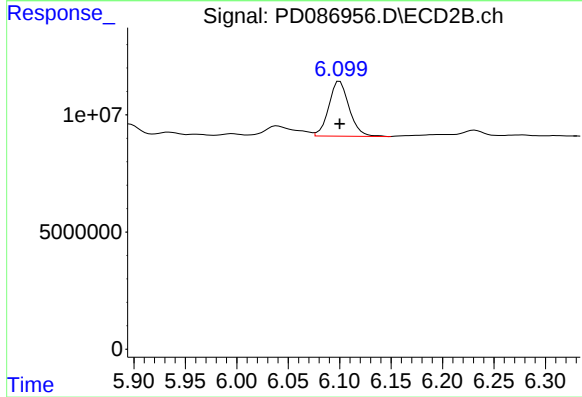

#27 Chlordane-5


R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 32276895
Conc: 50.37 ng/ml

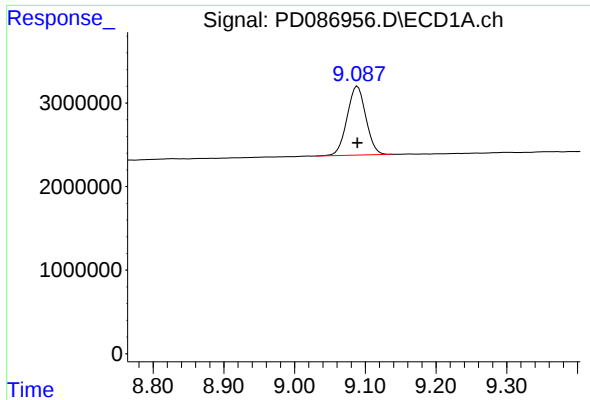

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 15210384
Conc: 4.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

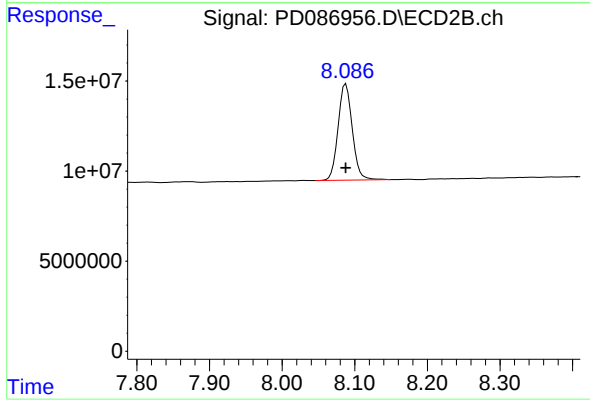

#28 Decachlorobiphenyl

R.T.: 8.088 min
Delta R.T.: 0.000 min
Response: 72619775
Conc: 5.26 ng/ml