

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112822\
 Data File : PD073236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2022 03:50
 Operator : AR\AJ
 Sample : PB149271BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS271

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/29/2022
 Supervised By :Ankita Jodhani 11/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 04:26:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	43555088	1240.3E6	18.163	18.987
27)	SA Decachlor...	7.826	8.908	76432554	517.5E6	33.496	34.968
Target Compounds							
2)	A alpha-BHC	3.200	3.922	13916305	399.5E6	3.802	4.581
3)	MA gamma-BHC...	3.530	4.255	13679273	330.5E6	4.122	4.871
4)	MA Heptachlor	3.862	4.822	13842750	219.3E6	4.144	4.775
5)	MB Aldrin	4.140	5.160	13841112	194.7E6	4.107m	4.847
6)	B beta-BHC	3.832	4.470	6716407	117.6E6	4.183	4.400m
7)	B delta-BHC	4.061	4.714	13773216	254.8E6	3.790	4.683
8)	B Heptachlo...	4.645	5.591	13164779	163.6E6	4.237	4.840m
9)	A Endosulfan I	5.014	5.977	12276757	130.7E6	4.344	4.493
10)	B trans-Chl...	4.894	5.846	13354905	140.0E6	4.333	4.432
11)	B cis-Chlor...	4.957	5.921	13747972	139.4E6	4.391	4.390
12)	B 4,4'-DDE	5.145	6.095	23795423	256.9E6	7.954	8.558
13)	MA Dieldrin	5.280	6.253	24669765	280.8E6	8.053	9.316
14)	MA Endrin	5.557	6.485	19623213	158.9E6	7.238	6.440
15)	B Endosulfa...	5.854	6.715	21166301	220.2E6	7.860m	9.116
16)	A 4,4'-DDD	5.704	6.620	19741838	221.2E6	8.194	9.651
17)	MA 4,4'-DDT	5.952	6.927	15302204	169.7E6	6.841	7.900
18)	B Endrin al...	6.037	6.846	17165628	165.6E6	7.948	8.741
19)	B Endosulfa...	6.260	7.079	18279329	169.7E6	7.285	8.161
20)	A Methoxychlor	6.535	7.407	46442832	383.6E6	37.081	41.109
21)	B Endrin ke...	6.770	7.569	22575591	197.3E6	7.734	8.838

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112822\
Data File : PD073236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2022 03:50
Operator : AR\AJ
Sample : PB149271BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 04:26:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD11722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

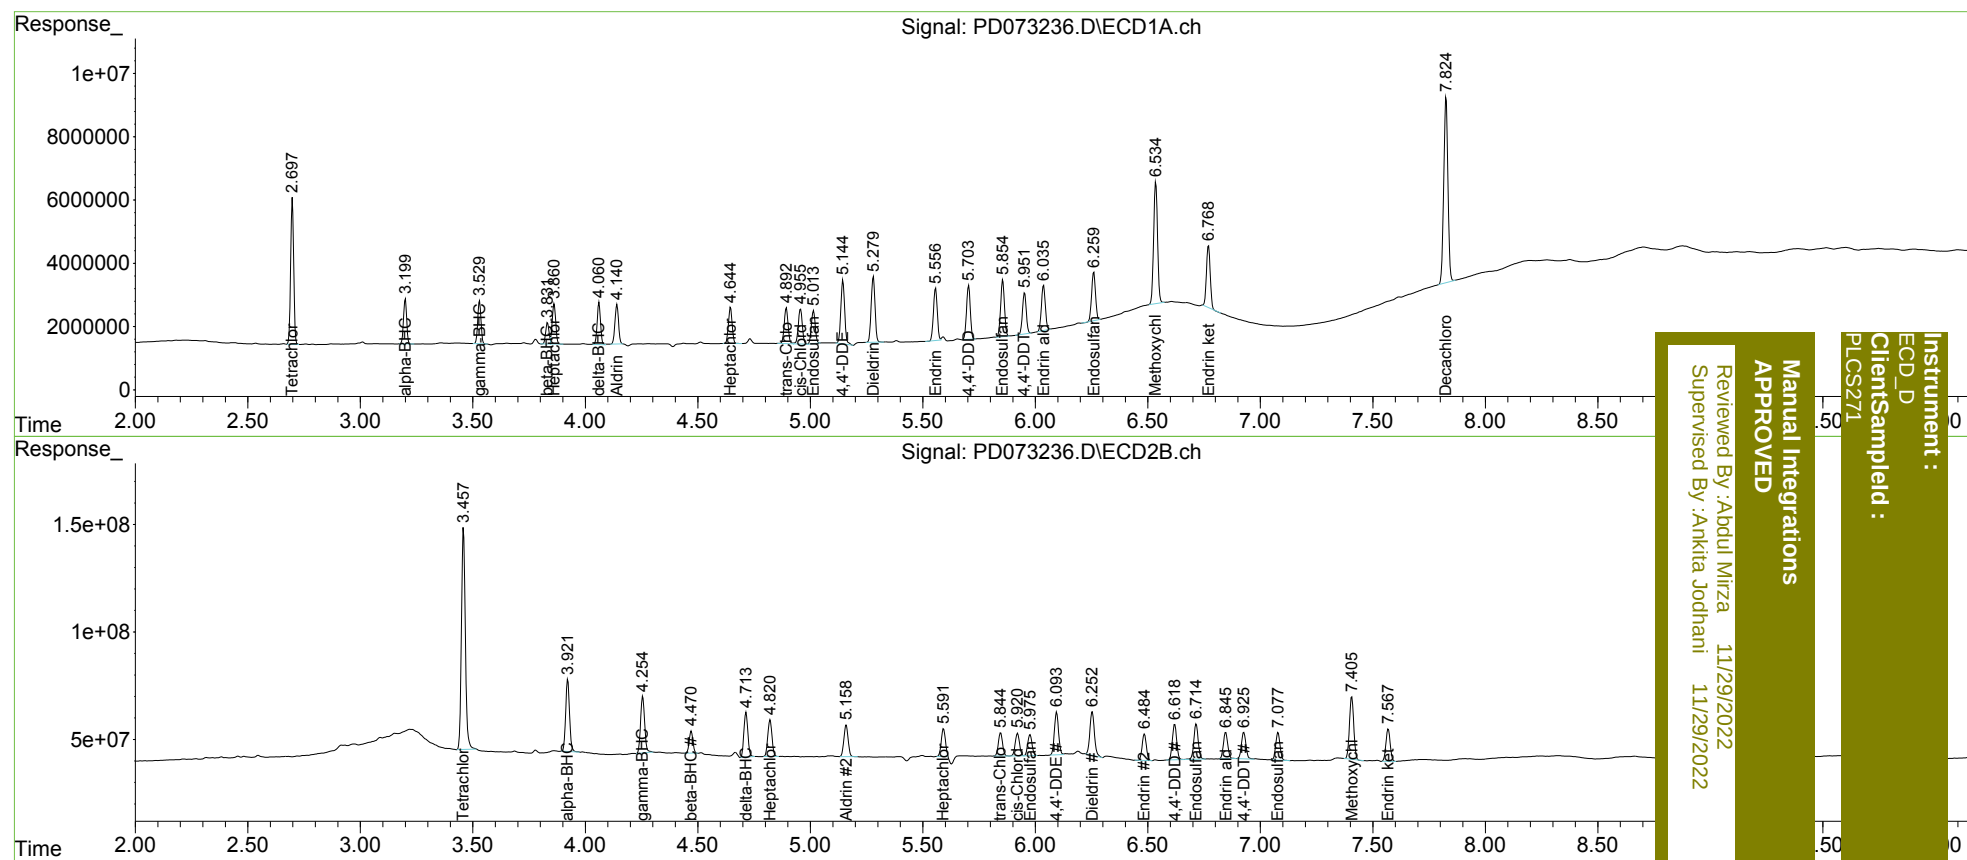

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/29/2022
Supervised By: Ankita Jodhani 11/29/2022

Instrument :
ECD_D
Client Sampled :
PLCS271