

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112822\
 Data File : PD073238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2022 04:17
 Operator : AR\AJ
 Sample : N5658-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQT3MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/29/2022
 Supervised By :Ankita Jodhani 11/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 05:22:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.459	31081694	874.2E6	12.962	13.382
27)	SA Decachlor...	7.825	8.907	50525761	378.8E6	22.142	25.596
Target Compounds							
2)	A alpha-BHC	3.201	3.922	172.7E6	3276.3E6	47.186	37.570m
3)	MA gamma-BHC...	3.531	4.256	157.5E6	2680.6E6	47.455	39.508
4)	MA Heptachlor	3.862	4.822	159.6E6	1868.7E6	47.770	40.694
5)	MB Aldrin	4.141	5.160	157.8E6	1607.7E6	46.824	40.032
6)	B beta-BHC	3.833	4.471	62792333	1127.6E6	39.110	42.203
7)	B delta-BHC	4.061	4.715	152.5E6	2037.8E6	41.970	37.452
8)	B Heptachlo...	4.645	5.592	128.5E6	1361.9E6	41.369	40.290
9)	A Endosulfan I	5.014	5.976	111.1E6	1103.3E6	39.321	37.929
10)	B trans-Chl...	4.894	5.846	326.3E6	2583.1E6	105.861	81.768
11)	B cis-Chlor...	4.957	5.921	155.0E6	1556.8E6	49.501	49.037
12)	B 4,4'-DDE	5.145	6.094	277.5E6	2400.2E6	92.760	79.947
13)	MA Dieldrin	5.280	6.253	360.8E6	3048.6E6	117.770	101.138
14)	MA Endrin	5.557	6.485	257.1E6	1934.7E6	94.836	78.433
15)	B Endosulfa...	5.854	6.715	227.8E6	1760.5E6	84.573m	72.877
16)	A 4,4'-DDD	5.704	6.618	203.7E6	1957.8E6	84.551	85.425m
17)	MA 4,4'-DDT	5.951	6.927	253.7E6	1975.0E6	113.413	91.958
18)	B Endrin al...	6.037	6.846	154.2E6	1207.7E6	71.415	63.751
19)	B Endosulfa...	6.260	7.077	220.3E6	1839.0E6	87.784	88.437m
20)	A Methoxychlor	6.535	7.406	540.5E6	3861.1E6	431.526	413.814
21)	B Endrin ke...	6.770	7.569	231.6E6	1695.0E6	79.353	75.912

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112822\
Data File : PD073238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2022 04:17
Operator : AR\AJ
Sample : N5658-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 05:22:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

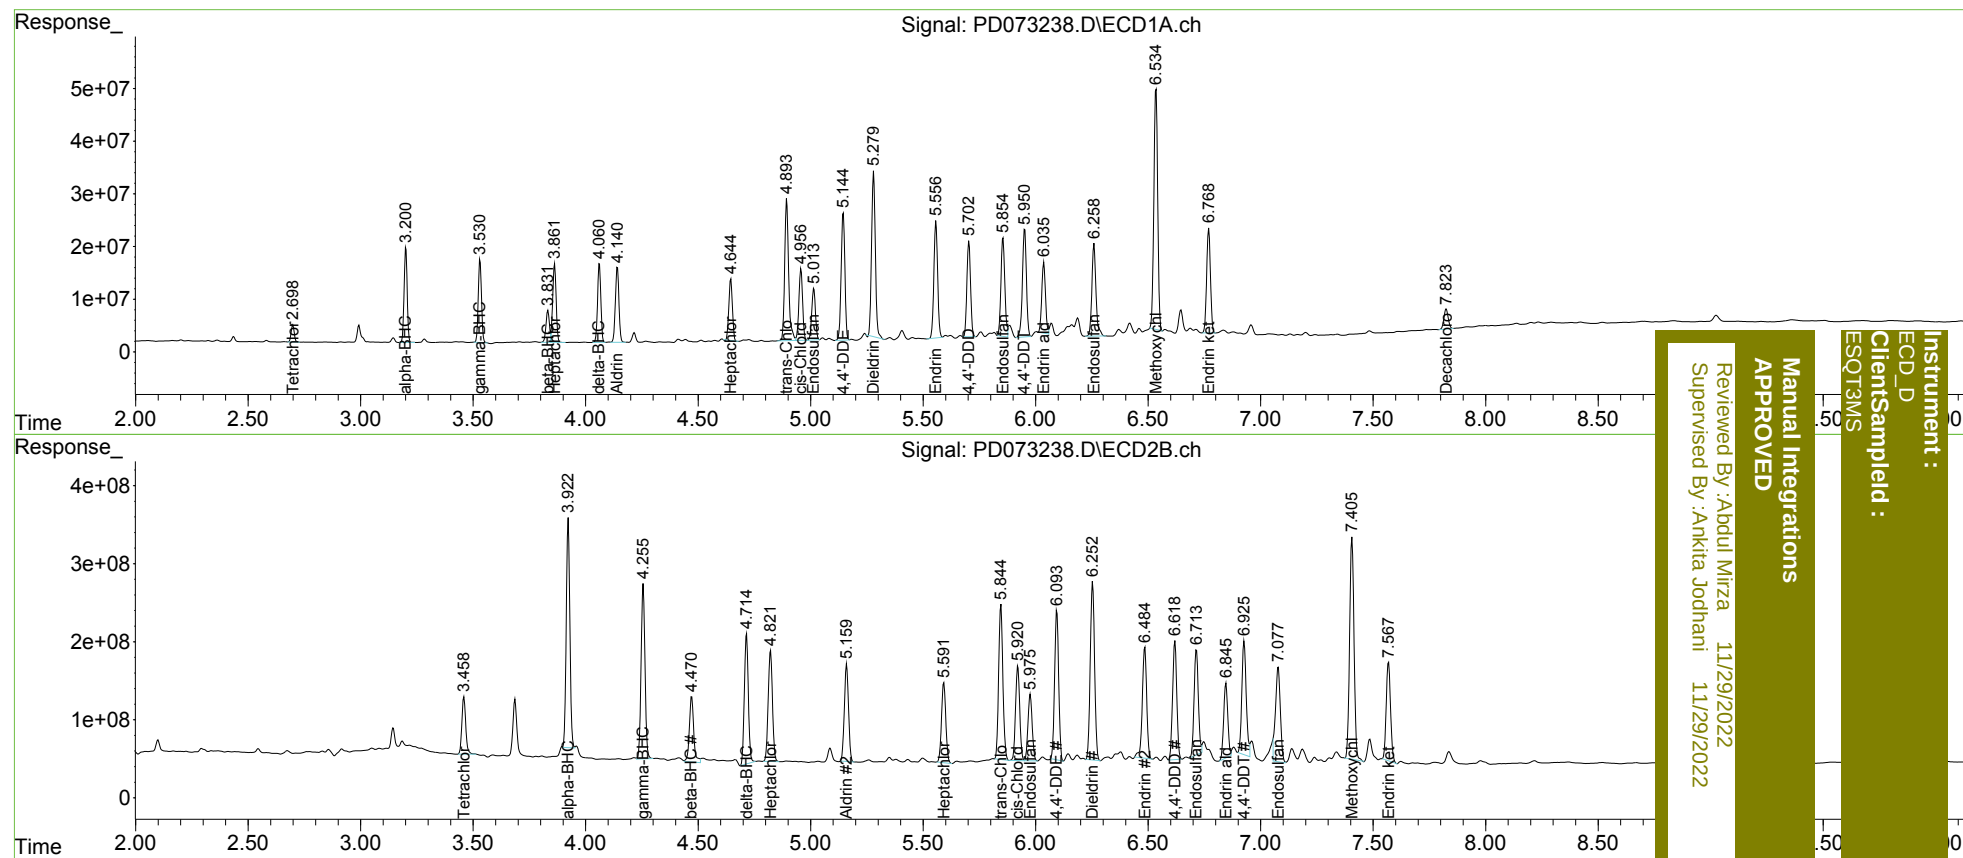

Instrument :
ECD_D
ClientSampled :
ESQ3MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/29/2022
Supervised By: Ankita Jodhani 11/29/2022