

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
 Data File : PD067114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2021 18:38
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 05:16:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:16:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	3.967	11546445	45839313	5.281	5.699
27)	SA Decachlor...	8.162	9.022	13349414	58388339	11.872	11.385
Target Compounds							
2)	A alpha-BHC	3.873	4.360	16001263	59123391	4.865	5.543
3)	MA gamma-BHC...	4.154	4.645	16898234	55605331	5.396	5.561
4)	MA Heptachlor	4.447	5.145	16185939	52414057	5.025	5.632
9)	A Endosulfan I	5.469	6.194	13953553	39855130	5.231	5.424
13)	MA Dieldrin	5.711	6.452	28783342	80383240	9.889	10.691
14)	MA Endrin	5.969	6.671	23124509	58898426	10.080	9.855
16)	A 4,4'-DDD	6.094	6.797	21095173	63334573	9.858	10.711
17)	MA 4,4'-DDT	6.333	7.095	20834874	61762603	9.708	10.636
20)	A Methoxychlor	6.880	7.557	54245786	159.7E6	54.388	56.887


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
Data File : PD067114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2021 18:38
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 05:16:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:16:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

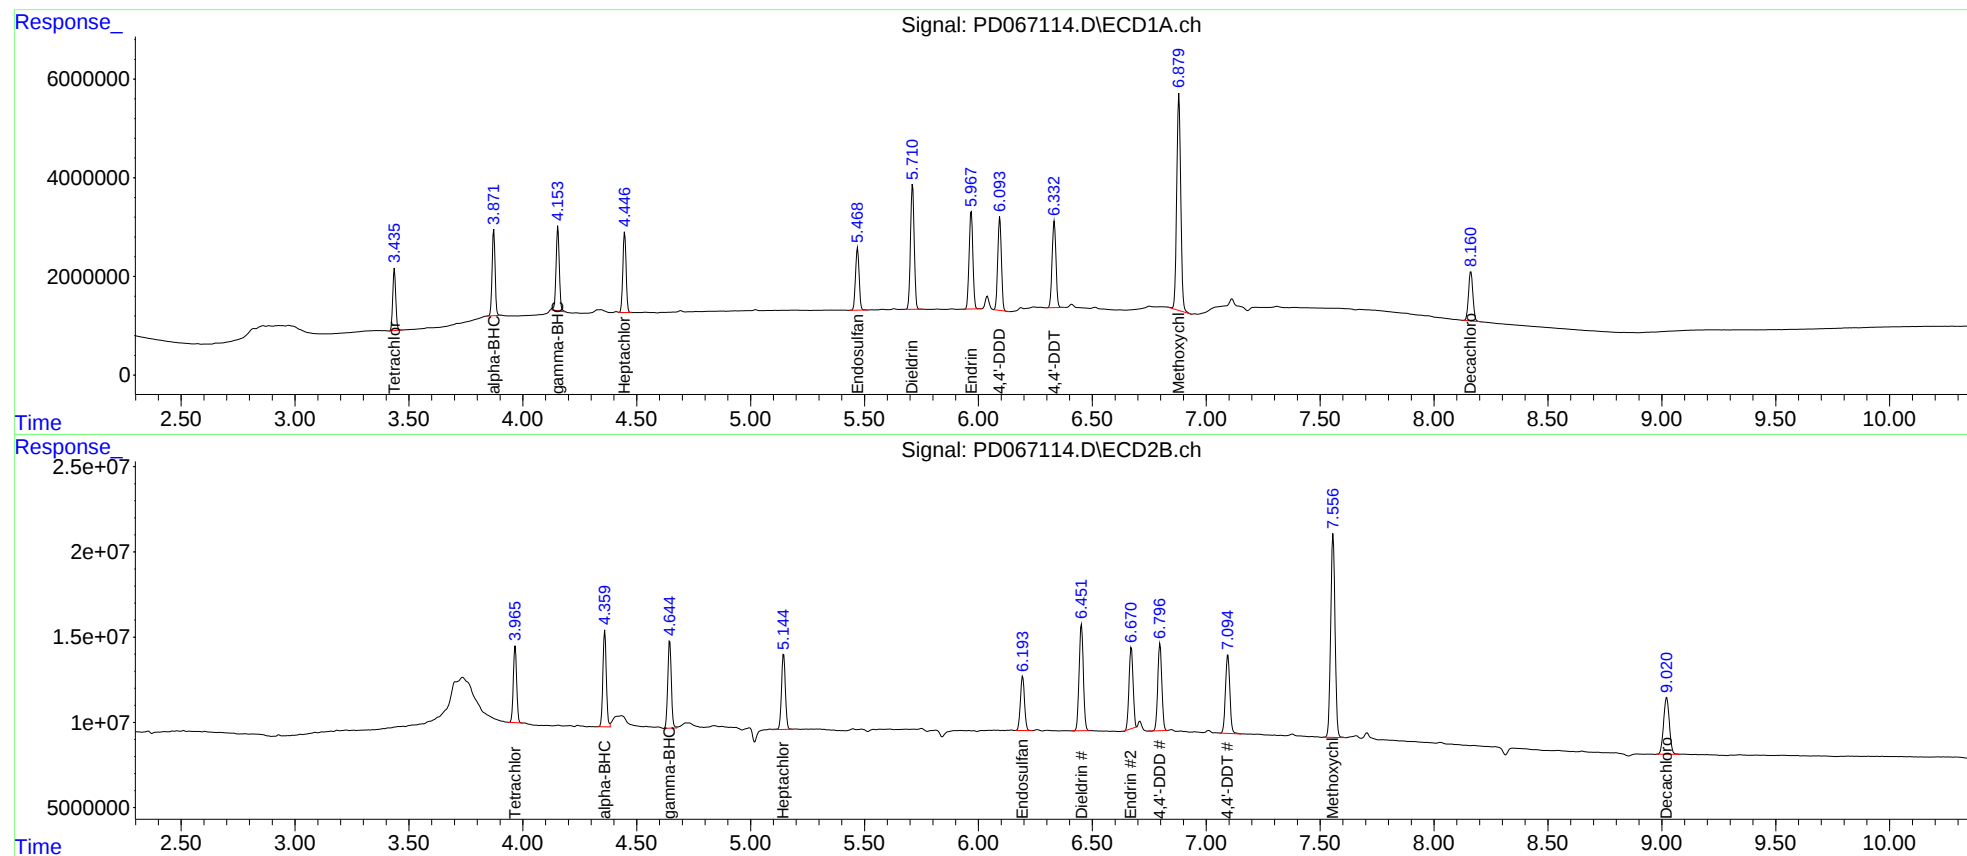

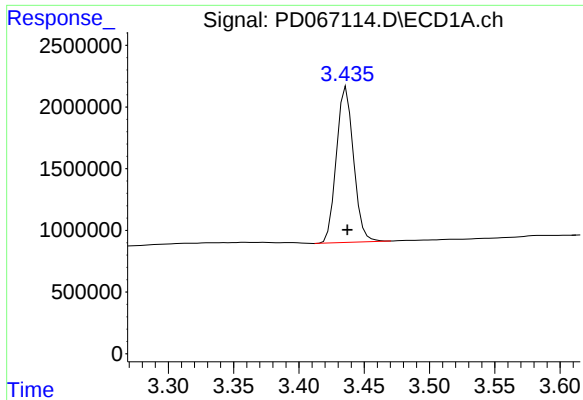


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 11546445
Conc: 5.28 ng/ml

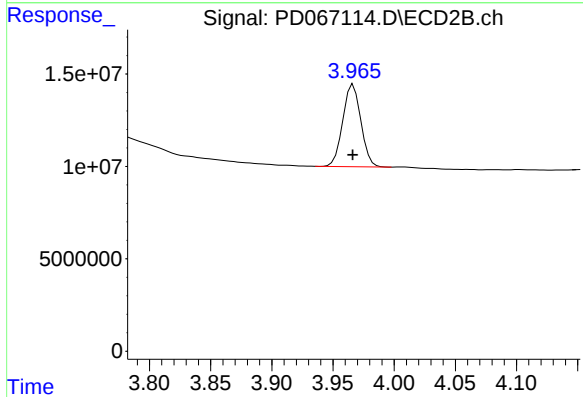


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 45839313
Conc: 5.70 ng/ml

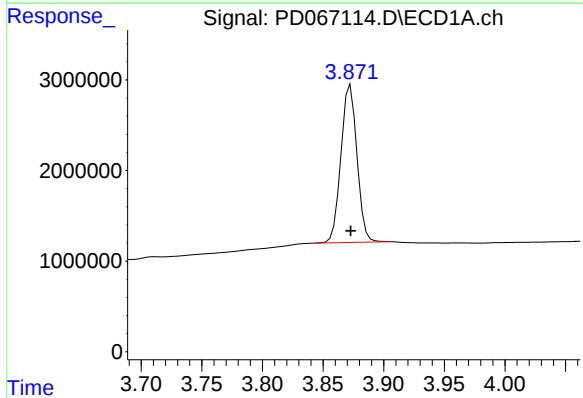


#2 alpha-BHC

R.T.: 3.873 min
Delta R.T.: 0.000 min
Response: 16001263
Conc: 4.86 ng/ml

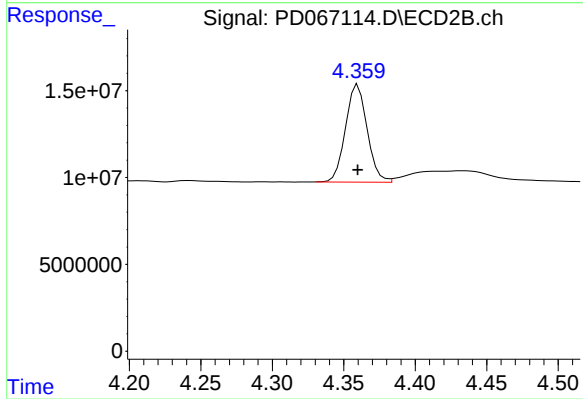


#2 alpha-BHC

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 59123391
Conc: 5.54 ng/ml

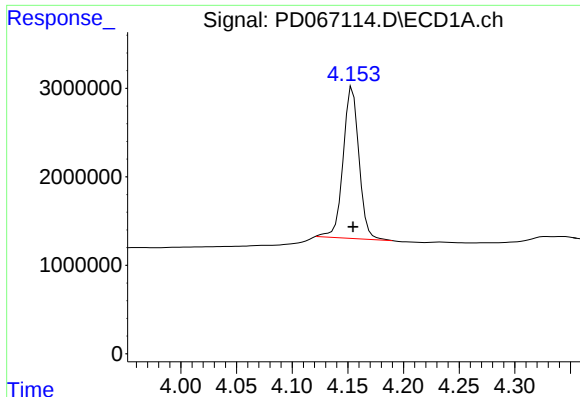


#3 gamma-BHC (Lindane)

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 16898234
Conc: 5.40 ng/ml

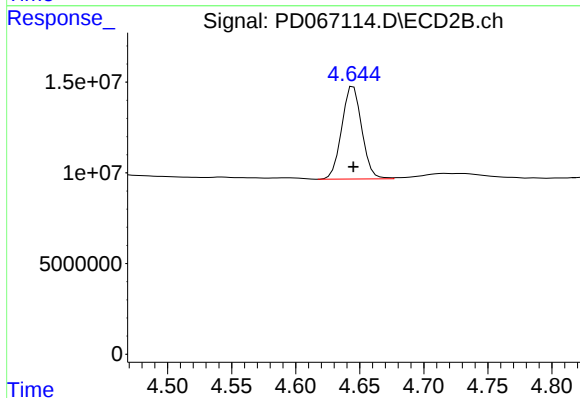


#3 gamma-BHC (Lindane)

R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 55605331
Conc: 5.56 ng/ml

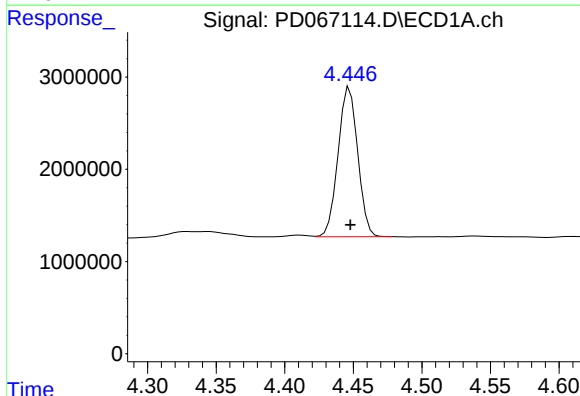


#4 Heptachlor

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 16185939
Conc: 5.03 ng/ml

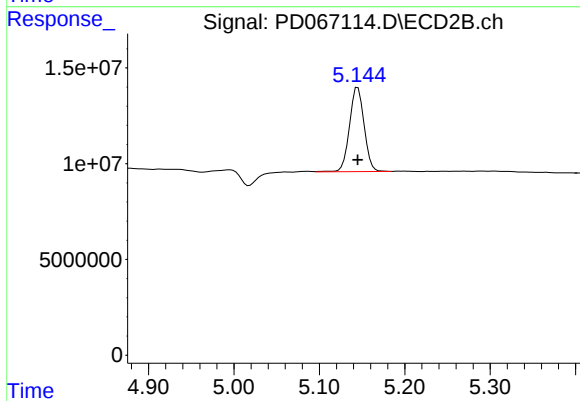


#4 Heptachlor

R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 52414057
Conc: 5.63 ng/ml

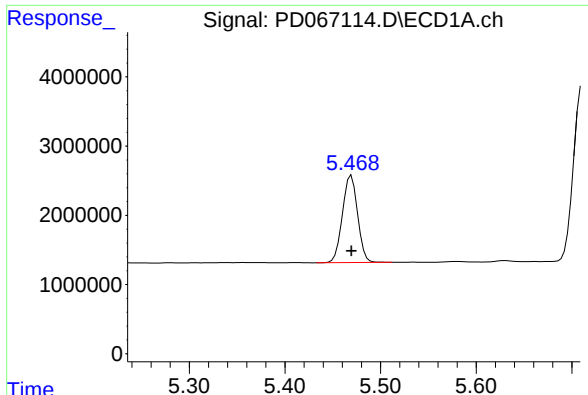


#9 Endosulfan I

R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 13953553
Conc: 5.23 ng/ml

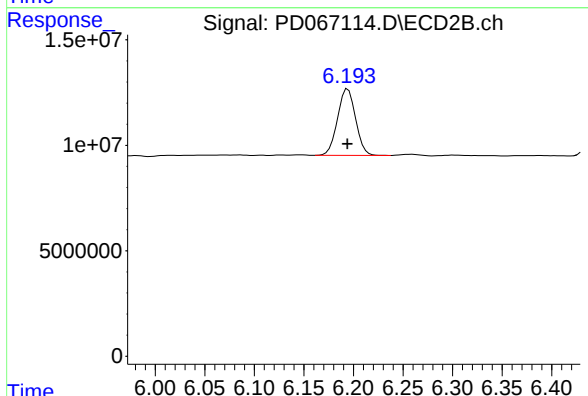


#9 Endosulfan I

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 39855130
Conc: 5.42 ng/ml

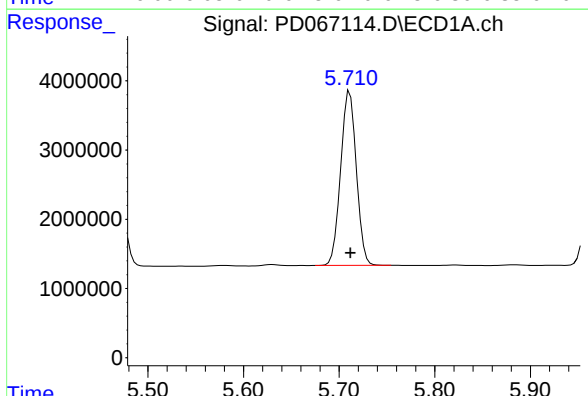


#13 Dieldrin

R.T.: 5.711 min
Delta R.T.: 0.000 min
Response: 28783342
Conc: 9.89 ng/ml

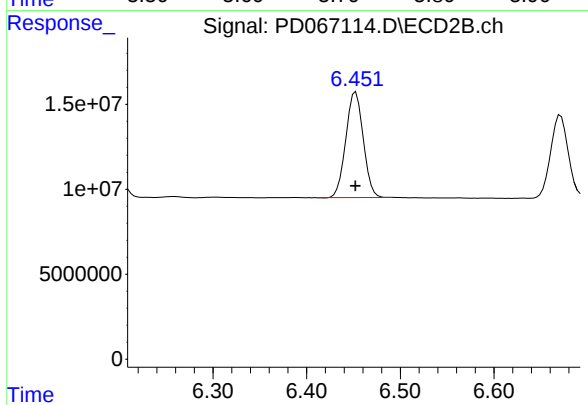


#13 Dieldrin

R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 80383240
Conc: 10.69 ng/ml

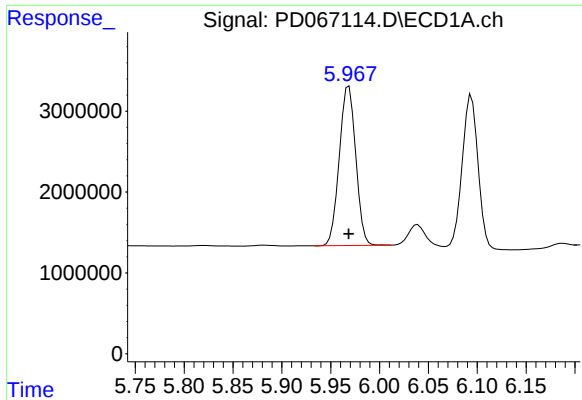


#14 Endrin

R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 23124509
Conc: 10.08 ng/ml

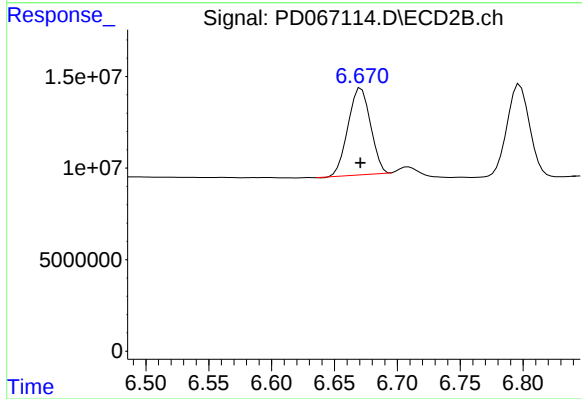


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 58898426
Conc: 9.85 ng/ml

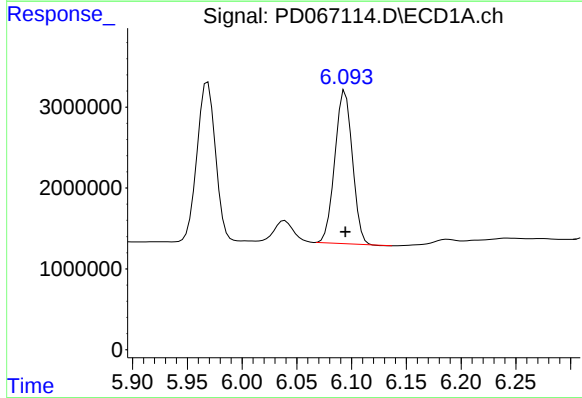


#16 4,4'-DDD

R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 21095173
Conc: 9.86 ng/ml

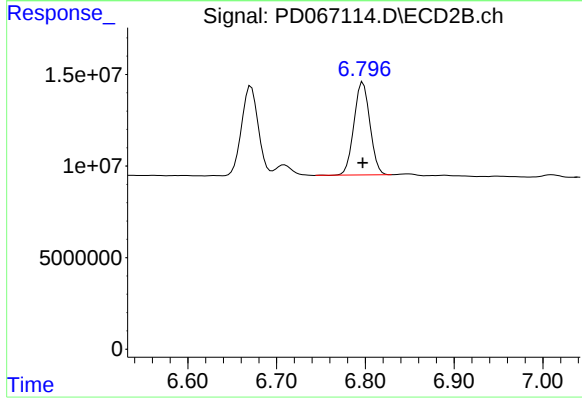


#16 4,4'-DDD

R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 63334573
Conc: 10.71 ng/ml

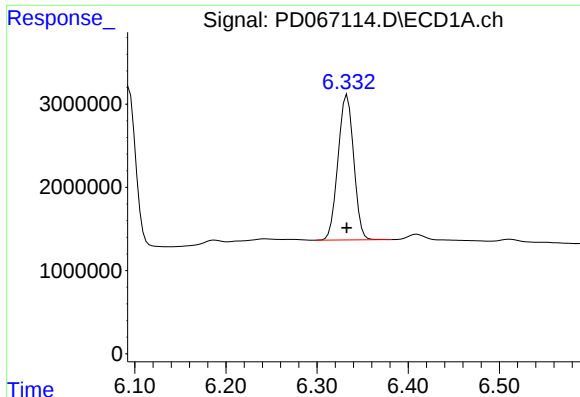


#17 4,4'-DDT

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 20834874
Conc: 9.71 ng/ml

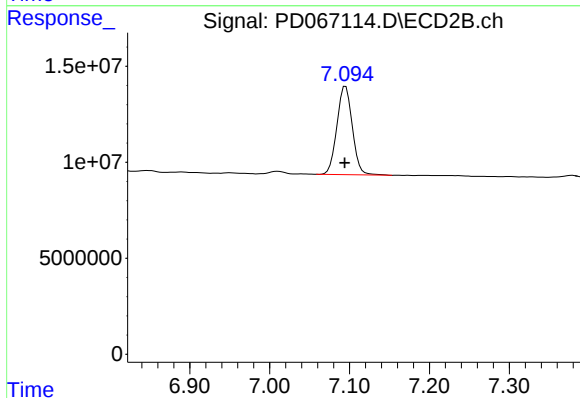


#17 4,4'-DDT

R.T.: 7.095 min
Delta R.T.: 0.001 min
Response: 61762603
Conc: 10.64 ng/ml

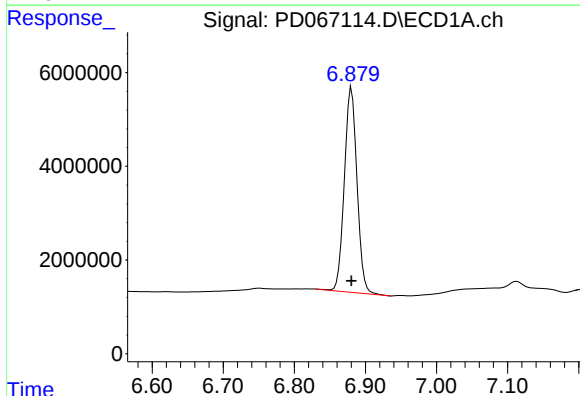


#20 Methoxychlor

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 54245786
Conc: 54.39 ng/ml

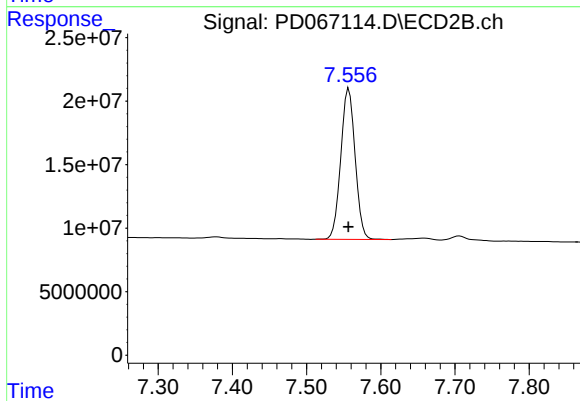


#20 Methoxychlor

R.T.: 7.557 min
Delta R.T.: 0.000 min
Response: 159746747
Conc: 56.89 ng/ml

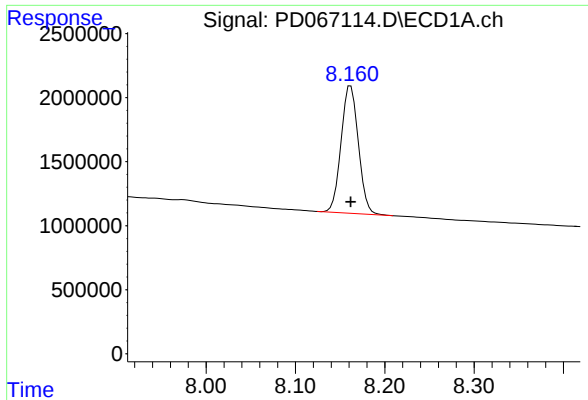

#27 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 13349414
Conc: 11.87 ng/ml

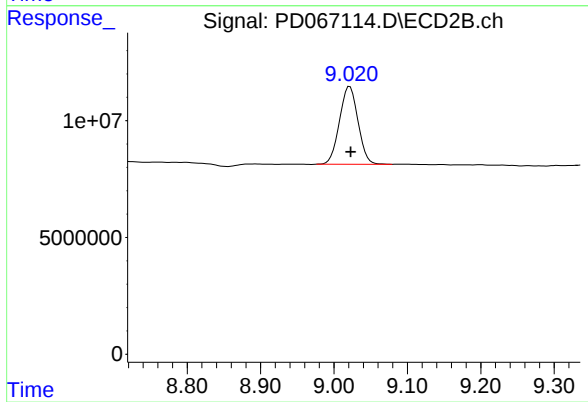

#27 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.001 min
Response: 58388339
Conc: 11.38 ng/ml