

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
 Data File : PD067116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2021 19:05
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 05:16:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:16:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	3.967	22901866	87671929	10.474	10.899
27)	SA Decachlor...	8.162	9.022	24729045	110.0E6	21.992	21.457
Target Compounds							
2)	A alpha-BHC	3.873	4.360	32926055	114.3E6	10.011	10.719
3)	MA gamma-BHC...	4.154	4.645	32783472	106.9E6	10.469	10.689
4)	MA Heptachlor	4.448	5.145	32694763	99571806	10.151	10.700
9)	A Endosulfan I	5.469	6.194	27492941	77975251	10.308	10.611
13)	MA Dieldrin	5.712	6.453	58440222	158.0E6	20.077	21.016
14)	MA Endrin	5.969	6.671	47648351	124.7E6	20.771	20.861
16)	A 4,4'-DDD	6.094	6.797	43310951	124.7E6	20.239	21.087
17)	MA 4,4'-DDT	6.333	7.095	42692614	121.1E6	19.893	20.848
20)	A Methoxychlor	6.881	7.557	104.9E6	304.2E6	105.203	108.315


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
Data File : PD067116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2021 19:05
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 05:16:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:16:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

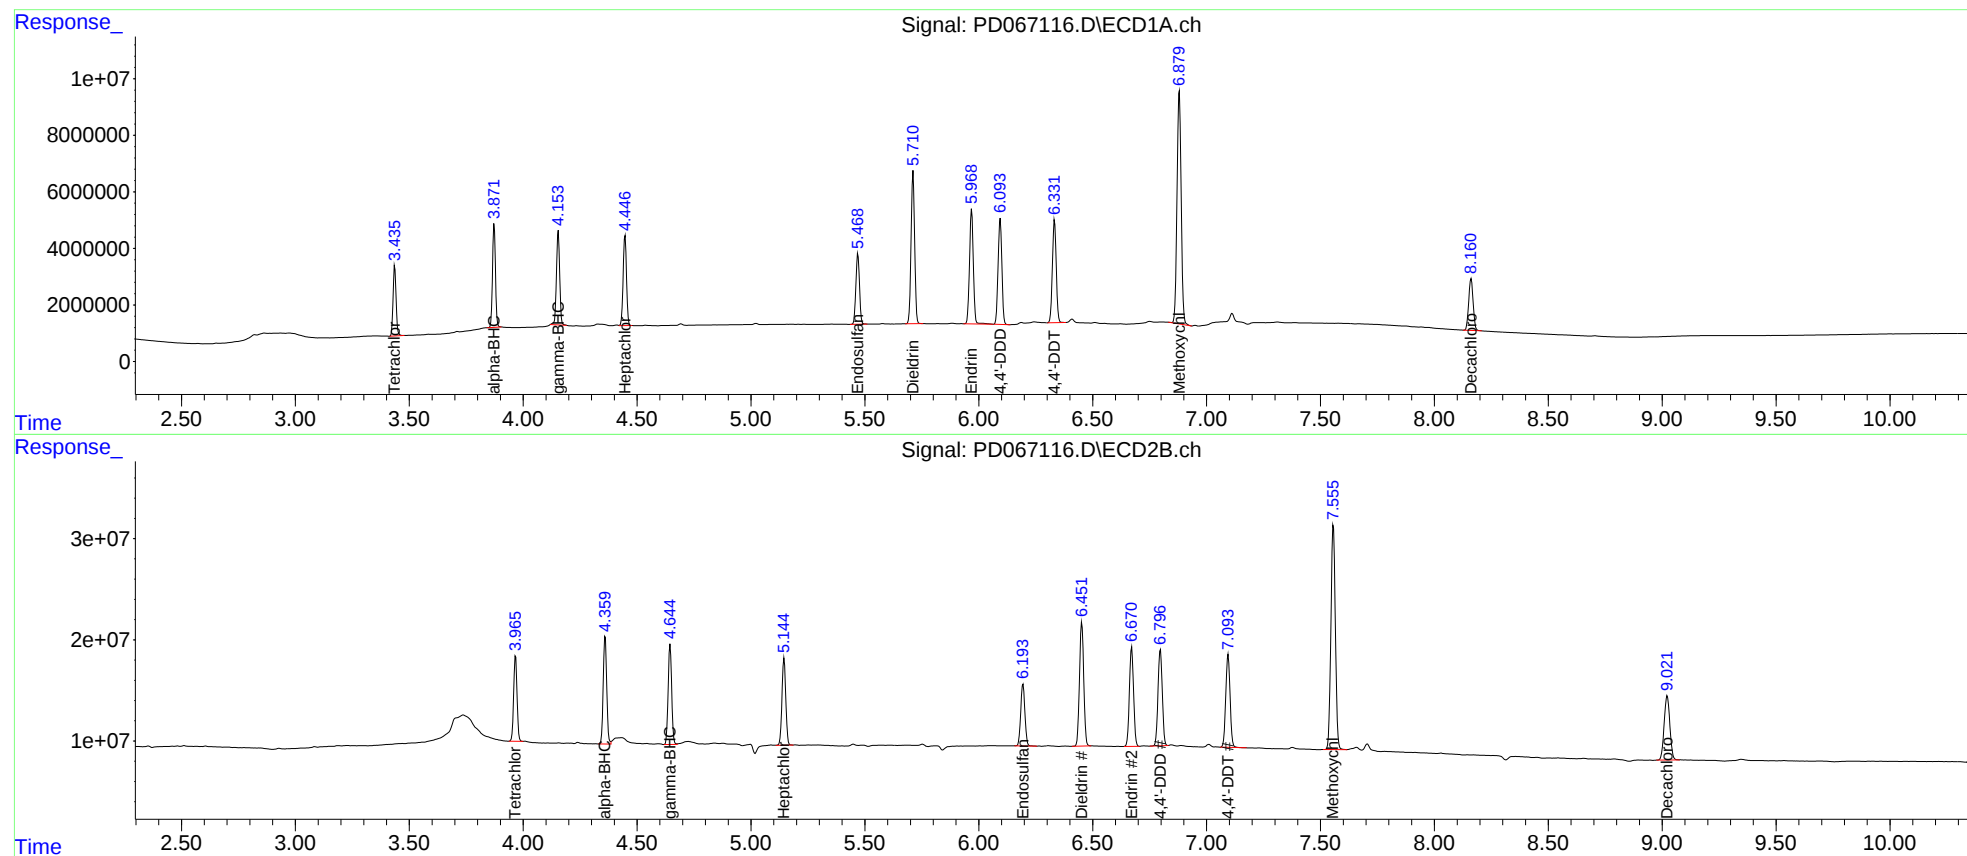

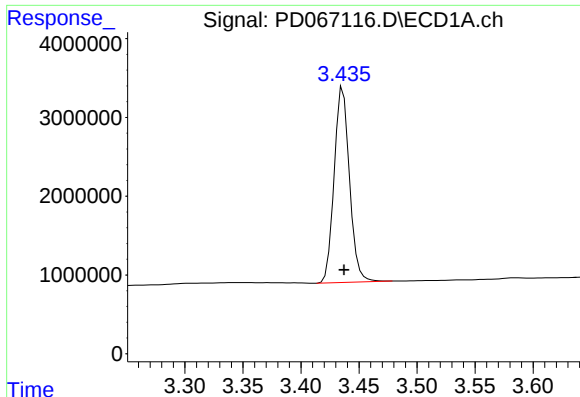


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 22901866
Conc: 10.47 ng/ml

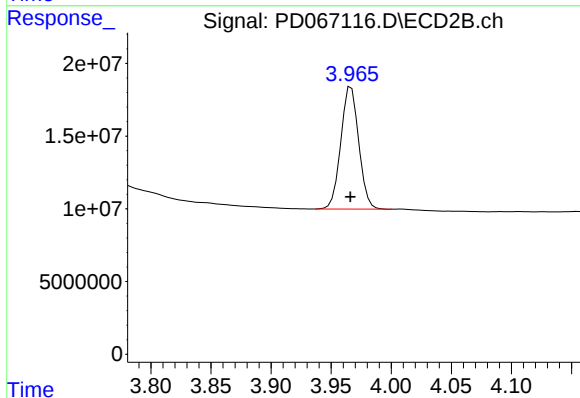


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 87671929
Conc: 10.90 ng/ml

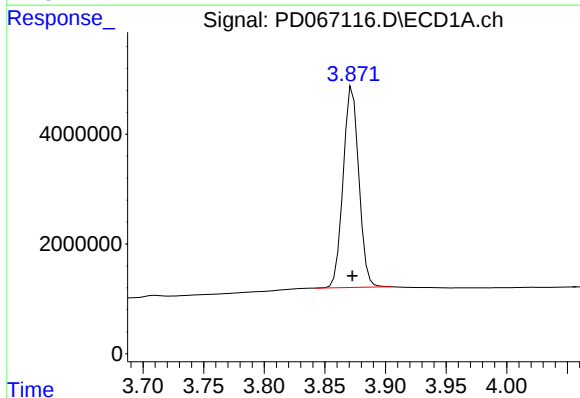


#2 alpha-BHC

R.T.: 3.873 min
Delta R.T.: 0.000 min
Response: 32926055
Conc: 10.01 ng/ml

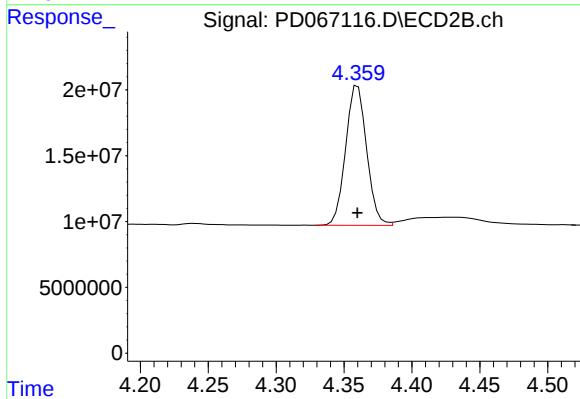


#2 alpha-BHC

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 114337810
Conc: 10.72 ng/ml

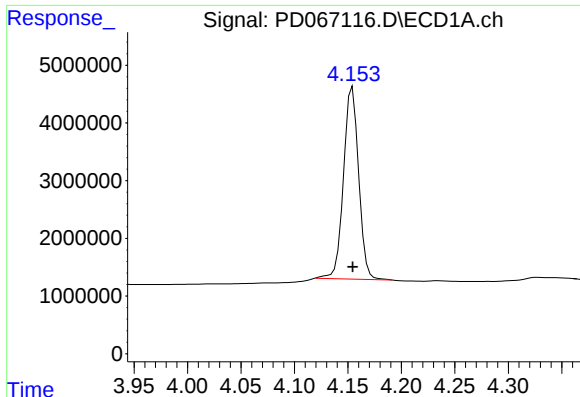


#3 gamma-BHC (Lindane)

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 32783472
Conc: 10.47 ng/ml

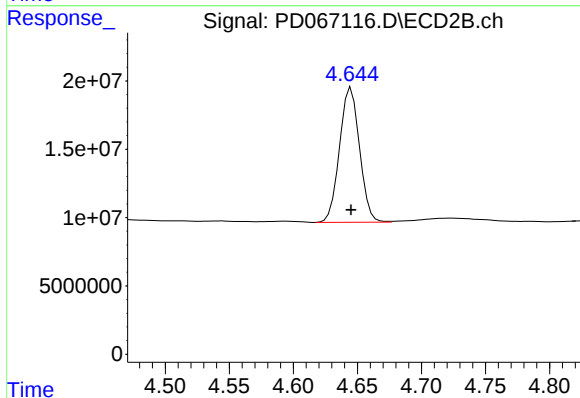


#3 gamma-BHC (Lindane)

R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 106881487
Conc: 10.69 ng/ml

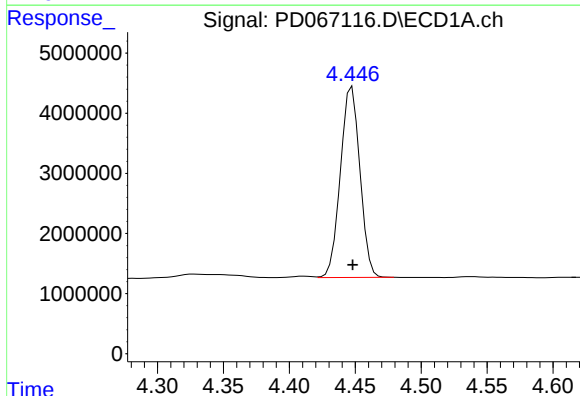


#4 Heptachlor

R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 32694763
Conc: 10.15 ng/ml

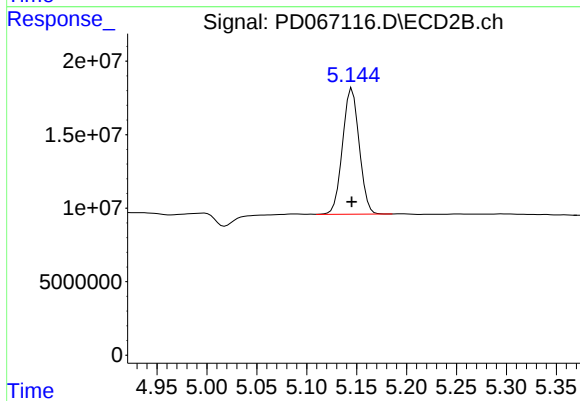


#4 Heptachlor

R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 99571806
Conc: 10.70 ng/ml

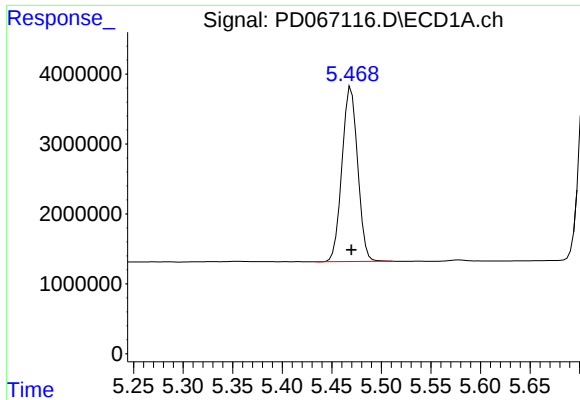


#9 Endosulfan I

R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 27492941
Conc: 10.31 ng/ml

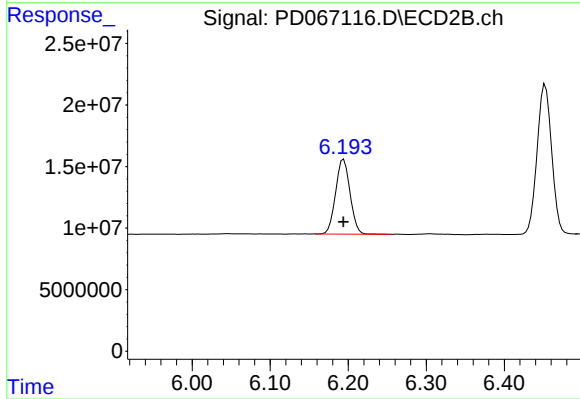


#9 Endosulfan I

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 77975251
Conc: 10.61 ng/ml

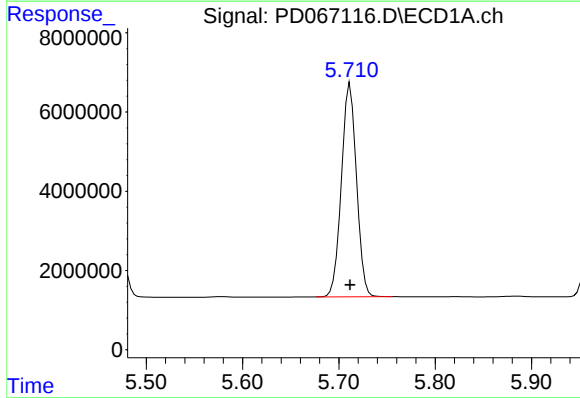


#13 Dieldrin

R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 58440222
Conc: 20.08 ng/ml

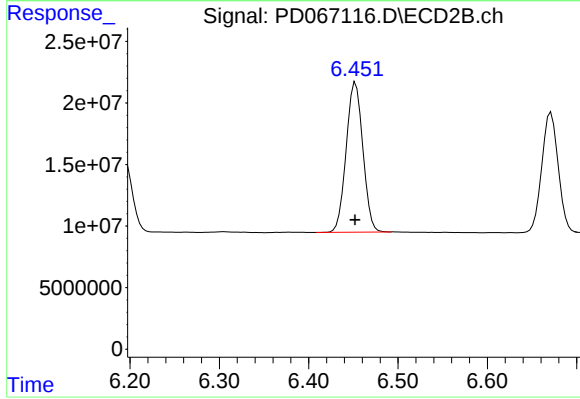


#13 Dieldrin

R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 158011291
Conc: 21.02 ng/ml

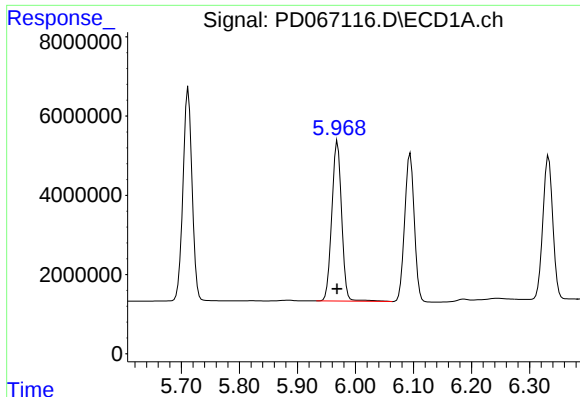


#14 Endrin

R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 47648351
Conc: 20.77 ng/ml

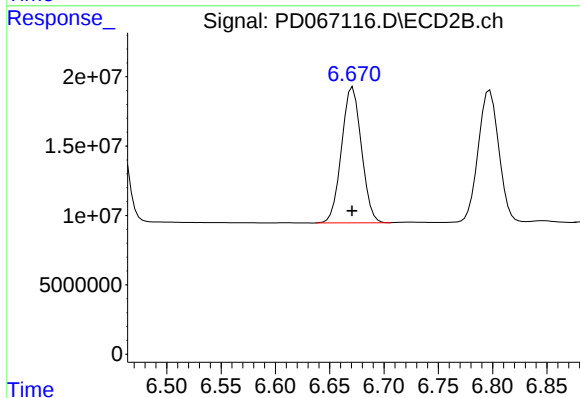


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 124683633
Conc: 20.86 ng/ml

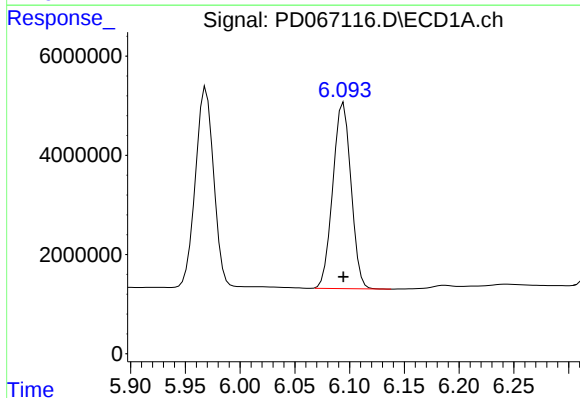


#16 4,4'-DDD

R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 43310951
Conc: 20.24 ng/ml

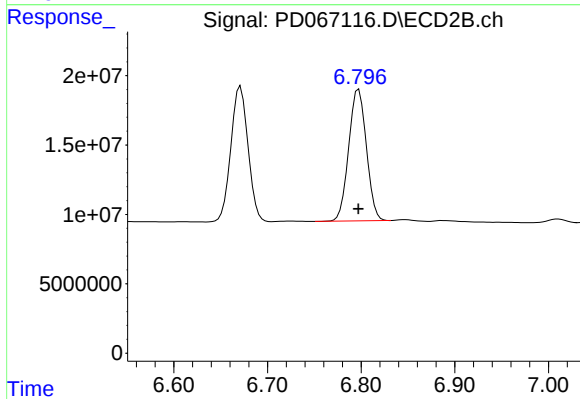


#16 4,4'-DDD

R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 124694481
Conc: 21.09 ng/ml

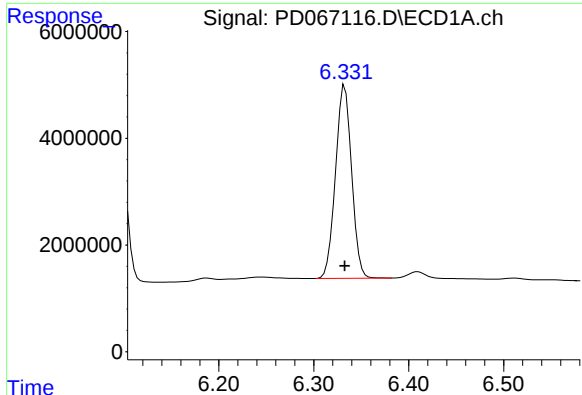


#17 4,4'-DDT

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 42692614
Conc: 19.89 ng/ml

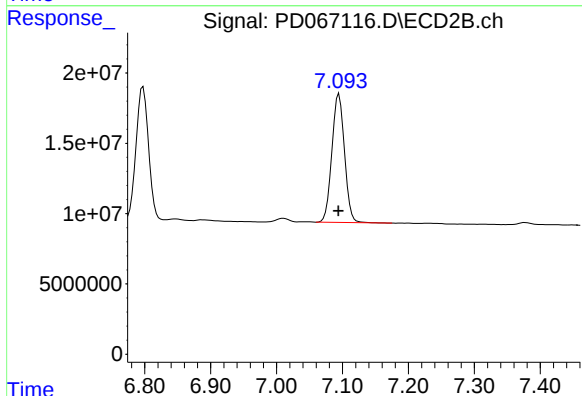


#17 4,4'-DDT

R.T.: 7.095 min
Delta R.T.: 0.000 min
Response: 121061485
Conc: 20.85 ng/ml

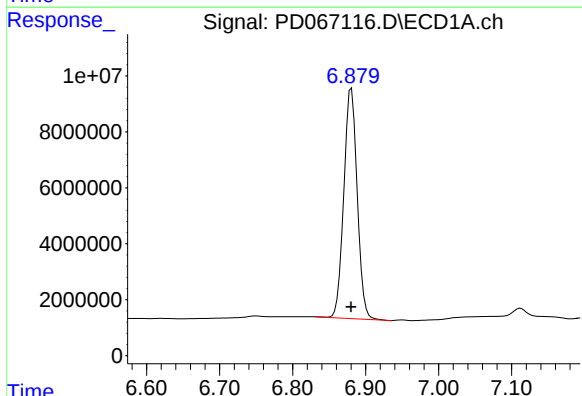


#20 Methoxychlor

R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 104928658
Conc: 105.20 ng/ml

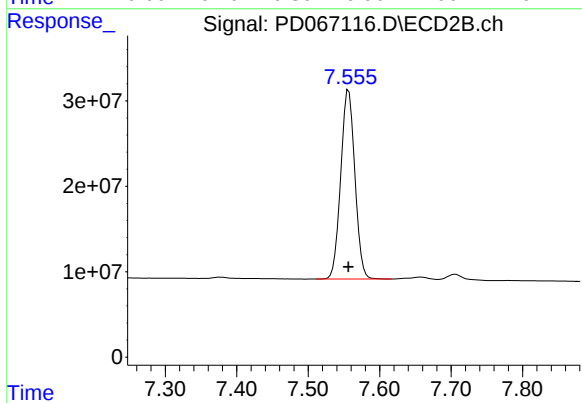


#20 Methoxychlor

R.T.: 7.557 min
Delta R.T.: 0.000 min
Response: 304163991
Conc: 108.32 ng/ml

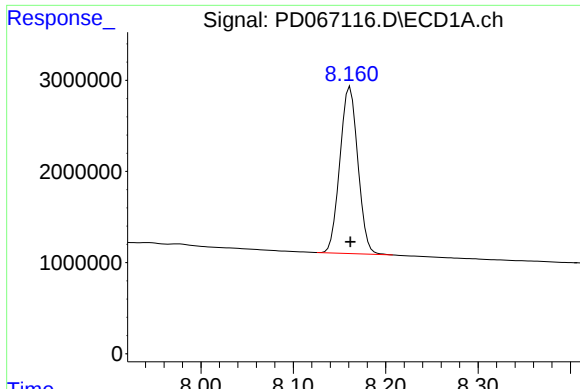

#27 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 24729045
Conc: 21.99 ng/ml

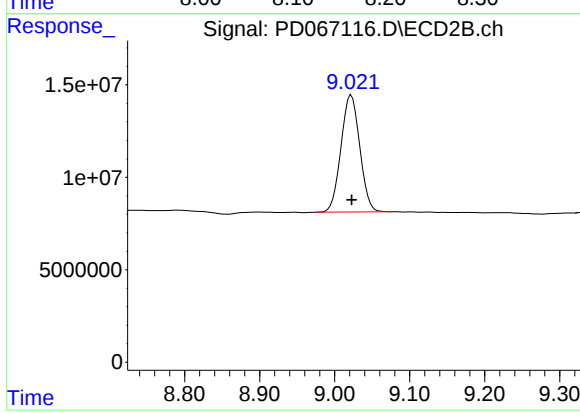

#27 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 110042080
Conc: 21.46 ng/ml