

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
 Data File : PD067118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2021 19:33
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 05:16:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:16:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.966	43730530	160.9E6	20.000	20.000
27)	SA Decachlor...	8.162	9.023	44977524	205.1E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.873	4.360	65782169	213.3E6	20.000	20.000
3)	MA gamma-BHC...	4.154	4.645	62630075	200.0E6	20.000	20.000
4)	MA Heptachlor	4.448	5.145	64416709	186.1E6	20.000	20.000
9)	A Endosulfan I	5.470	6.194	53345053	147.0E6	20.000	20.000
13)	MA Dieldrin	5.712	6.452	116.4E6	300.7E6	40.000	40.000
14)	MA Endrin	5.969	6.671	91761267	239.1E6	40.000	40.000
16)	A 4,4'-DDD	6.094	6.797	85597086	236.5E6	40.000	40.000
17)	MA 4,4'-DDT	6.333	7.094	85845344	232.3E6	40.000	40.000
20)	A Methoxychlor	6.880	7.556	199.5E6	561.6E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
Data File : PD067118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2021 19:33
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 05:16:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:16:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

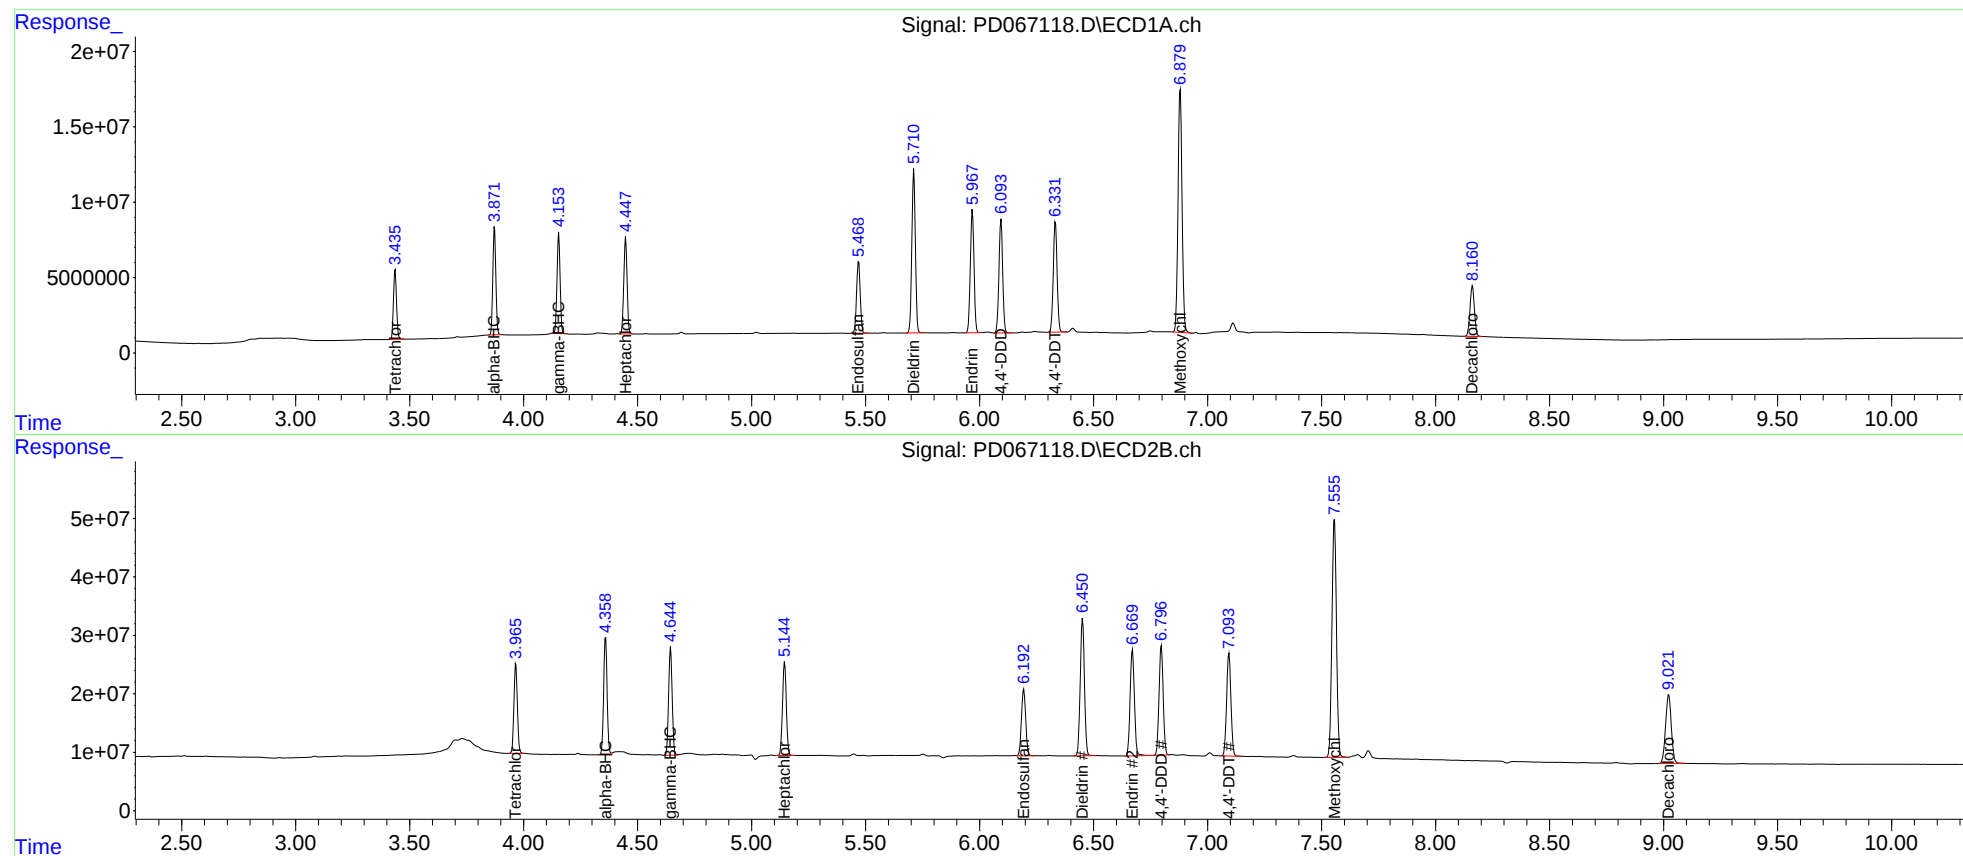

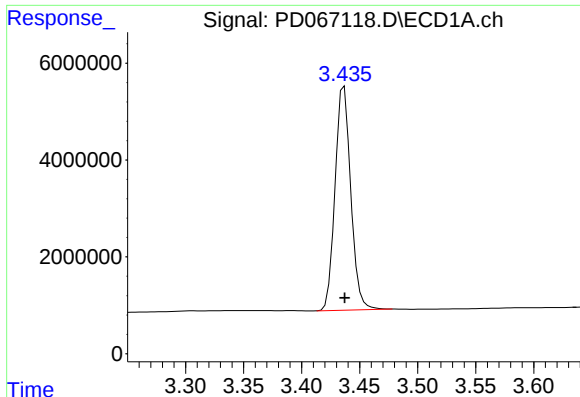


#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: 0.000 min
Response: 43730530
Conc: 20.00 ng/ml

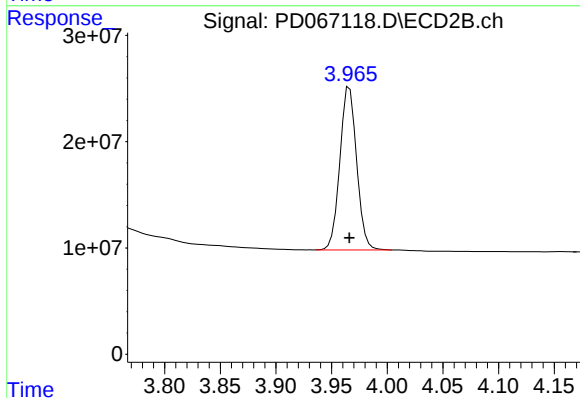


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 160876744
Conc: 20.00 ng/ml

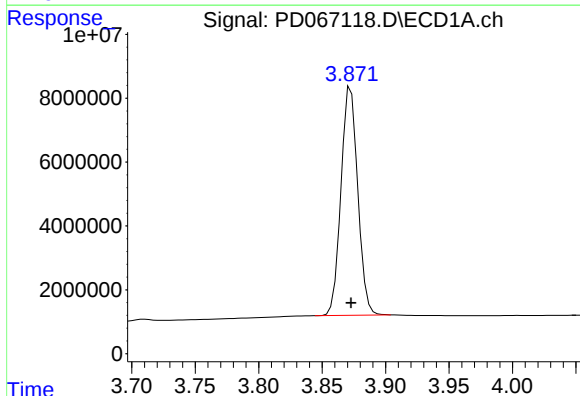


#2 alpha-BHC

R.T.: 3.873 min
Delta R.T.: 0.000 min
Response: 65782169
Conc: 20.00 ng/ml

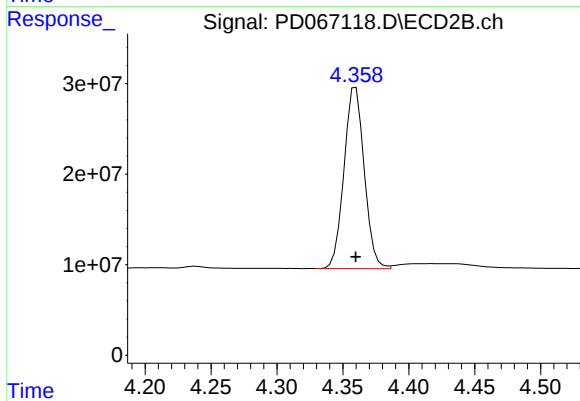


#2 alpha-BHC

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 213340681
Conc: 20.00 ng/ml

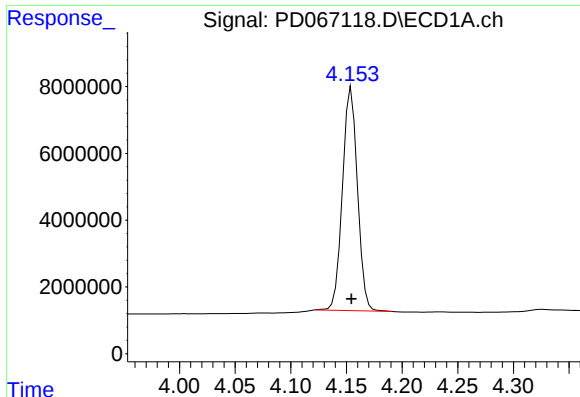


#3 gamma-BHC (Lindane)

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 62630075
Conc: 20.00 ng/ml

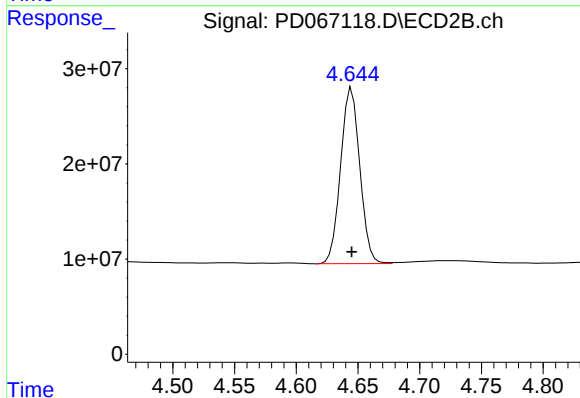


#3 gamma-BHC (Lindane)

R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 199989791
Conc: 20.00 ng/ml

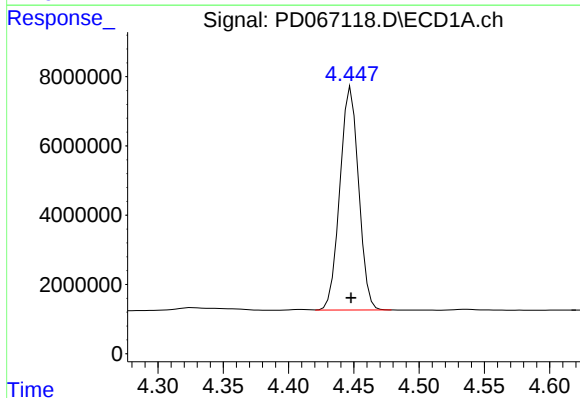


#4 Heptachlor

R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 64416709
Conc: 20.00 ng/ml

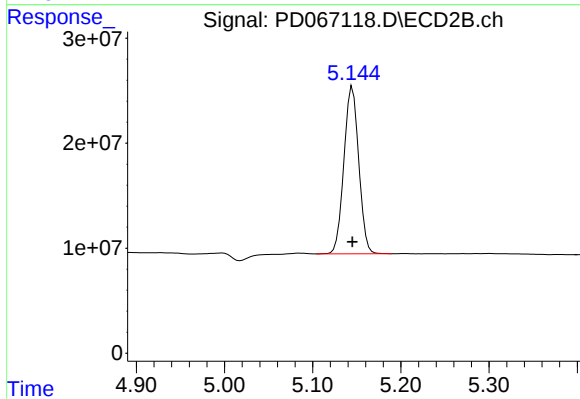


#4 Heptachlor

R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 186118358
Conc: 20.00 ng/ml

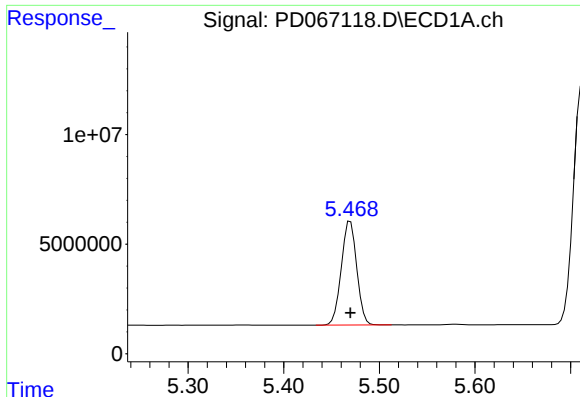


#9 Endosulfan I

R.T.: 5.470 min
Delta R.T.: 0.000 min
Response: 53345053
Conc: 20.00 ng/ml

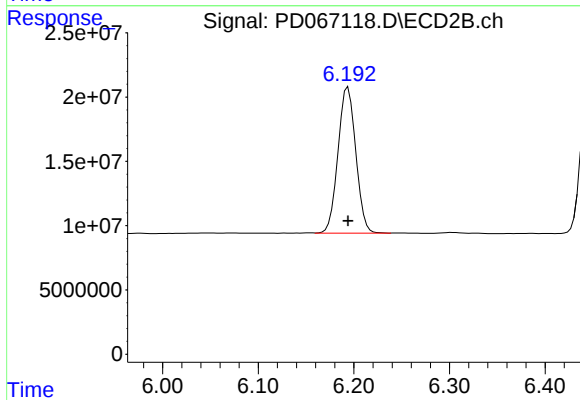


#9 Endosulfan I

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 146967882
Conc: 20.00 ng/ml

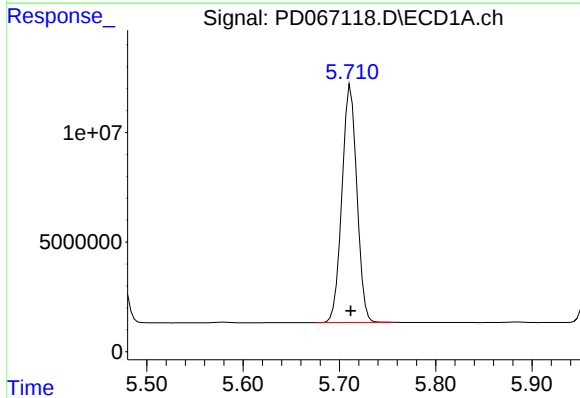


#13 Dieldrin

R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 116429602
Conc: 40.00 ng/ml

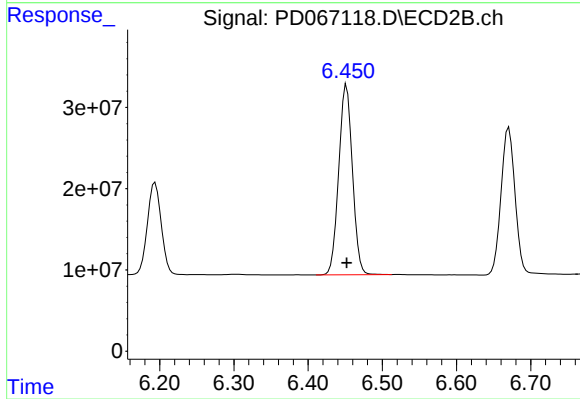


#13 Dieldrin

R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 300741553
Conc: 40.00 ng/ml

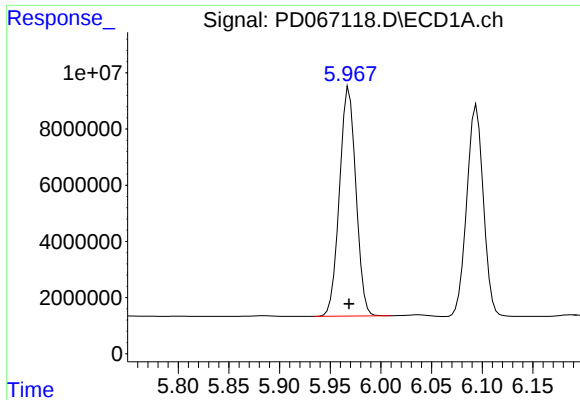


#14 Endrin

R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 91761267
Conc: 40.00 ng/ml

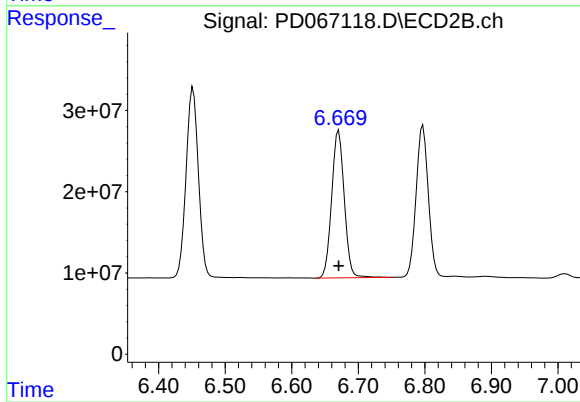


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 239071528
Conc: 40.00 ng/ml

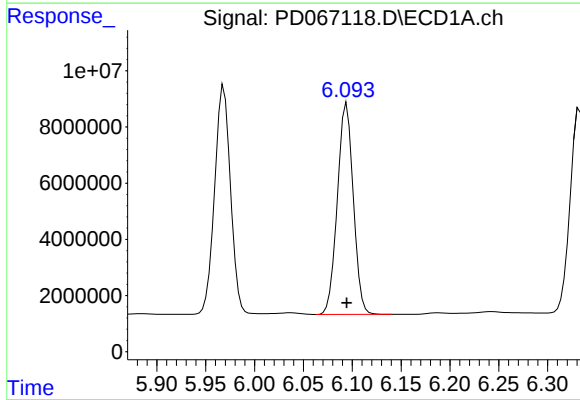


#16 4,4'-DDD

R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 85597086
Conc: 40.00 ng/ml

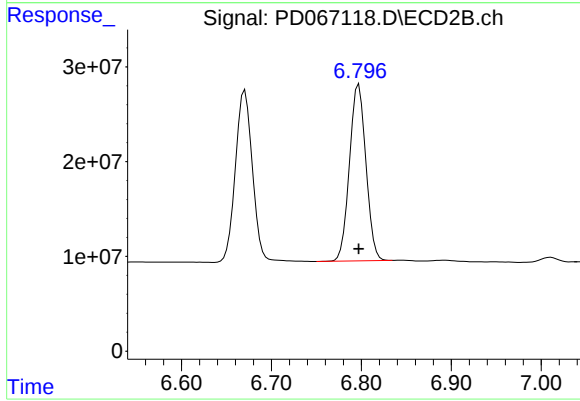


#16 4,4'-DDD

R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 236530026
Conc: 40.00 ng/ml

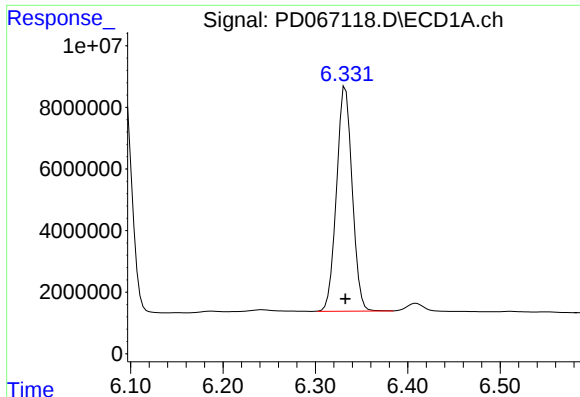


#17 4,4'-DDT

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 85845344
Conc: 40.00 ng/ml

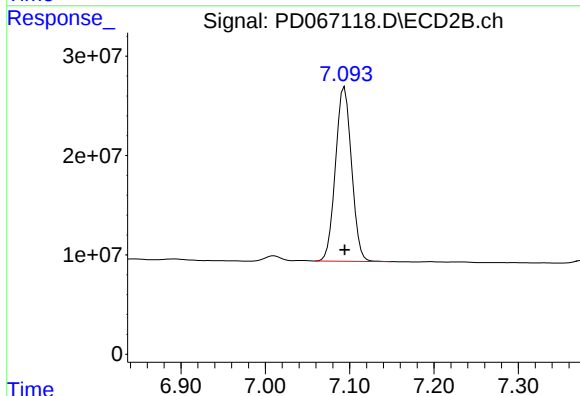


#17 4,4'-DDT

R.T.: 7.094 min
Delta R.T.: 0.000 min
Response: 232279587
Conc: 40.00 ng/ml

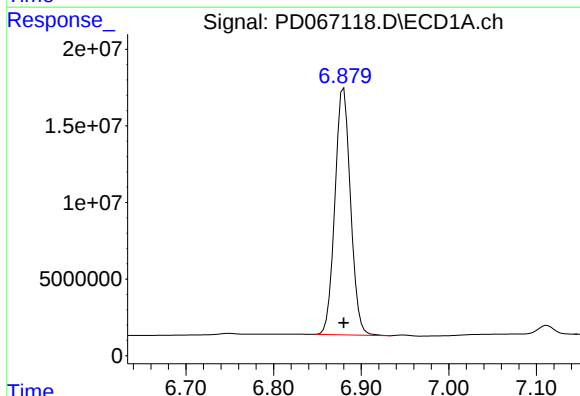


#20 Methoxychlor

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 199477743
Conc: 200.00 ng/ml

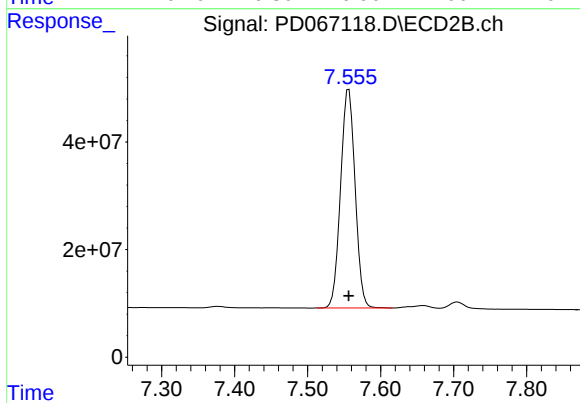


#20 Methoxychlor

R.T.: 7.556 min
Delta R.T.: 0.000 min
Response: 561626492
Conc: 200.00 ng/ml

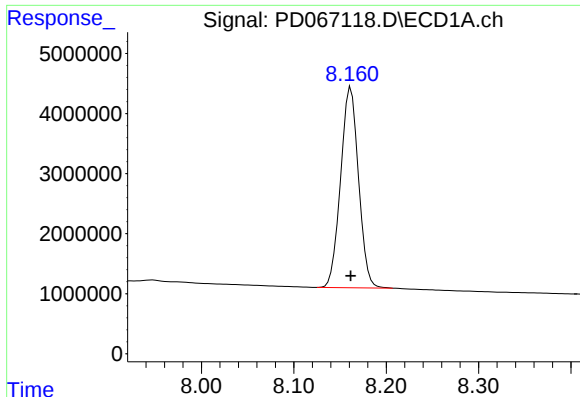

#27 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 44977524
Conc: 40.00 ng/ml

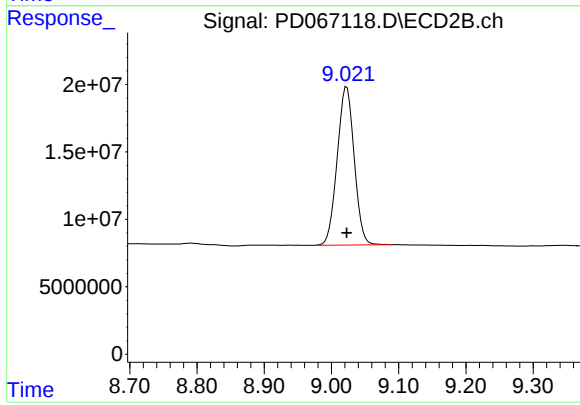

#27 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 205143621
Conc: 40.00 ng/ml