

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
 Data File : PD067120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2021 20:01
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 05:16:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:16:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.966	82702505	289.0E6	37.824	35.927
27)	SA Decachlor...	8.163	9.022	81496687	369.6E6	72.478	72.075
Target Compounds							
2)	A alpha-BHC	3.873	4.360	129.6E6	396.3E6	39.390	37.152
3)	MA gamma-BHC...	4.155	4.645	121.6E6	370.0E6	38.844	37.001
4)	MA Heptachlor	4.448	5.145	125.2E6	344.6E6	38.885	37.028
9)	A Endosulfan I	5.470	6.194	101.9E6	268.8E6	38.187	36.581
13)	MA Dieldrin	5.713	6.453	226.9E6	559.4E6	77.950	74.405
14)	MA Endrin	5.969	6.671	180.6E6	444.3E6	78.716	74.342
16)	A 4,4'-DDD	6.094	6.798	165.4E6	438.6E6	77.314	74.171
17)	MA 4,4'-DDT	6.334	7.095	169.5E6	438.2E6	78.980	75.468
20)	A Methoxychlor	6.881	7.557	375.5E6	1018.8E6	376.495	362.802


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
Data File : PD067120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2021 20:01
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 05:16:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:16:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

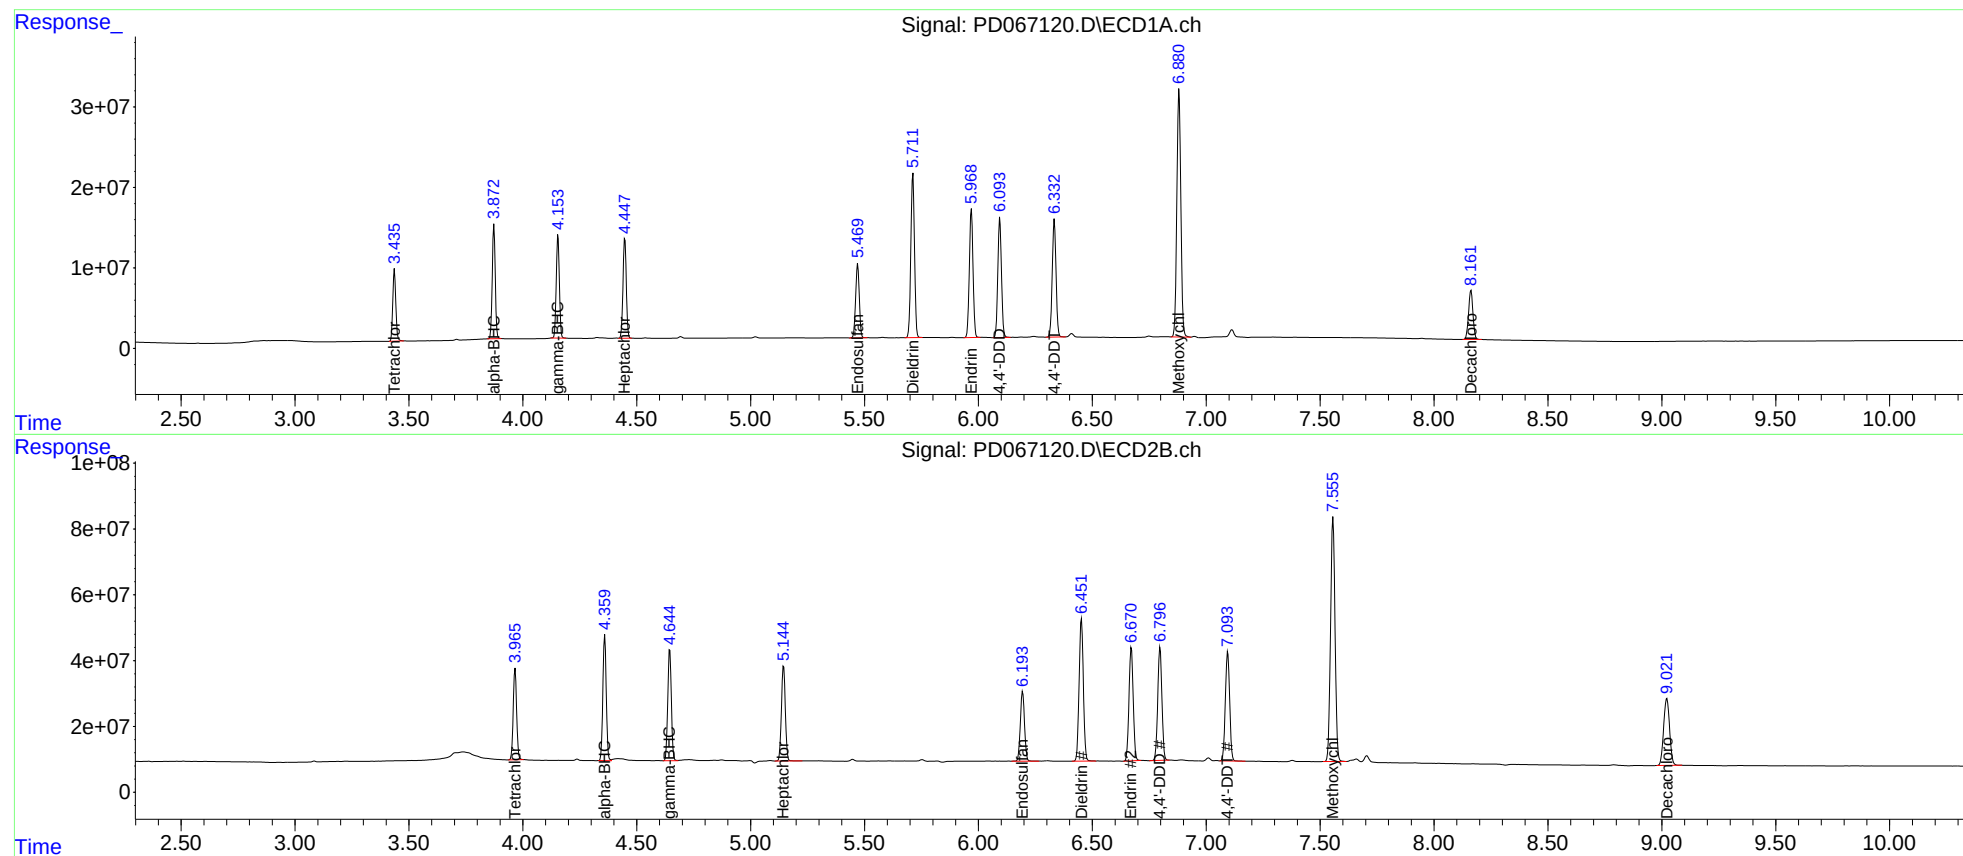

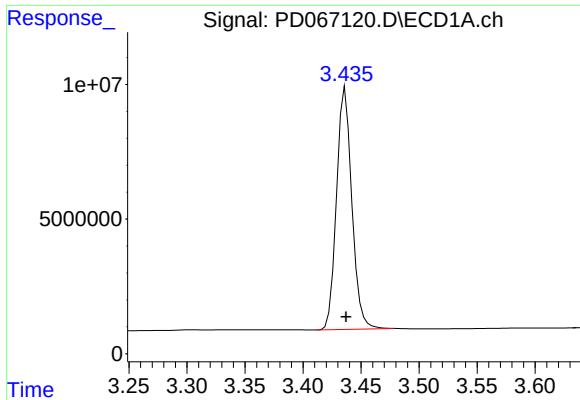


#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: 0.000 min
Response: 82702505
Conc: 37.82 ng/ml

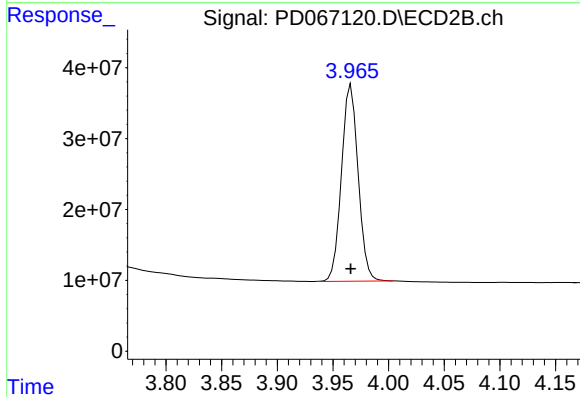


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 288988489
Conc: 35.93 ng/ml

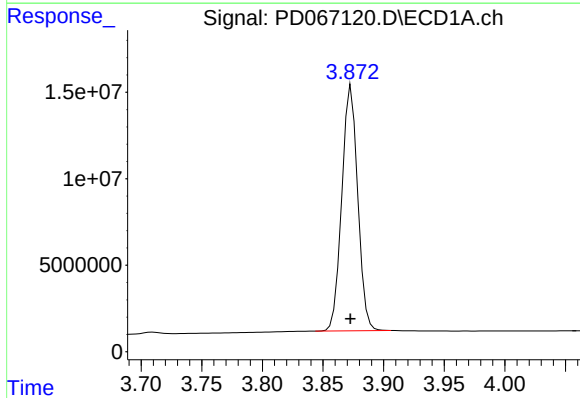


#2 alpha-BHC

R.T.: 3.873 min
Delta R.T.: 0.000 min
Response: 129556494
Conc: 39.39 ng/ml

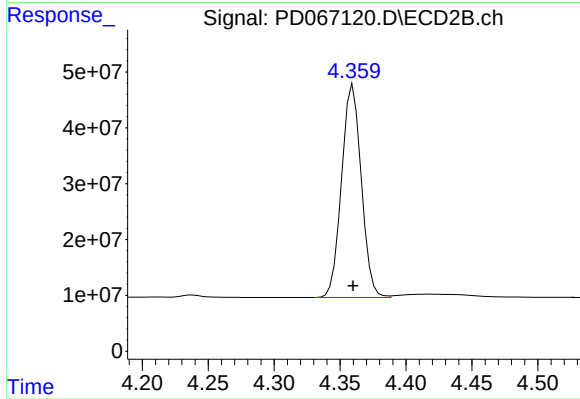


#2 alpha-BHC

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 396297846
Conc: 37.15 ng/ml

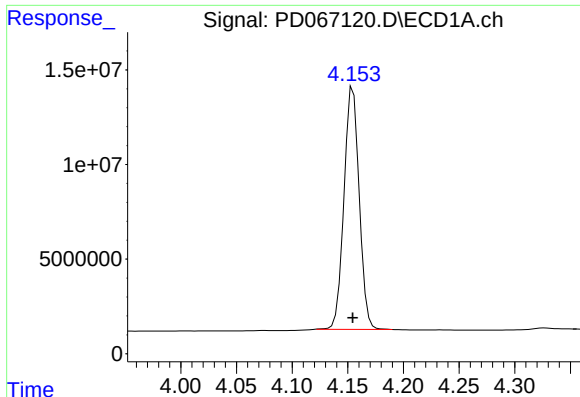


#3 gamma-BHC (Lindane)

R.T.: 4.155 min
Delta R.T.: 0.000 min
Response: 121639890
Conc: 38.84 ng/ml

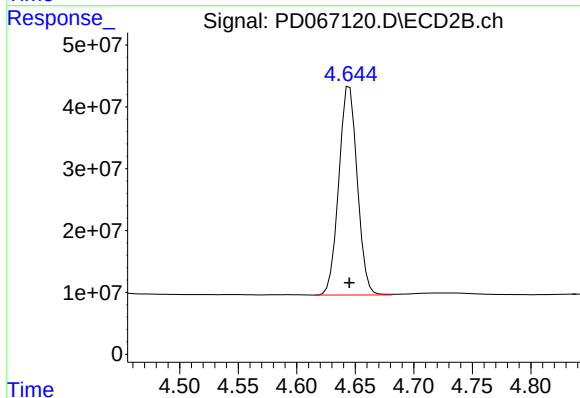


#3 gamma-BHC (Lindane)

R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 369986721
Conc: 37.00 ng/ml

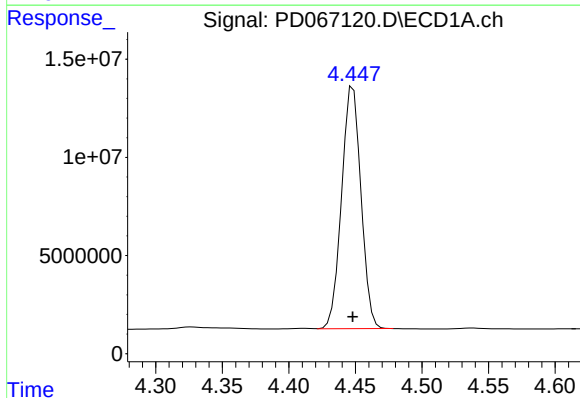


#4 Heptachlor

R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 125241753
Conc: 38.88 ng/ml

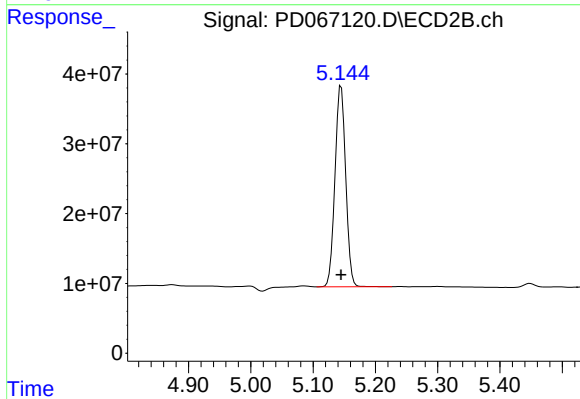


#4 Heptachlor

R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 344579495
Conc: 37.03 ng/ml

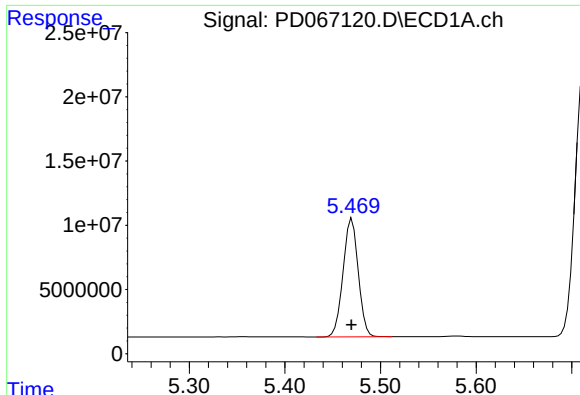


#9 Endosulfan I

R.T.: 5.470 min
Delta R.T.: 0.000 min
Response: 101853108
Conc: 38.19 ng/ml

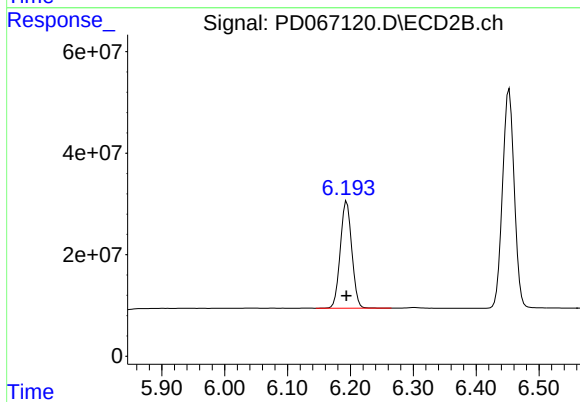


#9 Endosulfan I

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 268810799
Conc: 36.58 ng/ml

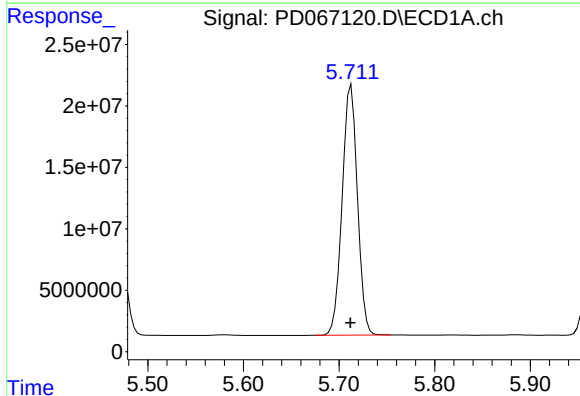


#13 Dieldrin

R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 226893492
Conc: 77.95 ng/ml

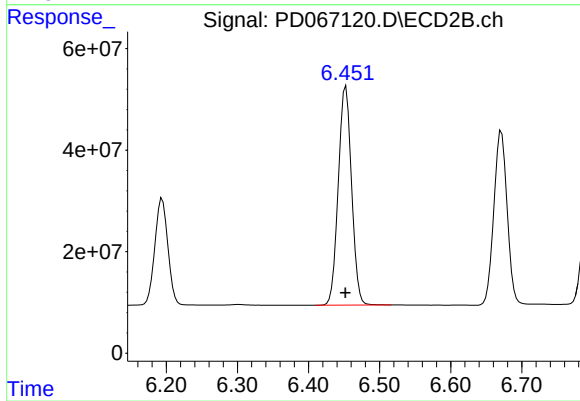


#13 Dieldrin

R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 559414469
Conc: 74.40 ng/ml

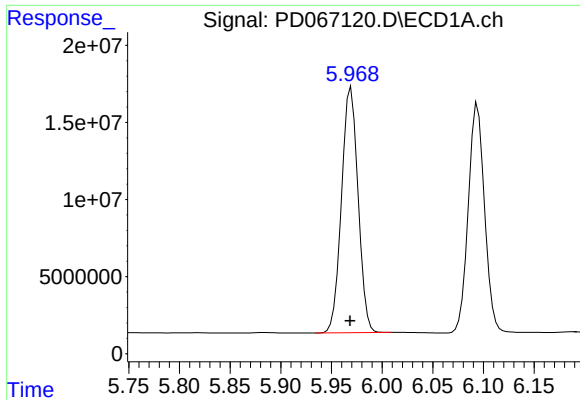


#14 Endrin

R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 180578125
Conc: 78.72 ng/ml

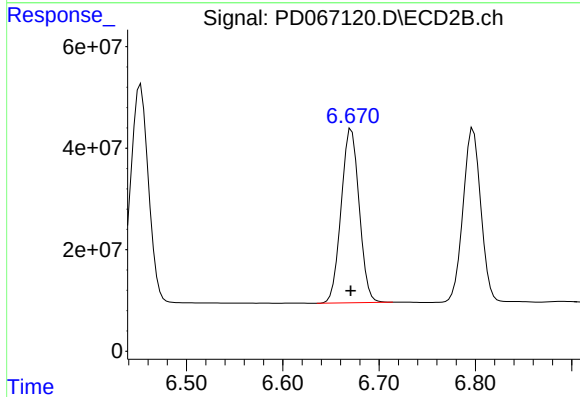


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 444323542
Conc: 74.34 ng/ml

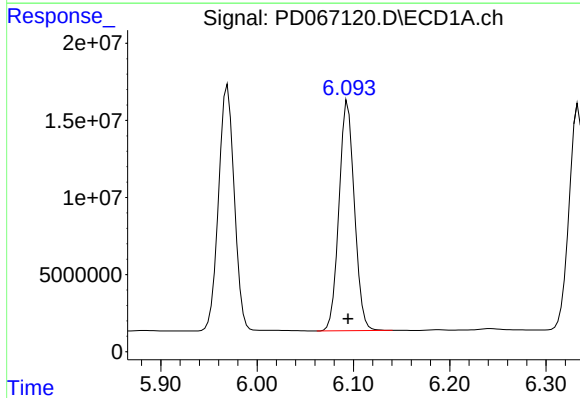


#16 4,4'-DDD

R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 165446545
Conc: 77.31 ng/ml

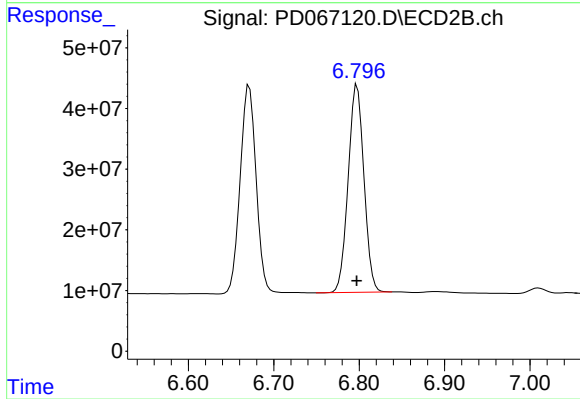


#16 4,4'-DDD

R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 438594665
Conc: 74.17 ng/ml

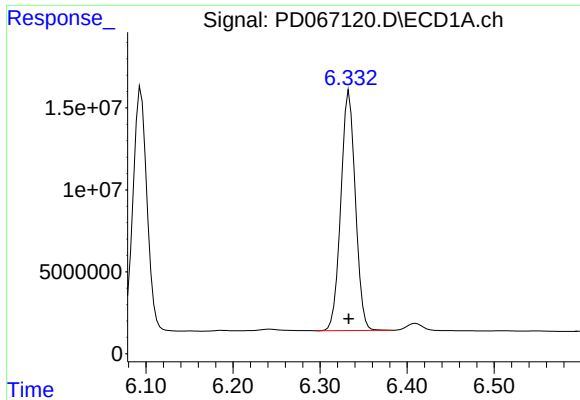


#17 4,4'-DDT

R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 169501590
Conc: 78.98 ng/ml

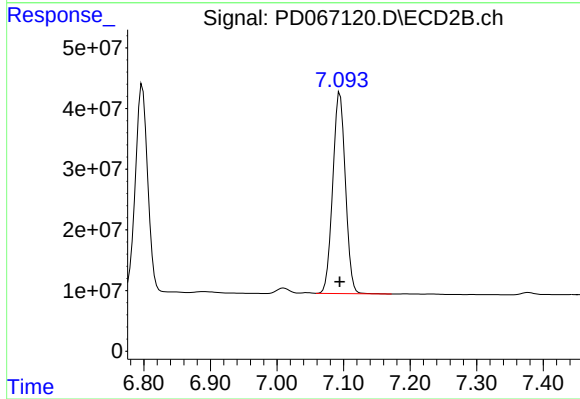


#17 4,4'-DDT

R.T.: 7.095 min
Delta R.T.: 0.000 min
Response: 438244648
Conc: 75.47 ng/ml

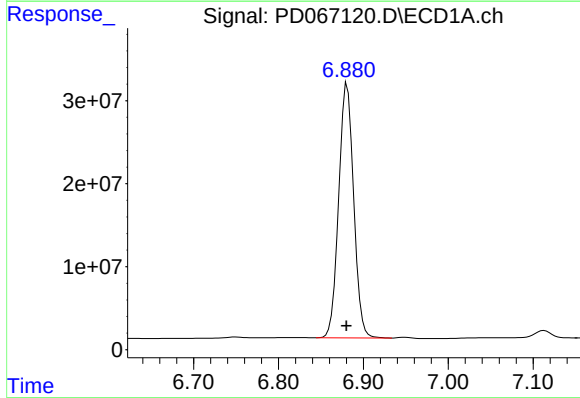


#20 Methoxychlor

R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 375511590
Conc: 376.49 ng/ml

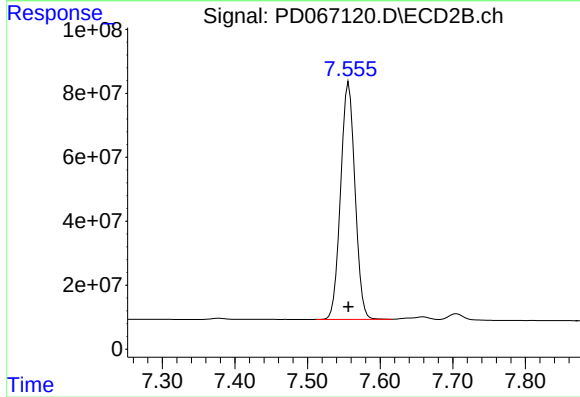


#20 Methoxychlor

R.T.: 7.557 min
Delta R.T.: 0.000 min
Response: 1018796514
Conc: 362.80 ng/ml

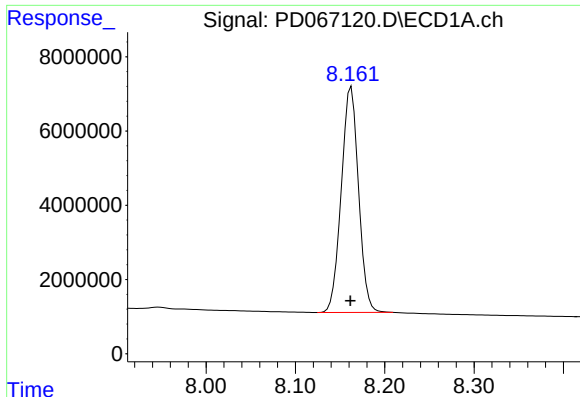

#27 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: 0.000 min
Response: 81496687
Conc: 72.48 ng/ml

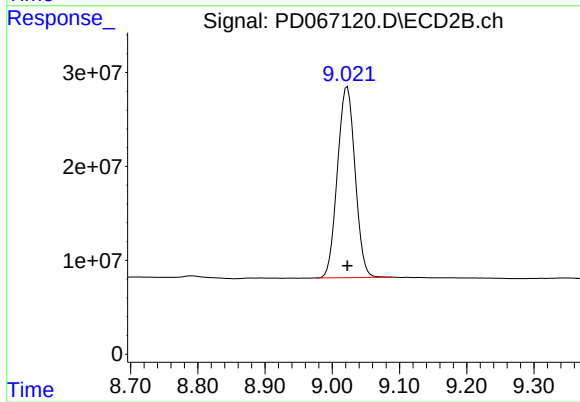

#27 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 369640680
Conc: 72.07 ng/ml