

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
 Data File : PD067122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2021 20:29
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 05:17:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:16:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	3.966	165.1E6	548.3E6	75.516	68.167
27)	SA Decachlor...	8.162	9.022	153.9E6	682.3E6	136.908	133.036
Target Compounds							
2)	A alpha-BHC	3.873	4.360	266.7E6	784.6E6	81.072	73.556
3)	MA gamma-BHC...	4.154	4.645	246.6E6	728.0E6	78.739	72.800
4)	MA Heptachlor	4.448	5.145	253.4E6	662.2E6	78.674	71.155
9)	A Endosulfan I	5.470	6.194	203.2E6	512.8E6	76.181	69.788
13)	MA Dieldrin	5.712	6.452	456.1E6	1080.7E6	156.708	143.736
14)	MA Endrin	5.968	6.671	358.7E6	856.5E6	156.352	143.310
16)	A 4,4'-DDD	6.094	6.797	333.9E6	844.2E6	156.036	142.772
17)	MA 4,4'-DDT	6.333	7.095	343.3E6	847.6E6	159.967	145.957
20)	A Methoxychlor	6.880	7.557	718.7E6	1859.6E6	720.587	662.231


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
Data File : PD067122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2021 20:29
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 05:17:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:16:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

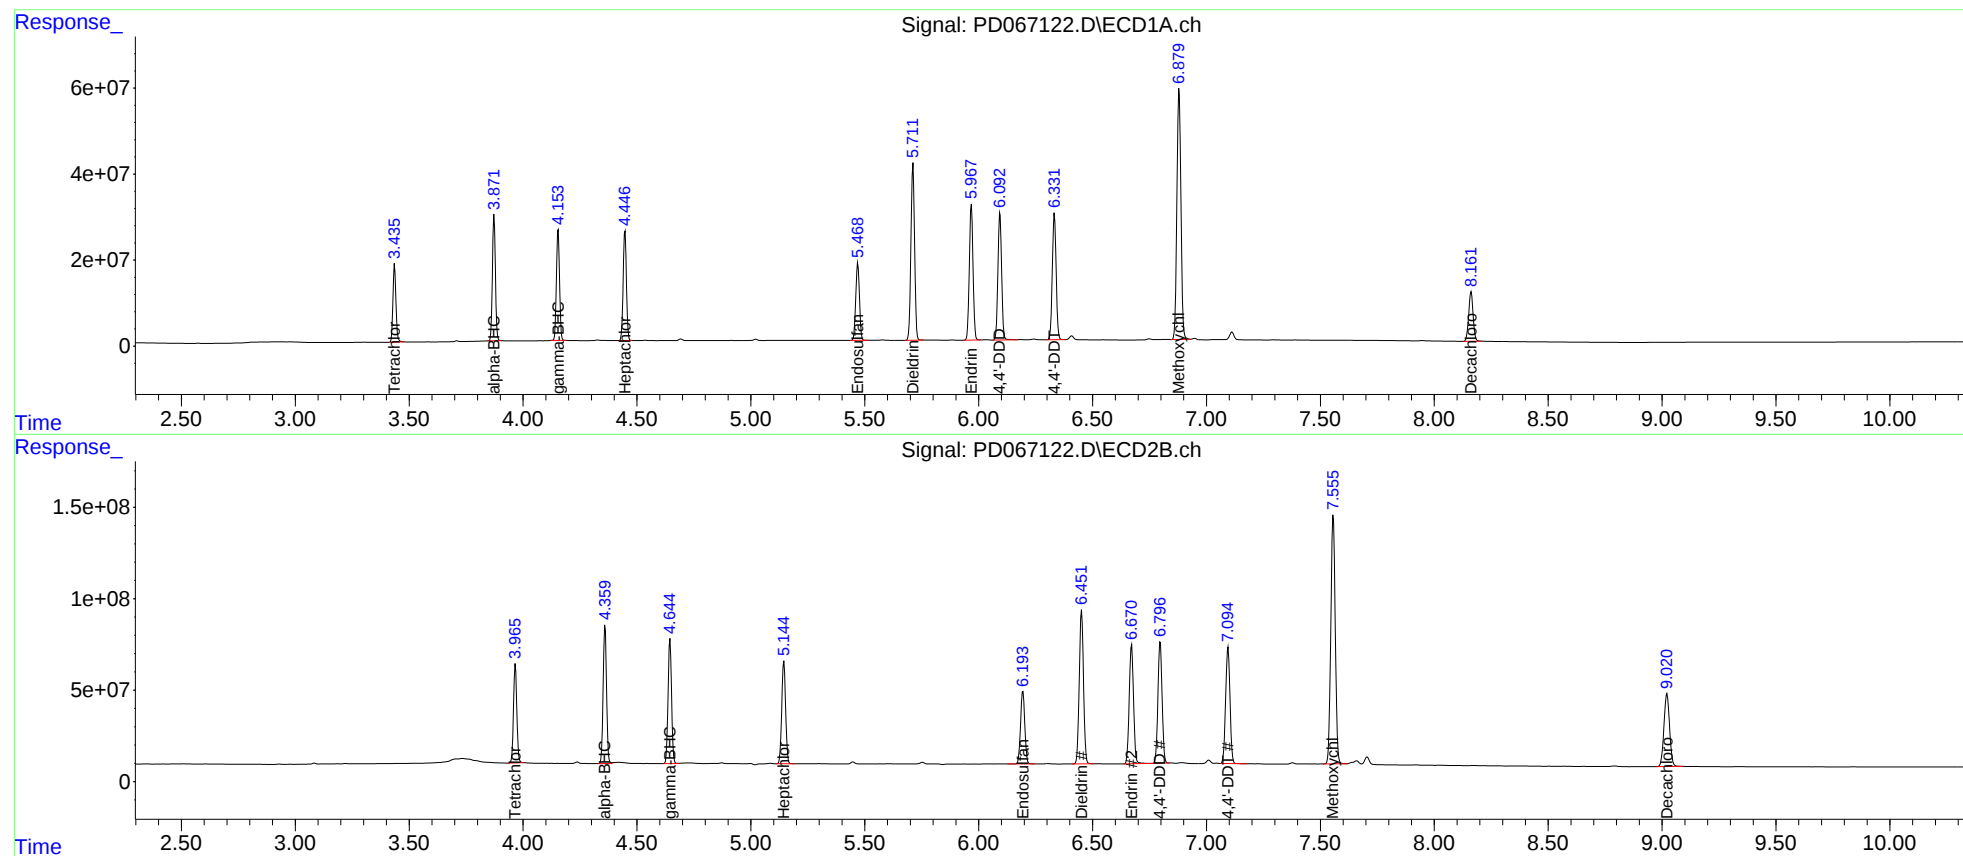

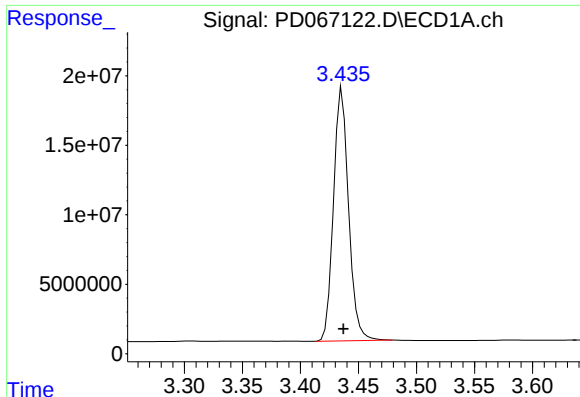


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 165116677
Conc: 75.52 ng/ml

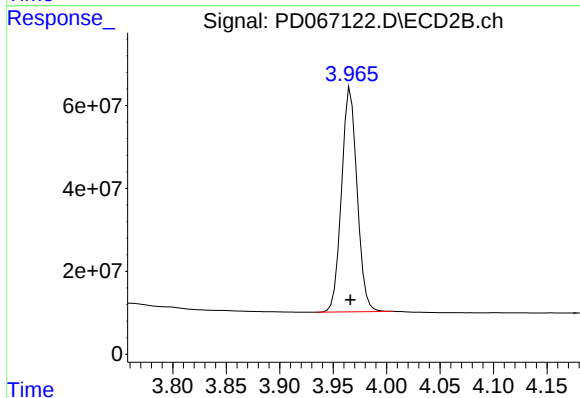


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 548320916
Conc: 68.17 ng/ml

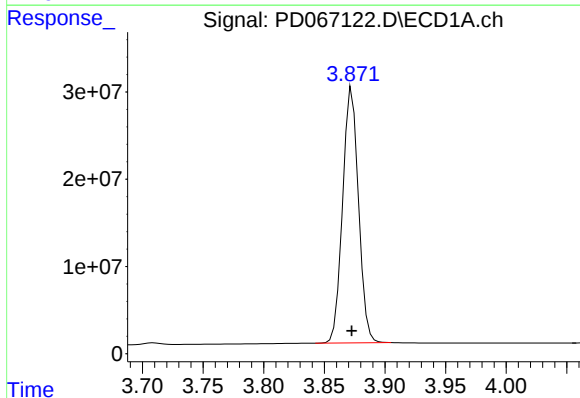


#2 alpha-BHC

R.T.: 3.873 min
Delta R.T.: 0.000 min
Response: 266653005
Conc: 81.07 ng/ml

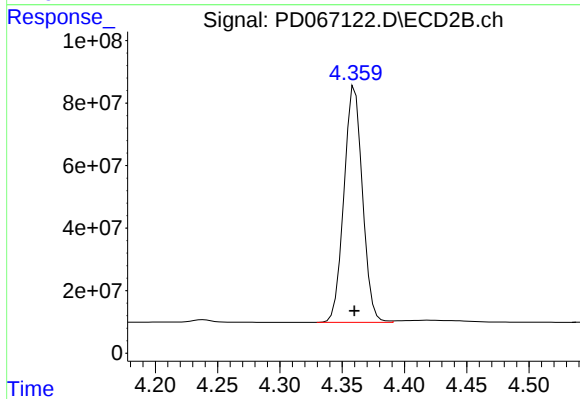


#2 alpha-BHC

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 784625360
Conc: 73.56 ng/ml

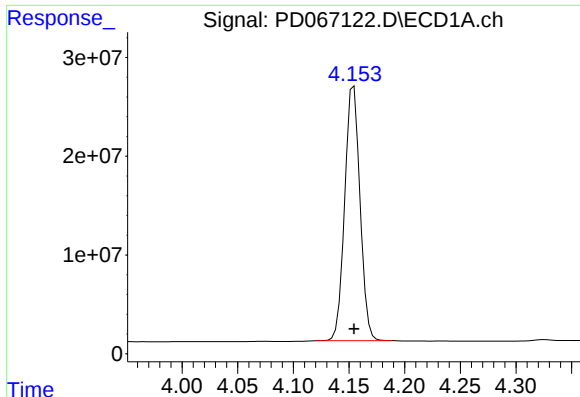


#3 gamma-BHC (Lindane)

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 246572682
Conc: 78.74 ng/ml

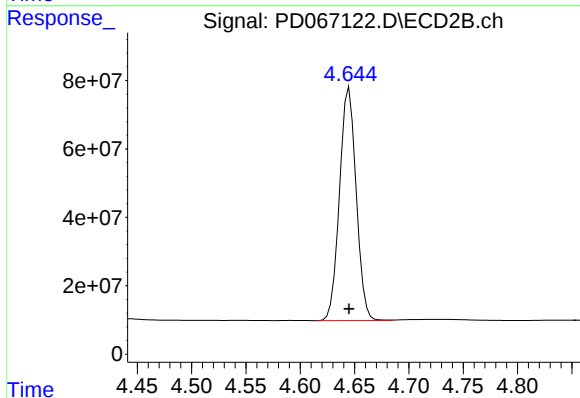


#3 gamma-BHC (Lindane)

R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 727967275
Conc: 72.80 ng/ml

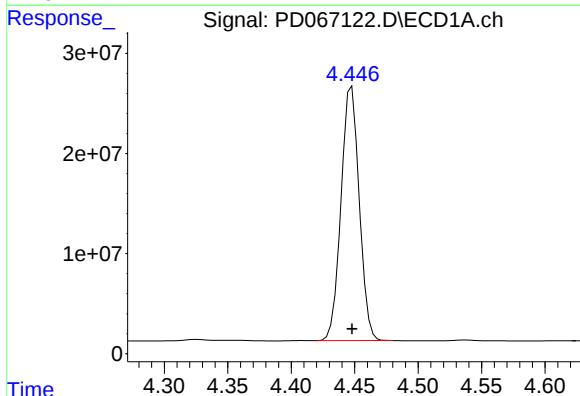


#4 Heptachlor

R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 253397616
Conc: 78.67 ng/ml

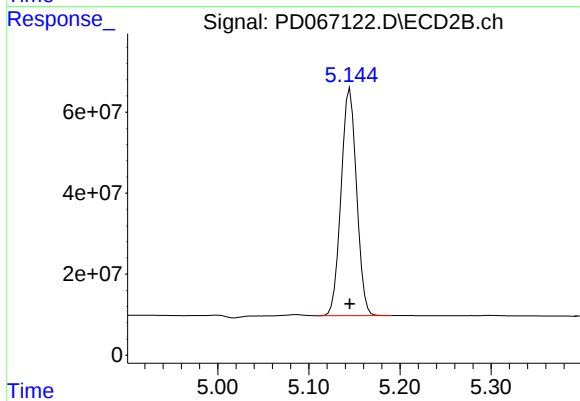


#4 Heptachlor

R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 662165649
Conc: 71.16 ng/ml

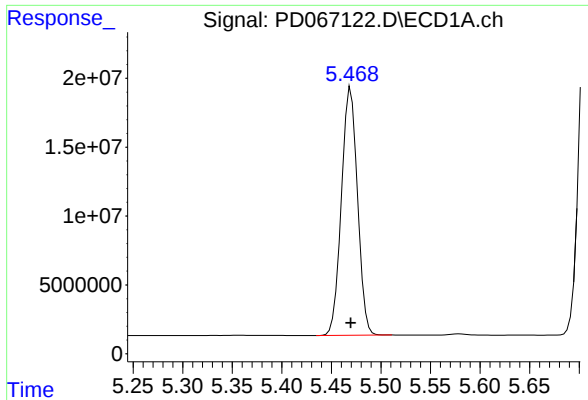


#9 Endosulfan I

R.T.: 5.470 min
Delta R.T.: 0.000 min
Response: 203192879
Conc: 76.18 ng/ml

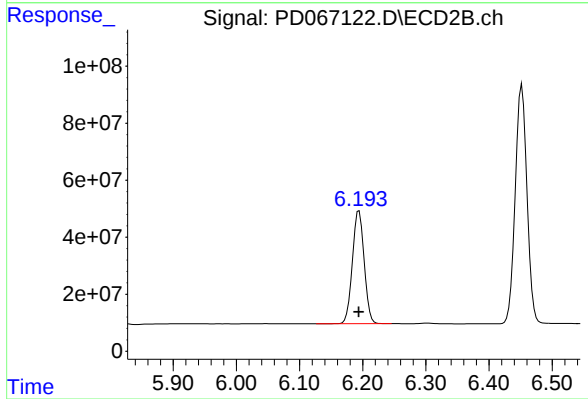


#9 Endosulfan I

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 512829693
Conc: 69.79 ng/ml

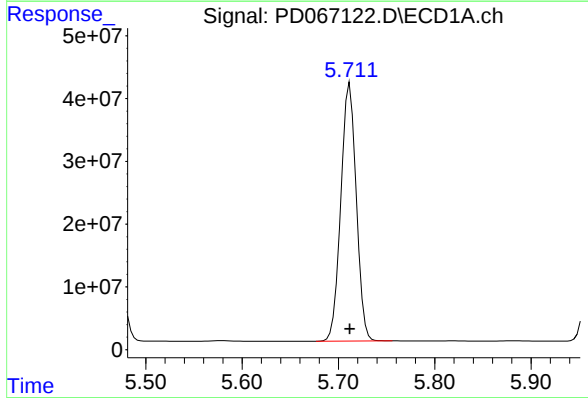


#13 Dieldrin

R.T.: 5.712 min
Delta R.T.: 0.000 min
Response: 456135280
Conc: 156.71 ng/ml

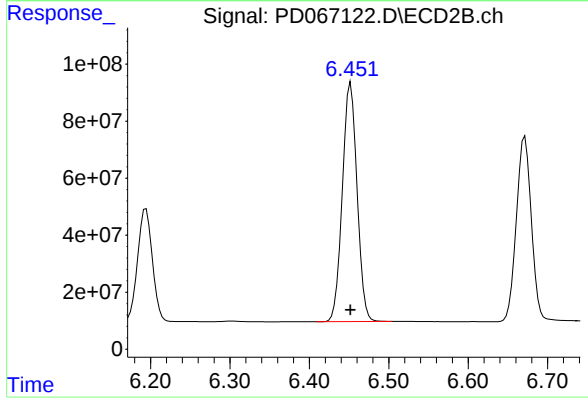


#13 Dieldrin

R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 1080685320
Conc: 143.74 ng/ml

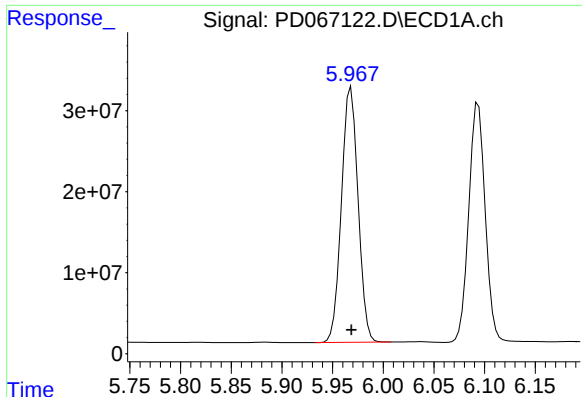


#14 Endrin

R.T.: 5.968 min
Delta R.T.: 0.000 min
Response: 358676612
Conc: 156.35 ng/ml

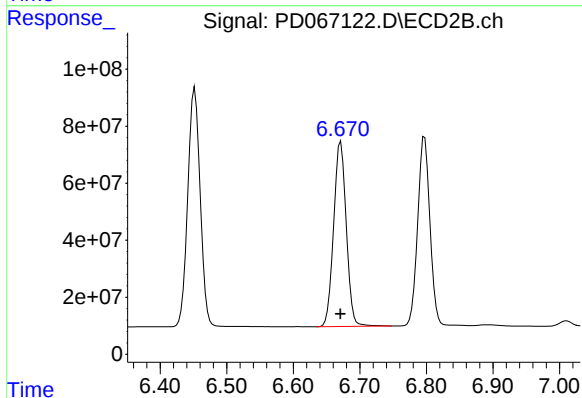


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 856533418
Conc: 143.31 ng/ml

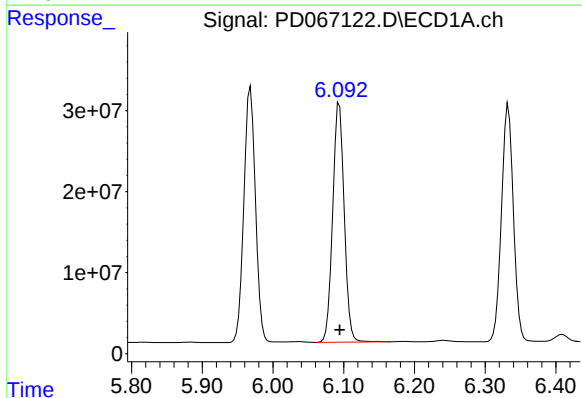


#16 4,4'-DDD

R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 333905561
Conc: 156.04 ng/ml

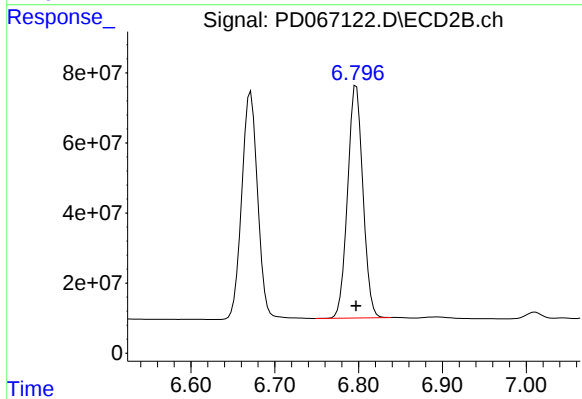


#16 4,4'-DDD

R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 844246171
Conc: 142.77 ng/ml

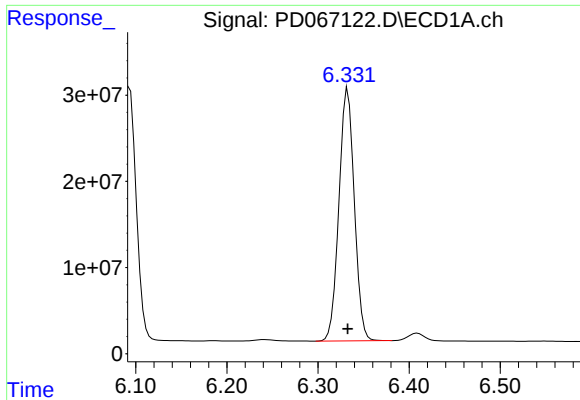


#17 4,4'-DDT

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 343311129
Conc: 159.97 ng/ml

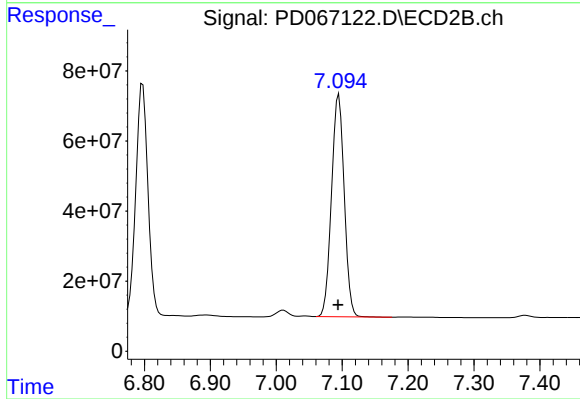


#17 4,4'-DDT

R.T.: 7.095 min
Delta R.T.: 0.000 min
Response: 847568984
Conc: 145.96 ng/ml

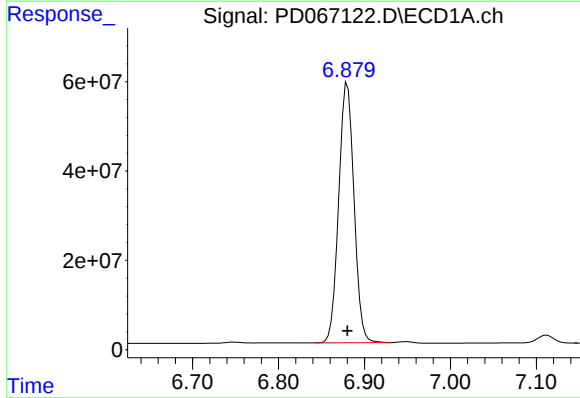


#20 Methoxychlor

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 718705339
Conc: 720.59 ng/ml

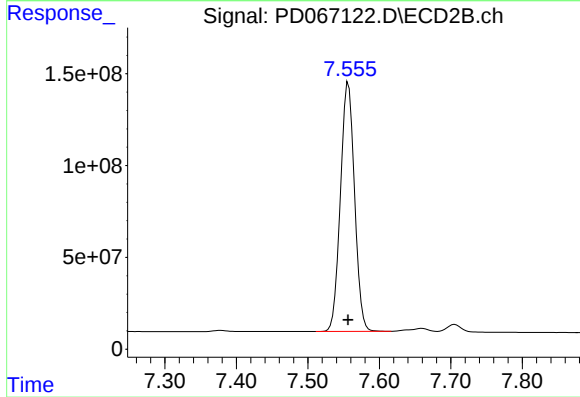


#20 Methoxychlor

R.T.: 7.557 min
Delta R.T.: 0.000 min
Response: 1859632607
Conc: 662.23 ng/ml

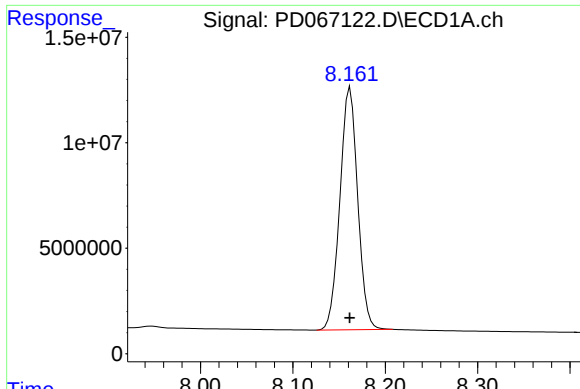

#27 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 153944260
Conc: 136.91 ng/ml

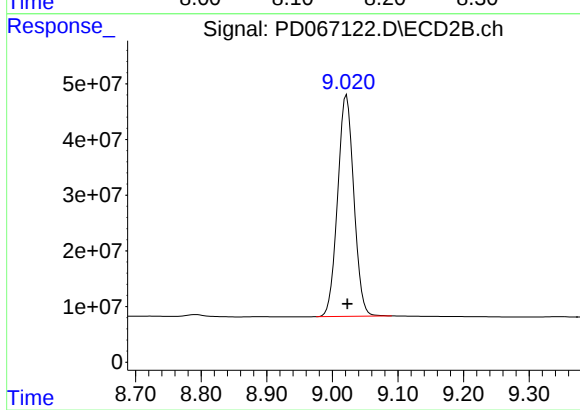

#27 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.001 min
Response: 682286475
Conc: 133.04 ng/ml