

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
 Data File : PD067123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2021 20:42
 Operator : AR\AJ
 Sample : INDB501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 04:55:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 04:54:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.966	157.0E6	522.6E6	75.964	68.225
27)	SA Decachlor...	8.162	9.022	150.1E6	669.0E6	137.869	136.589
Target Compounds							
5)	MB Aldrin	4.693	5.448	247.8E6	621.8E6	80.338	71.981
6)	B beta-BHC	4.403	4.822	94537238	315.7E6	71.611	67.640
7)	B delta-BHC	4.605	5.038	234.0E6	683.7E6	81.889	73.530
8)	B Heptachlo...	5.134	5.838	214.2E6	529.4E6	78.124	74.319
10)	B trans-Chl...	5.357	6.071	221.3E6	543.5E6	79.148	71.565
11)	B cis-Chlor...	5.416	6.143	213.9E6	525.1E6	77.726	70.926
12)	B 4,4'-DDE	5.580	6.303	406.1E6	987.2E6	162.015	147.020
15)	B Endosulfa...	6.241	6.885	345.5E6	879.2E6	154.814	144.342
18)	B Endrin al...	6.410	7.010	246.3E6	669.8E6	150.427	141.177
19)	B Endosulfa...	6.622	7.233	291.7E6	824.7E6	151.906	143.198
21)	B Endrin ke...	7.114	7.706	311.7E6	932.5E6	151.222	140.984


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
Data File : PD067123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2021 20:42
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 04:55:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 04:54:46 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

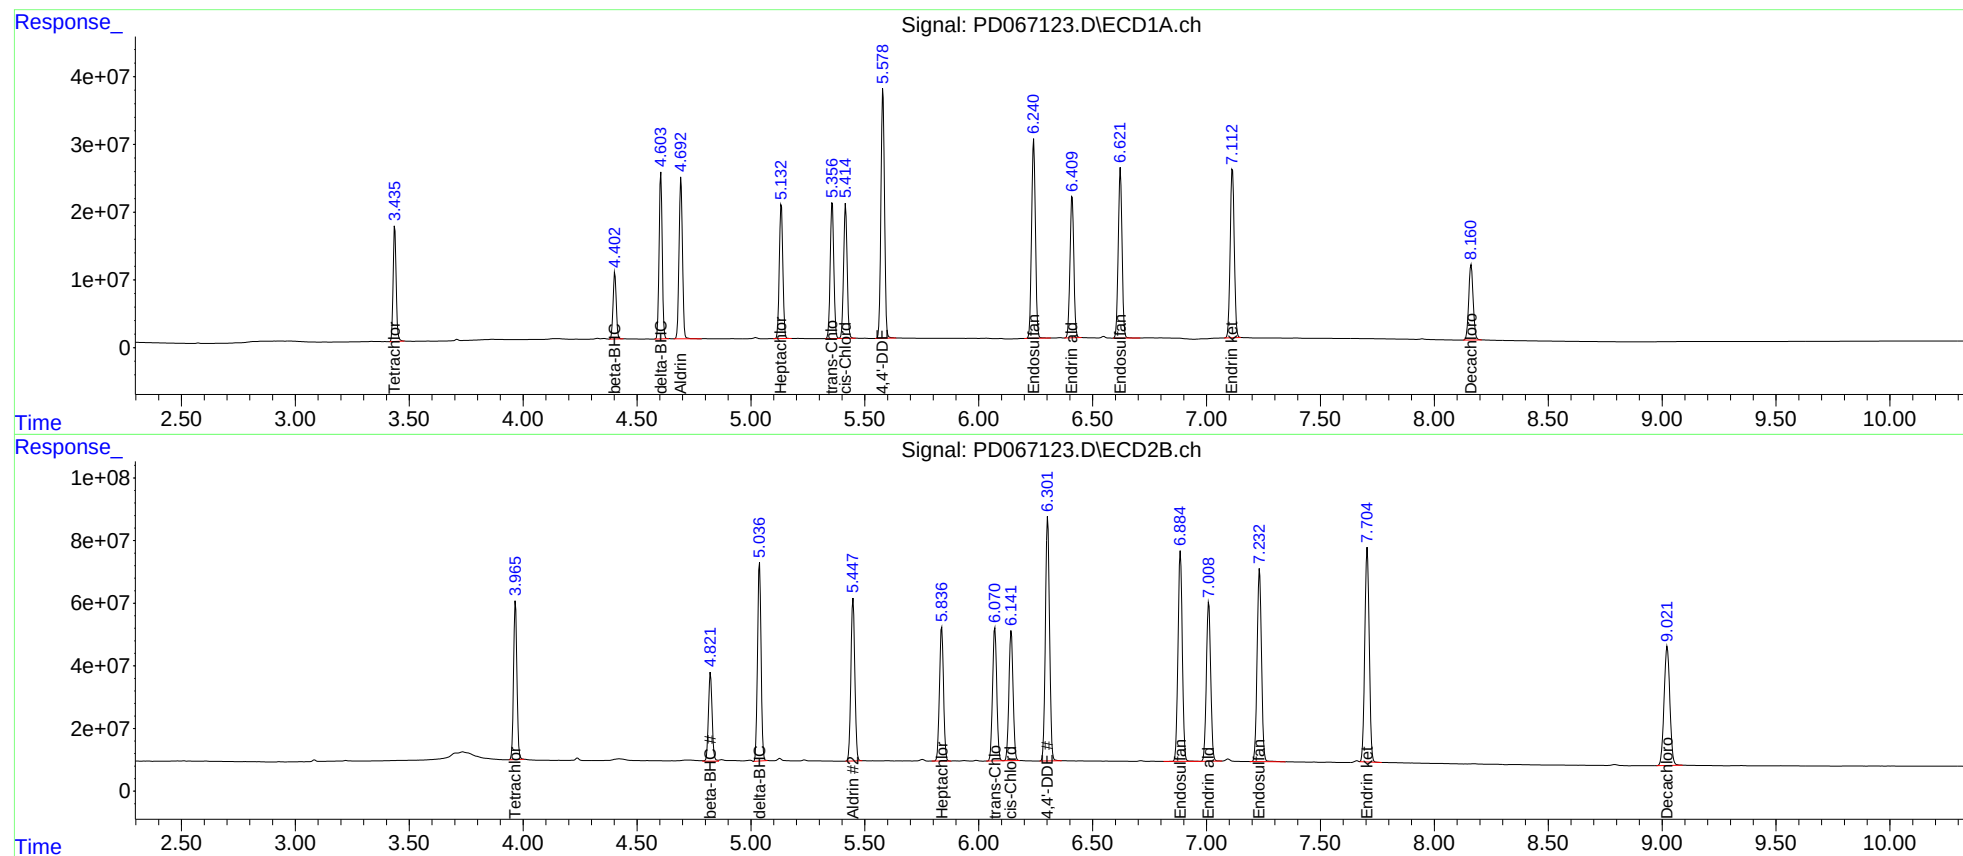

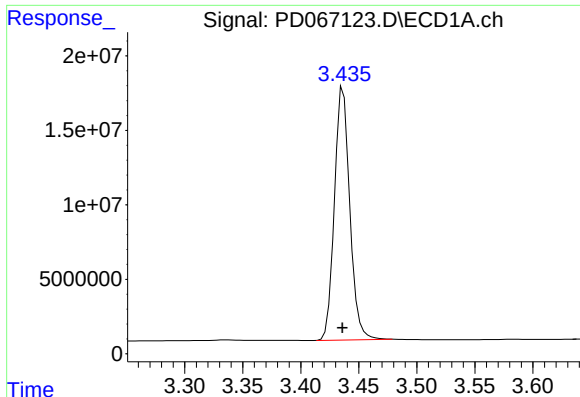


#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: 0.000 min
Response: 157042171
Conc: 75.96 ng/ml

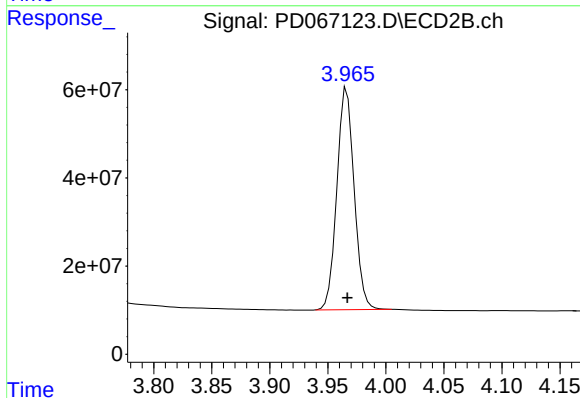


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 522568477
Conc: 68.23 ng/ml

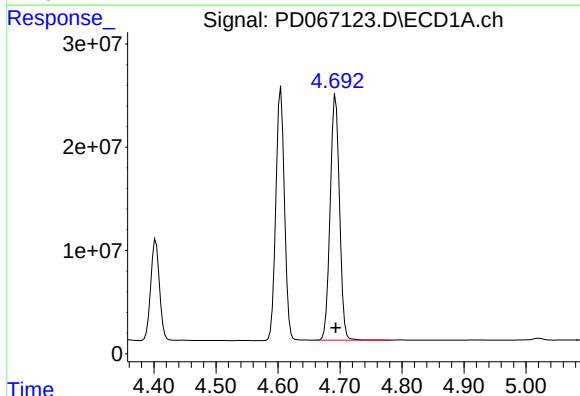


#5 Aldrin

R.T.: 4.693 min
Delta R.T.: 0.000 min
Response: 247795961
Conc: 80.34 ng/ml

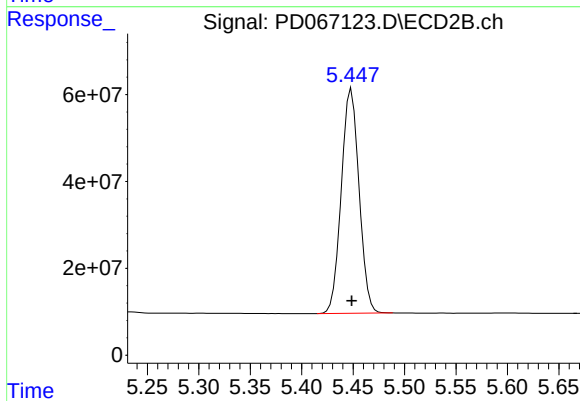


#5 Aldrin

R.T.: 5.448 min
Delta R.T.: 0.000 min
Response: 621753697
Conc: 71.98 ng/ml

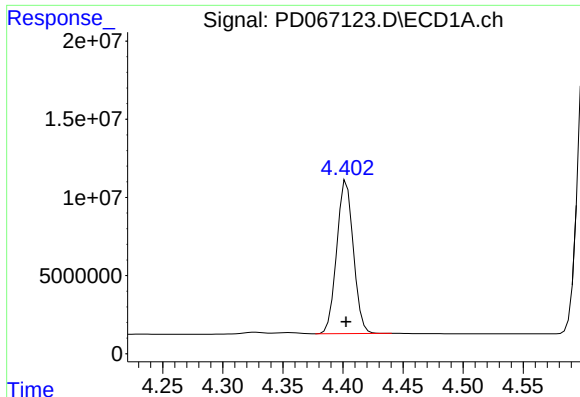


#6 beta-BHC

R.T.: 4.403 min
Delta R.T.: 0.000 min
Response: 94537238
Conc: 71.61 ng/ml

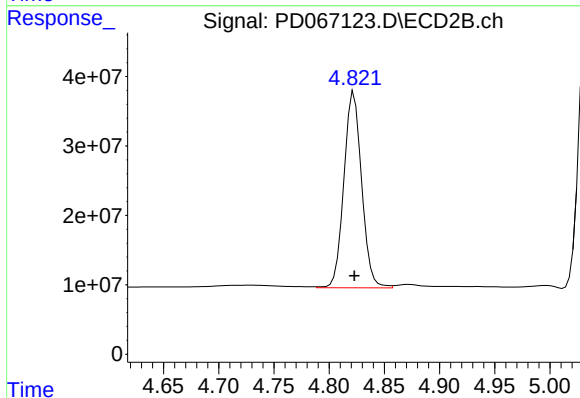


#6 beta-BHC

R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 315695719
Conc: 67.64 ng/ml

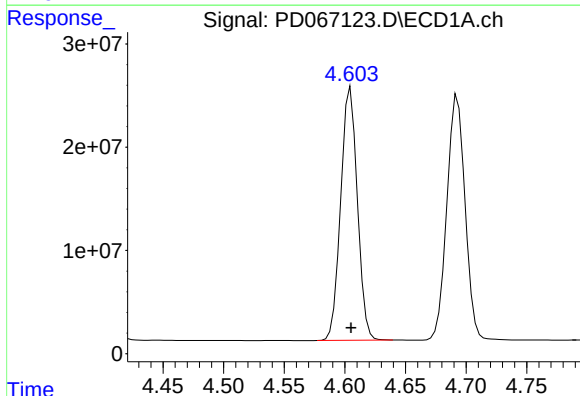


#7 delta-BHC

R.T.: 4.605 min
Delta R.T.: 0.000 min
Response: 234030924
Conc: 81.89 ng/ml

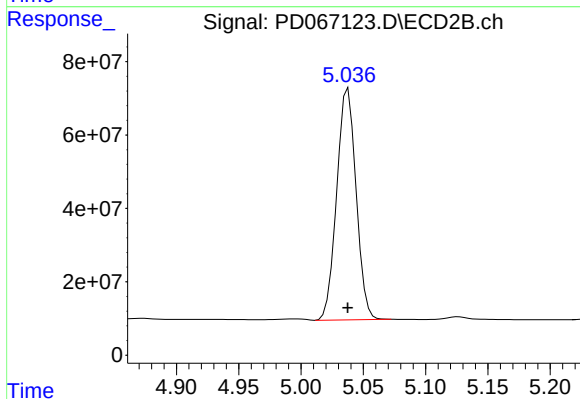


#7 delta-BHC

R.T.: 5.038 min
Delta R.T.: 0.000 min
Response: 683707309
Conc: 73.53 ng/ml

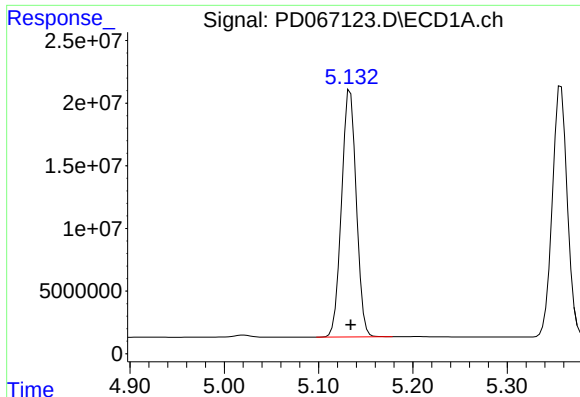


#8 Heptachlor epoxide

R.T.: 5.134 min
Delta R.T.: 0.000 min
Response: 214213913
Conc: 78.12 ng/ml

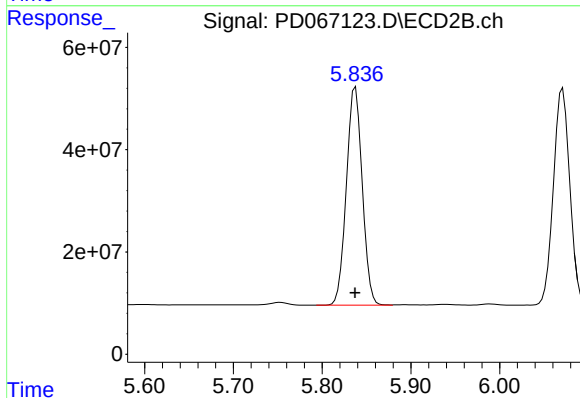


#8 Heptachlor epoxide

R.T.: 5.838 min
Delta R.T.: 0.000 min
Response: 529385917
Conc: 74.32 ng/ml

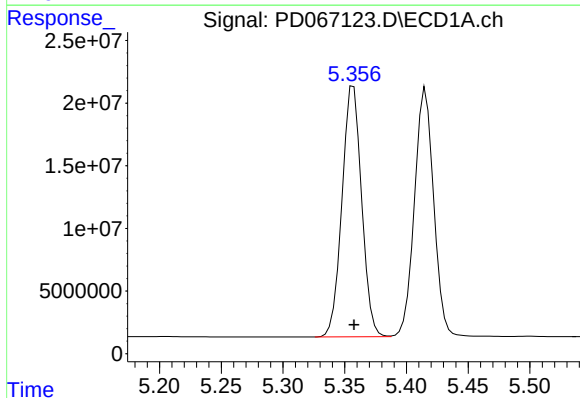


#10 trans-Chlordane

R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 221257731
Conc: 79.15 ng/ml

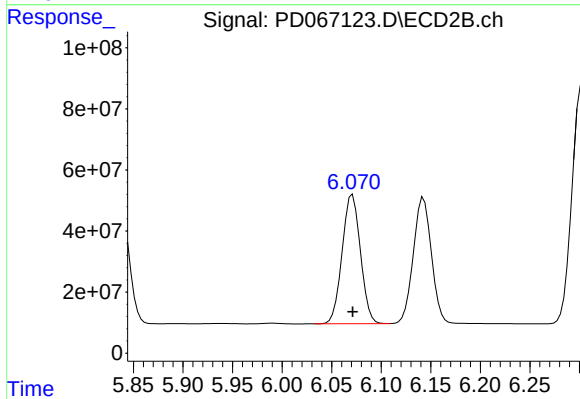


#10 trans-Chlordane

R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 543495543
Conc: 71.57 ng/ml

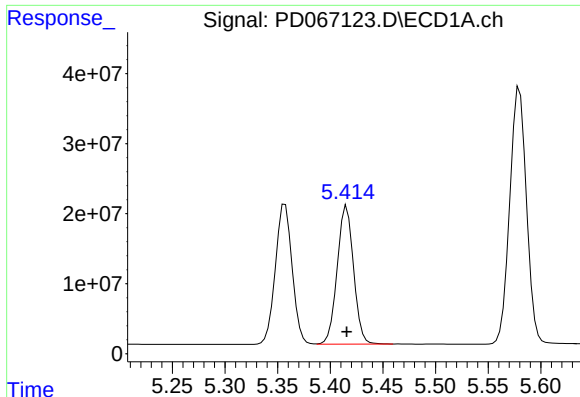


#11 cis-Chlordane

R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 213919860
Conc: 77.73 ng/ml

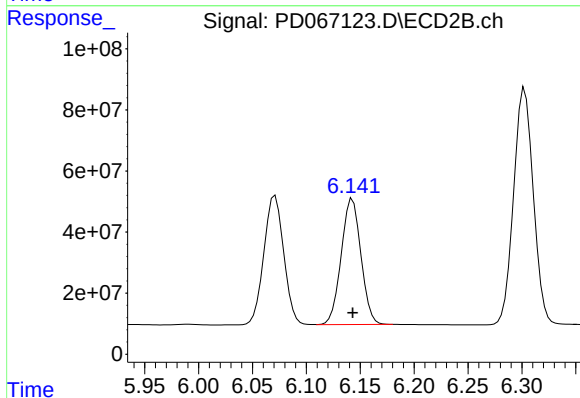


#11 cis-Chlordane

R.T.: 6.143 min
Delta R.T.: 0.000 min
Response: 525129537
Conc: 70.93 ng/ml

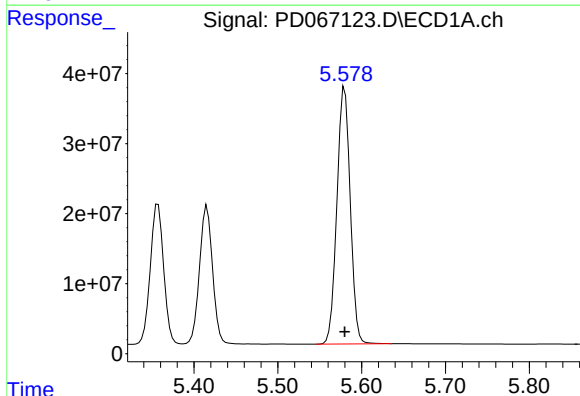


#12 4,4'-DDE

R.T.: 5.580 min
Delta R.T.: 0.000 min
Response: 406066813
Conc: 162.01 ng/ml

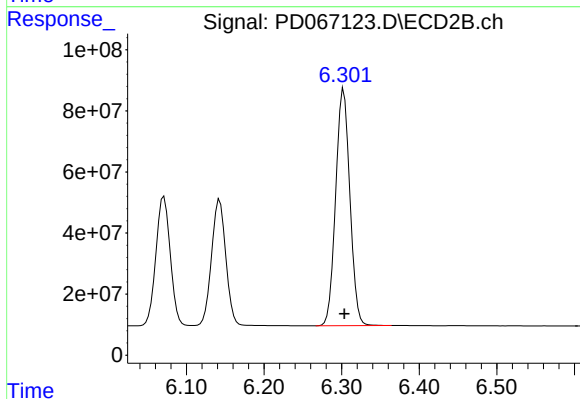


#12 4,4'-DDE

R.T.: 6.303 min
Delta R.T.: 0.000 min
Response: 987178886
Conc: 147.02 ng/ml

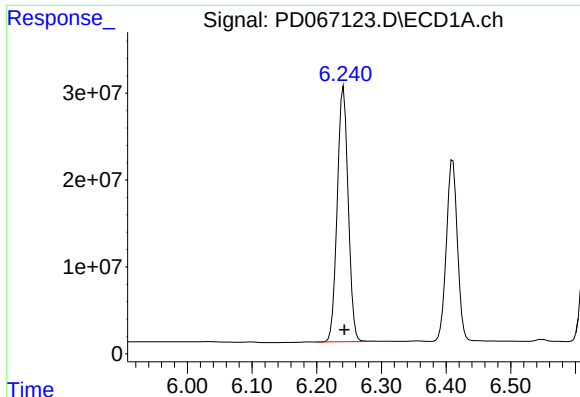


#15 Endosulfan II

R.T.: 6.241 min
Delta R.T.: -0.001 min
Response: 345513743
Conc: 154.81 ng/ml

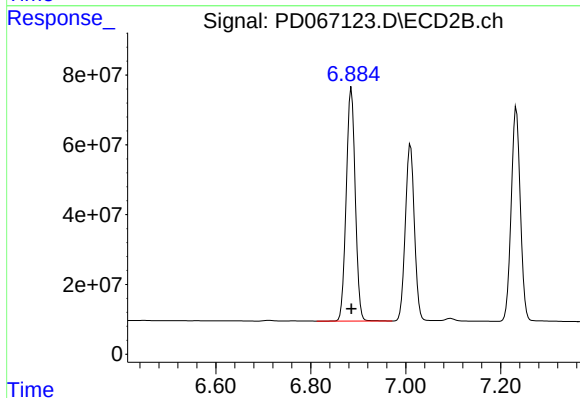


#15 Endosulfan II

R.T.: 6.885 min
Delta R.T.: 0.000 min
Response: 879186883
Conc: 144.34 ng/ml

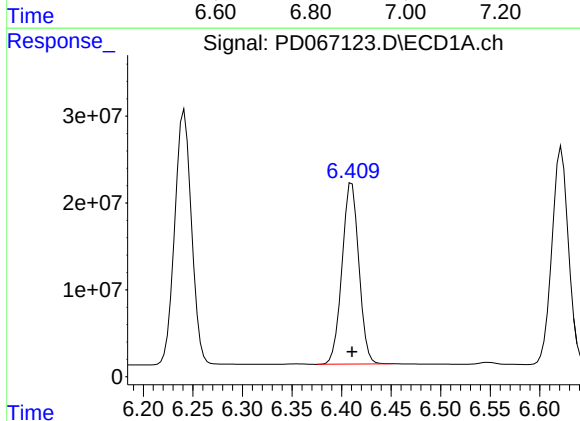


#18 Endrin aldehyde

R.T.: 6.410 min
Delta R.T.: 0.000 min
Response: 246315600
Conc: 150.43 ng/ml

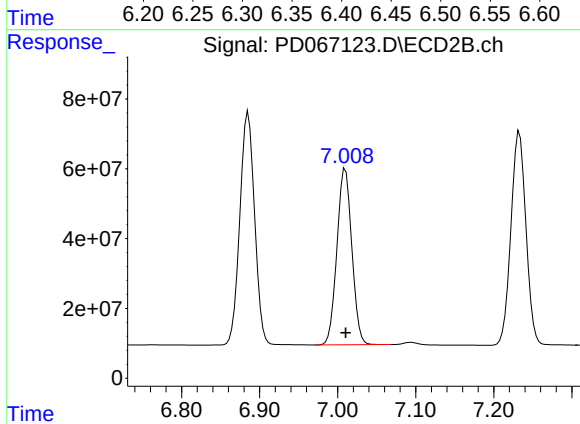


#18 Endrin aldehyde

R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 669849506
Conc: 141.18 ng/ml

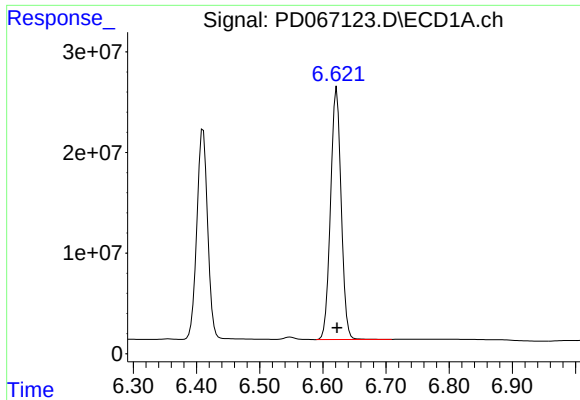


#19 Endosulfan Sulfate

R.T.: 6.622 min
Delta R.T.: 0.000 min
Response: 291672019
Conc: 151.91 ng/ml

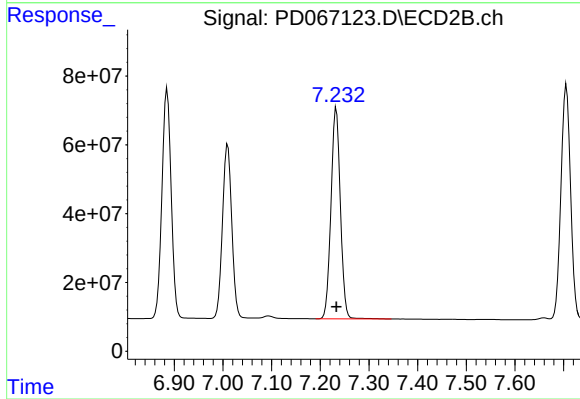


#19 Endosulfan Sulfate

R.T.: 7.233 min
Delta R.T.: 0.000 min
Response: 824731228
Conc: 143.20 ng/ml

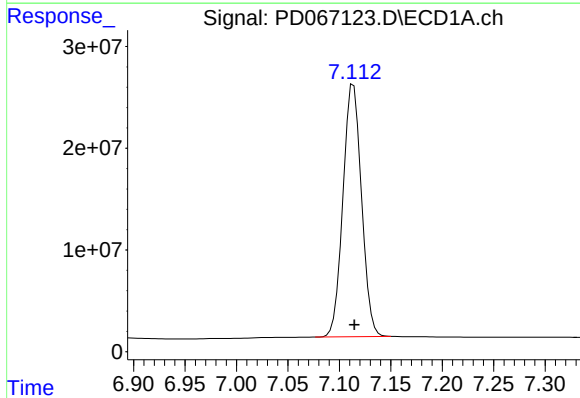


#21 Endrin ketone

R.T.: 7.114 min
Delta R.T.: 0.000 min
Response: 311745738
Conc: 151.22 ng/ml

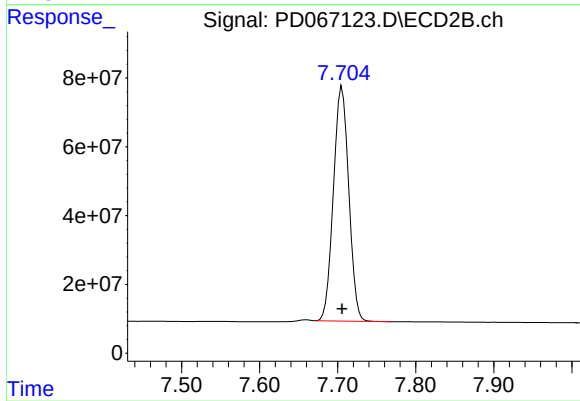


#21 Endrin ketone

R.T.: 7.706 min
Delta R.T.: 0.000 min
Response: 932501598
Conc: 140.98 ng/ml

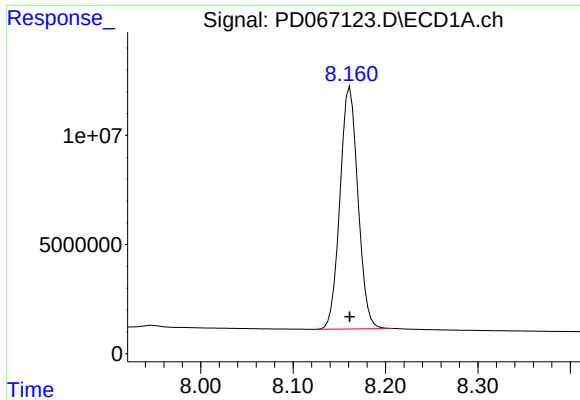

#27 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 150060682
Conc: 137.87 ng/ml

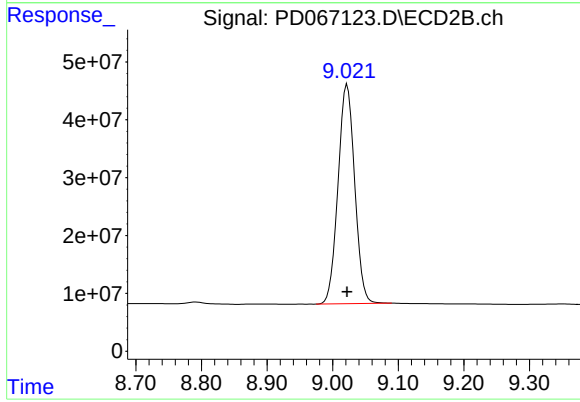

#27 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 668990107
Conc: 136.59 ng/ml