

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
 Data File : PD067107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2021 16:47
 Operator : AR\AJ
 Sample : RESC007
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 05:31:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:28:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.966	41747431	155.7E6	19.119	19.432
27)	SA Decachlor...	8.164	9.023	43767668	195.3E6	38.550	38.517
Target Compounds							
2)	A alpha-BHC	3.874	4.360	32315551	112.9E6	9.880	10.524
3)	MA gamma-BHC...	4.155	4.645	31039937	105.1E6	9.753	10.480
4)	MA Heptachlor	4.448	5.145	31960164	100.4E6	9.971	10.761
5)	MB Aldrin	4.693	5.449	30349313	89970605	9.809	10.434
6)	B beta-BHC	4.403	4.823	13466508	48212267	10.116	10.450
7)	B delta-BHC	4.605	5.037	27223185	94774793	9.517	10.707
8)	B Heptachlo...	5.135	5.837	27087089	71813422	9.808	10.246
9)	A Endosulfan I	5.471	6.194	26683710	77727067	10.036	10.722
10)	B trans-Chl...	5.358	6.071	27356043	78016593	9.709	10.279
11)	B cis-Chlor...	5.417	6.142	26829231	77149255	9.669	10.428
12)	B 4,4'-DDE	5.581	6.303	47965783	136.0E6	19.166	20.292
13)	MA Dieldrin	5.713	6.452	57192776	157.1E6	19.861	21.118
14)	MA Endrin	5.970	6.671	45991694	118.6E6	20.111	20.448
15)	B Endosulfa...	6.243	6.885	44380042	125.0E6	19.767	20.583
16)	A 4,4'-DDD	6.096	6.797	42252625	122.5E6	19.985	20.939
17)	MA 4,4'-DDT	6.334	7.095	41825458	118.8E6	19.676	20.624
18)	B Endrin al...	6.411	7.010	34122590	99167800	20.692	21.041
19)	B Endosulfa...	6.624	7.234	38195374	116.4E6	19.799	20.267
20)	A Methoxychlor	6.882	7.557	102.5E6	296.6E6	103.150	106.556
21)	B Endrin ke...	7.115	7.706	44459794	140.1E6	21.416	21.215

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
Data File : PD067107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2021 16:47
Operator : AR\AJ
Sample : RESC007
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 05:31:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

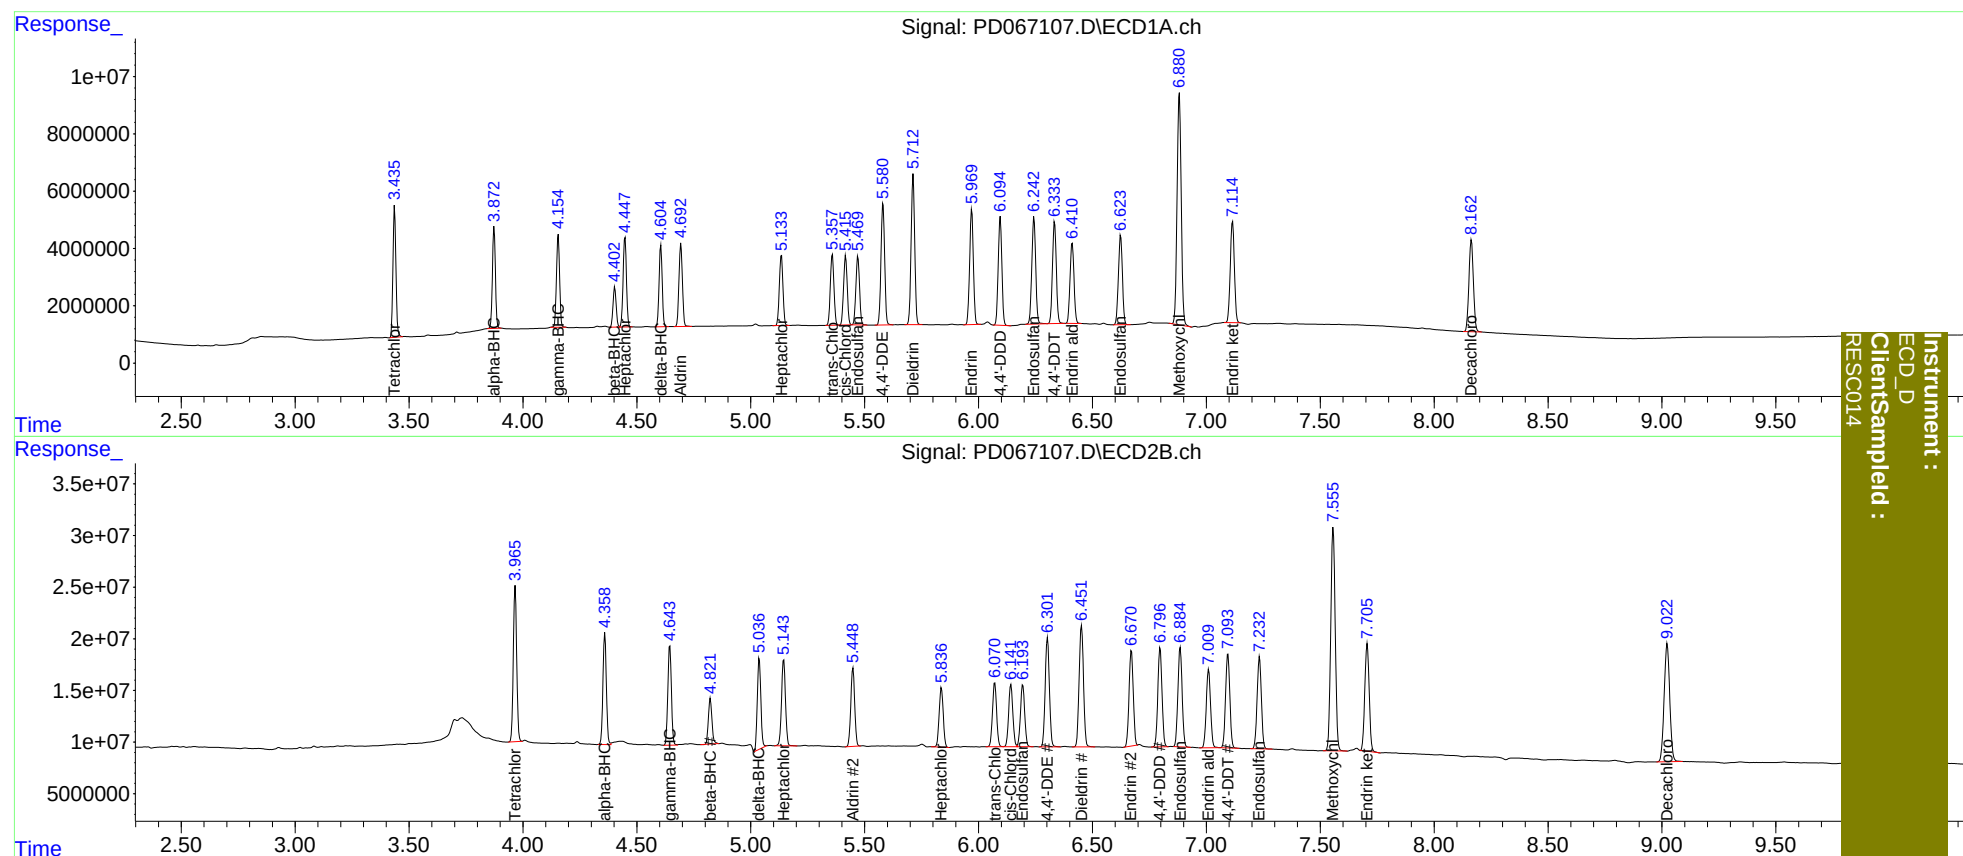

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
Data File : PD067107.D
Acq On : 29 Nov 2021 16:47
Operator : AR\AJ
Sample : RESC007
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Title : GC Extractables
Last Update : Tue Nov 30 05:28:01 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.437	3.874	100.00%
3.874	4.155	100.00%
4.155	4.403	100.00%
4.403	4.448	100.00%
4.448	4.605	100.00%
4.605	4.693	100.00%
4.693	5.135	100.00%
5.135	5.358	100.00%
5.358	5.417	100.00%
5.417	5.471	100.00%
5.471	5.581	100.00%
5.581	5.713	100.00%
5.713	5.970	100.00%
5.970	6.096	100.00%
6.096	6.243	100.00%
6.243	6.334	100.00%
6.334	6.411	100.00%
6.411	6.624	100.00%
6.624	6.882	100.00%
6.882	7.115	100.00%
7.115	8.164	100.00%

Signal #2


3.966	4.360	100.00%
4.360	4.645	100.00%
4.645	4.823	100.00%
4.823	5.037	100.00%
5.037	5.145	100.00%
5.145	5.449	100.00%
5.449	5.837	100.00%
5.837	6.071	100.00%
6.071	6.142	100.00%
6.142	6.194	98.50%
6.194	6.303	100.00%
6.303	6.452	100.00%
6.452	6.671	100.00%
6.671	6.797	100.00%
6.797	6.885	100.00%
6.885	7.010	100.00%
7.010	7.095	100.00%
7.095	7.234	100.00%
7.234	7.557	100.00%
7.557	7.706	100.00%
7.706	9.023	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112921\
Data File : PD067107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2021 16:47
Operator : AR\AJ
Sample : RESC007
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 05:31:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

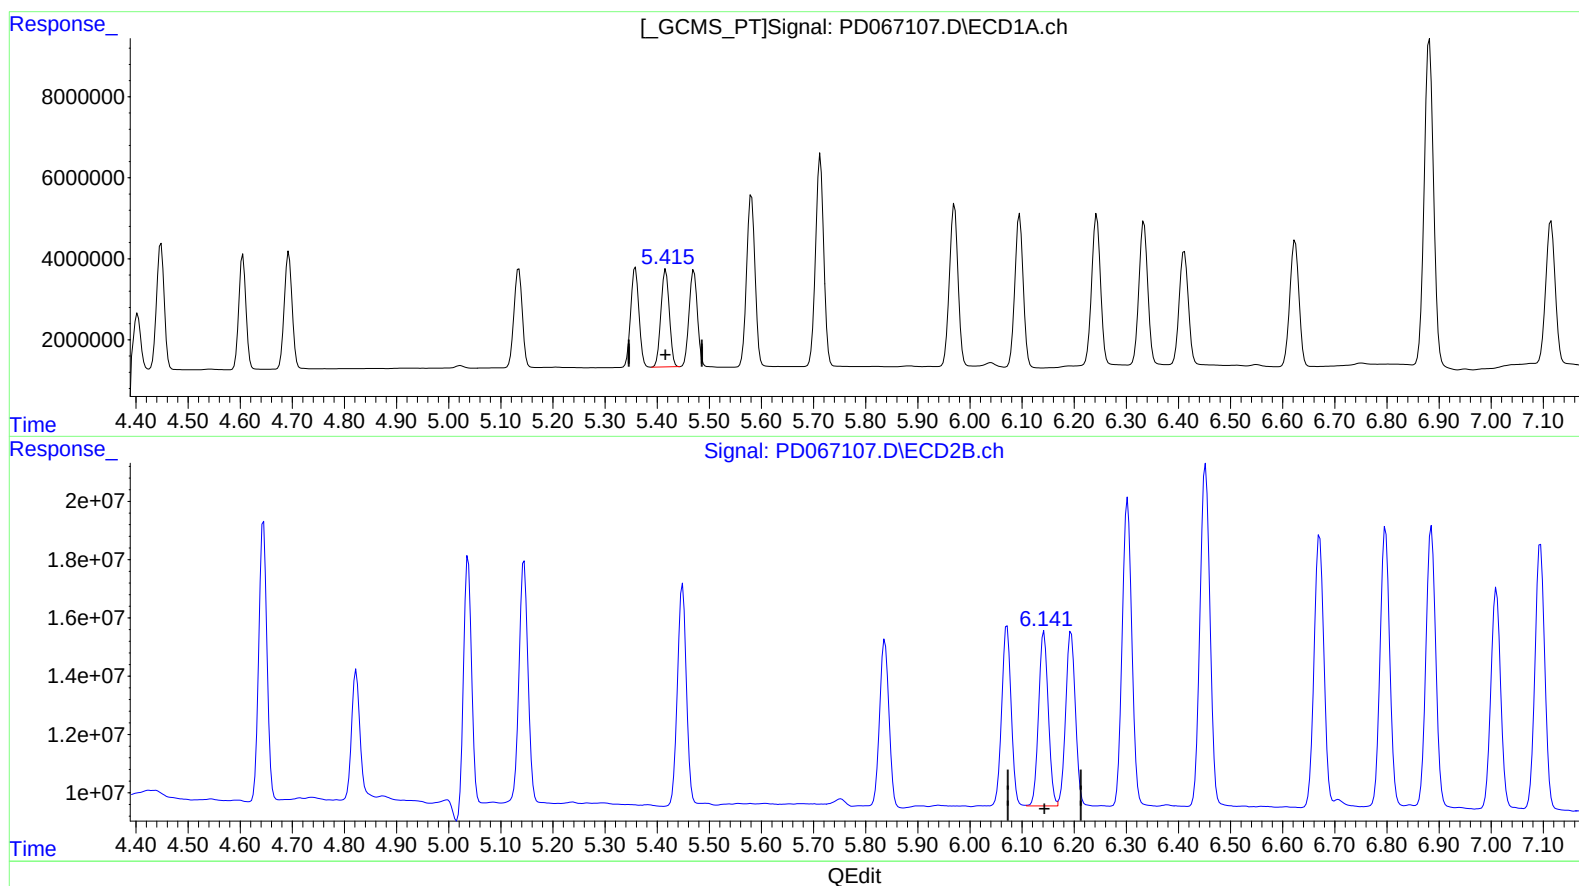

(11) cis-Chlordane (B)

5.417min 9.669 ng/ml

response 26829231

(11) cis-Chlordane #2 (B)

6.142min 10.428 ng/ml

response 77149255