

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113020\
 Data File : PD060399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2020 11:11
 Operator : DD\AJ
 Sample : L4862-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AZ1

Manual Integrations
 APPROVED

Ankita
 12/1/2020 12:11:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 00:22:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.023	10962567	35512130	9.627	9.659
2)	SA Decachlor...	8.295	9.110	19323645	41261617	14.269	14.236
Target Compounds							
11)	B cis-Chlor...	5.521	6.215	1081900	18621978	0.734	4.517 #
12)	B 4,4'-DDE	5.685	6.367	2519822	7410272	1.763	1.865
17)	MA 4,4'-DDT	6.445	7.157	3276850	5170522	2.683m	1.575m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113020\
Data File : PD060399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2020 11:11
Operator : DD\AJ
Sample : L4862-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 00:22:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

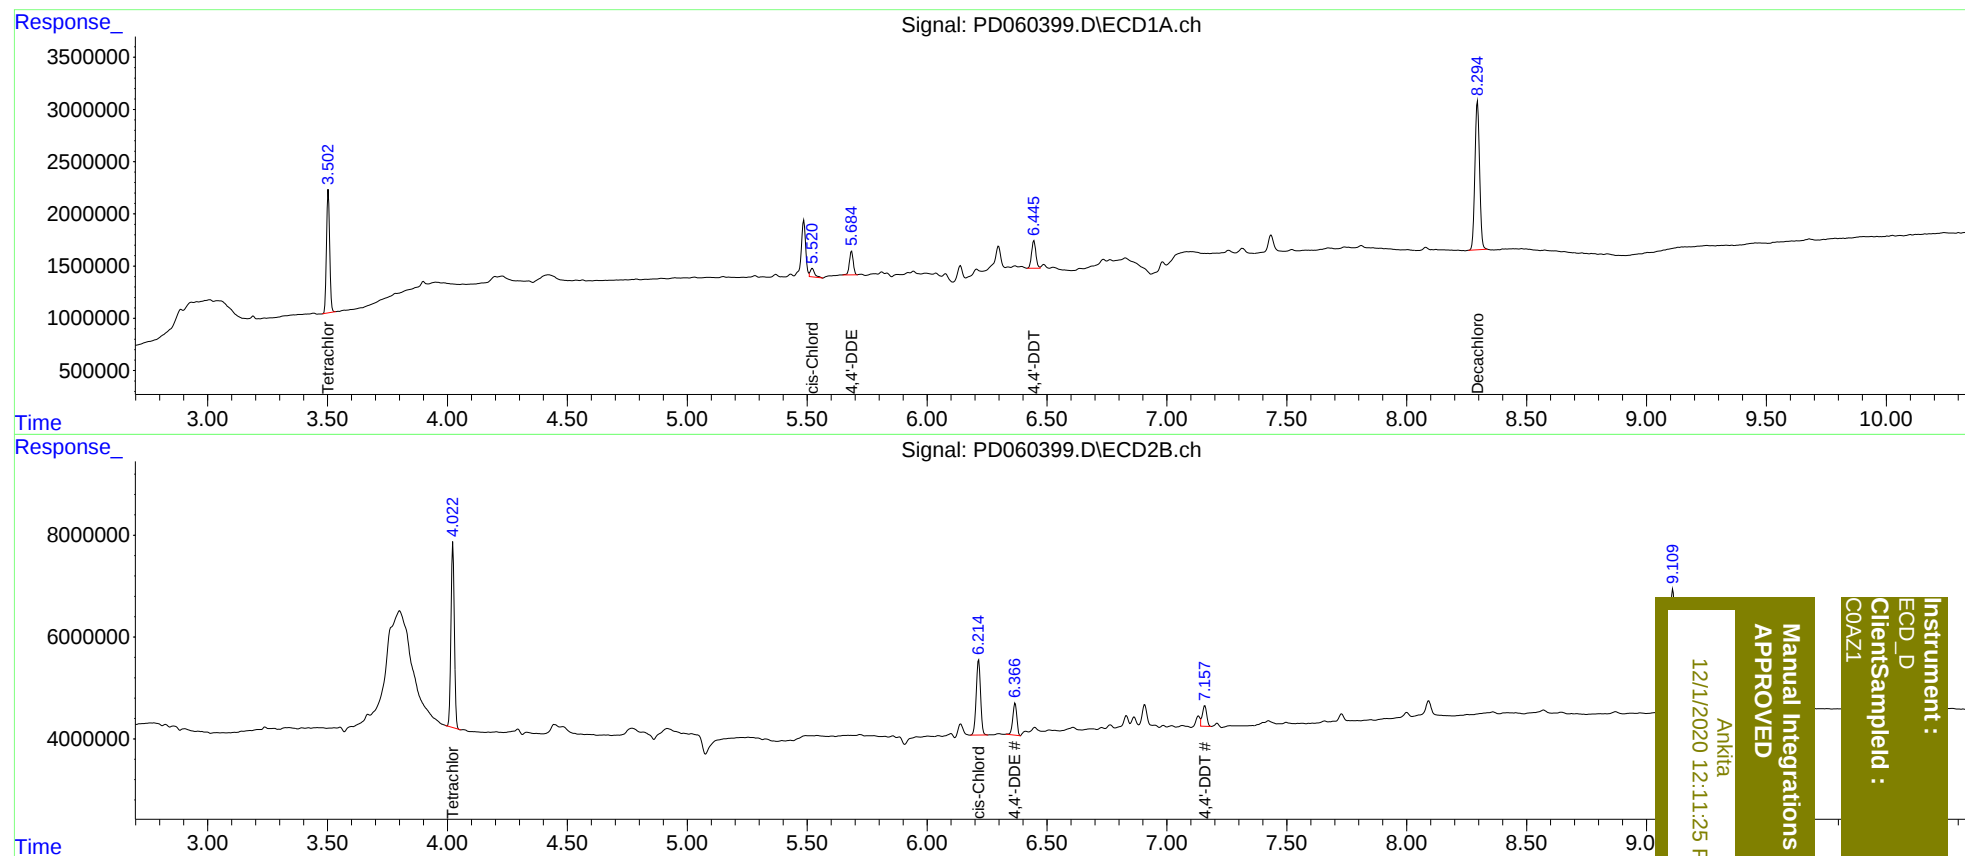

12/1/2020 12:11:25 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
C0A21