

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113020\
 Data File : PD060418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2020 15:37
 Operator : DD\AJ
 Sample : INDA325
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA325

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 05:09:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.023	26162597	85996676	22.975	23.391
27)	SA Decachlor...	8.296	9.111	61012248	124.9E6	45.054	43.089
Target Compounds							
2)	A alpha-BHC	3.944	4.414	37812266	127.0E6	23.055	23.296
3)	MA gamma-BHC...	4.230	4.700	35831094	116.0E6	23.012	23.441
4)	MA Heptachlor	4.537	5.212	36761292	110.3E6	23.546	22.758
9)	A Endosulfan I	5.576	6.264	32321597	90412122	23.472	23.113
13)	MA Dieldrin	5.822	6.521	71094460	195.9E6	46.709	46.190
14)	MA Endrin	6.081	6.740	55848632	148.8E6	44.867	42.886
16)	A 4,4'-DDD	6.205	6.859	59139647	158.3E6	48.616	47.795
17)	MA 4,4'-DDT	6.448	7.158	54634084	138.7E6	44.727	42.242
20)	A Methoxychlor	6.996	7.615	139.7E6	340.8E6	233.866	207.925

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113020\
Data File : PD060418.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2020 15:37
Operator : DD\AJ
Sample : INDA325
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 05:09:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

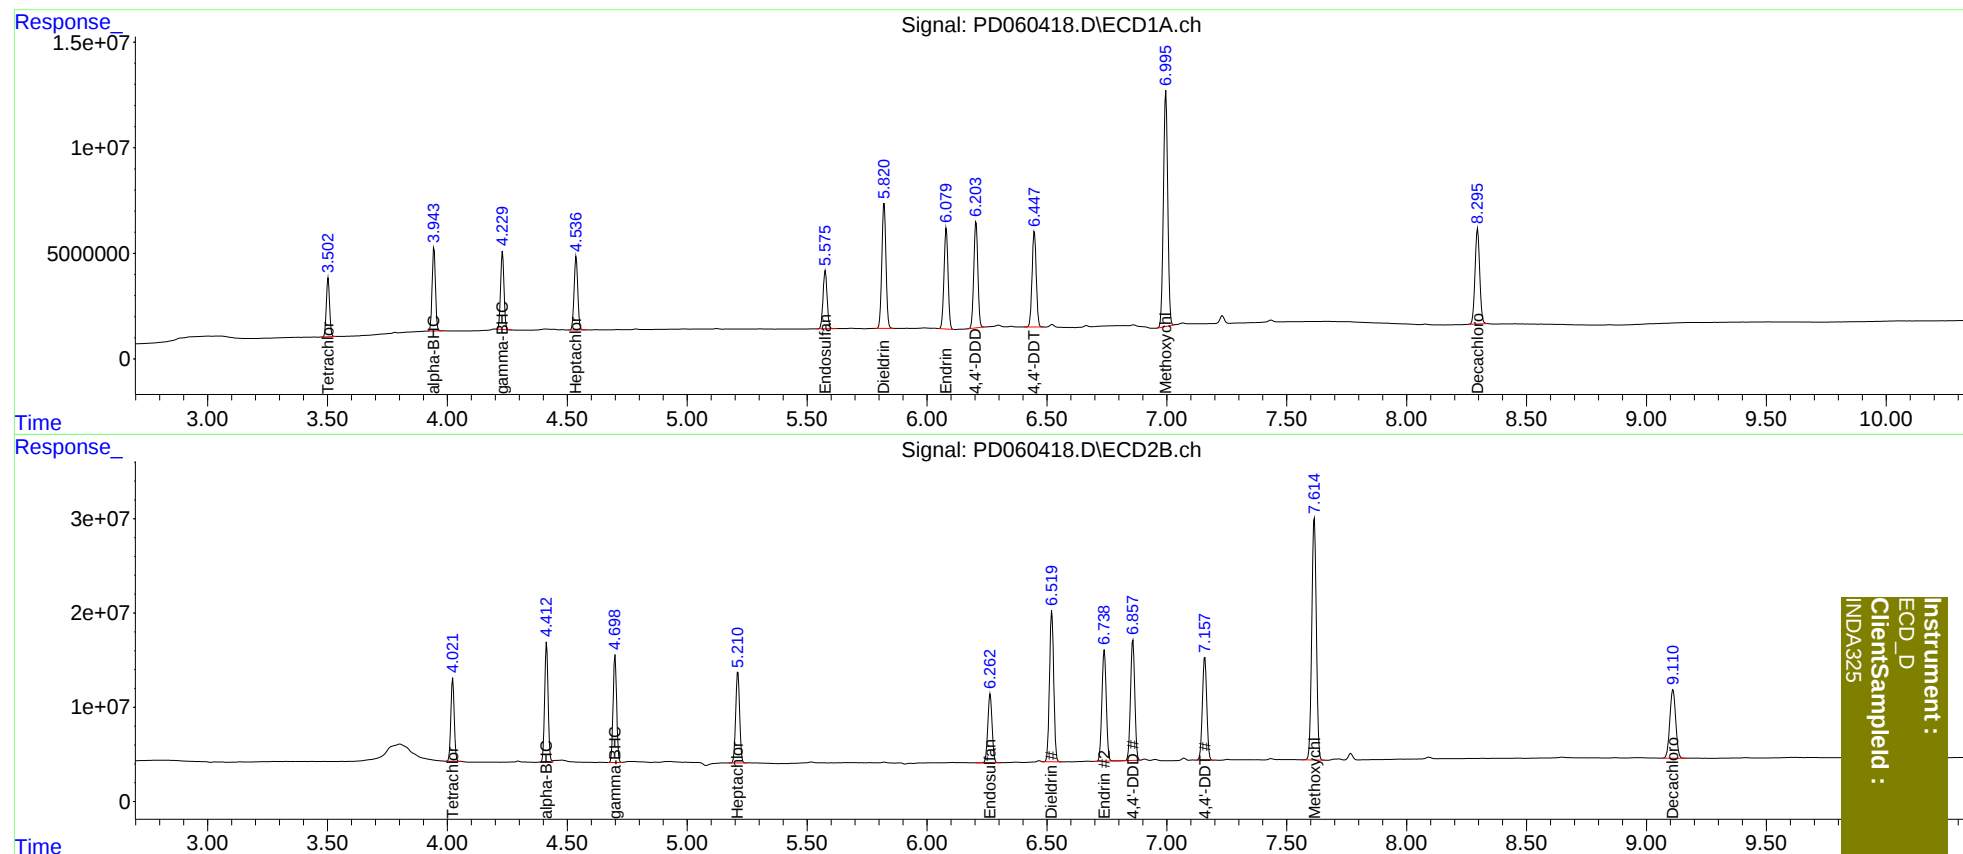

Instrument :
ECD_D
ClientSampled :
INDA325