

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113021\
 Data File : PD067134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 06:20
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 07:47:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 07:45:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	3.966	242.9E6	642.9E6	100.392	93.934
28)	SA Decachlor...	8.161	9.022	99882916	437.1E6	92.334	91.708
Target Compounds							
23)	Chlordane-1	4.298	4.956	79416693	253.7E6	987.250	969.526
24)	Chlordane-2	4.795	5.424	88088784	246.2E6	913.972	927.299
25)	Chlordane-3	5.358	6.071	277.9E6	898.7E6	1005.427	964.980
26)	Chlordane-4	5.415	6.143	227.7E6	1035.6E6	1009.163	956.040
27)	Chlordane-5	6.249	6.952	87938646	204.6E6	970.874	950.054



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113021\
Data File : PD067134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 06:20
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 07:47:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 07:45:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

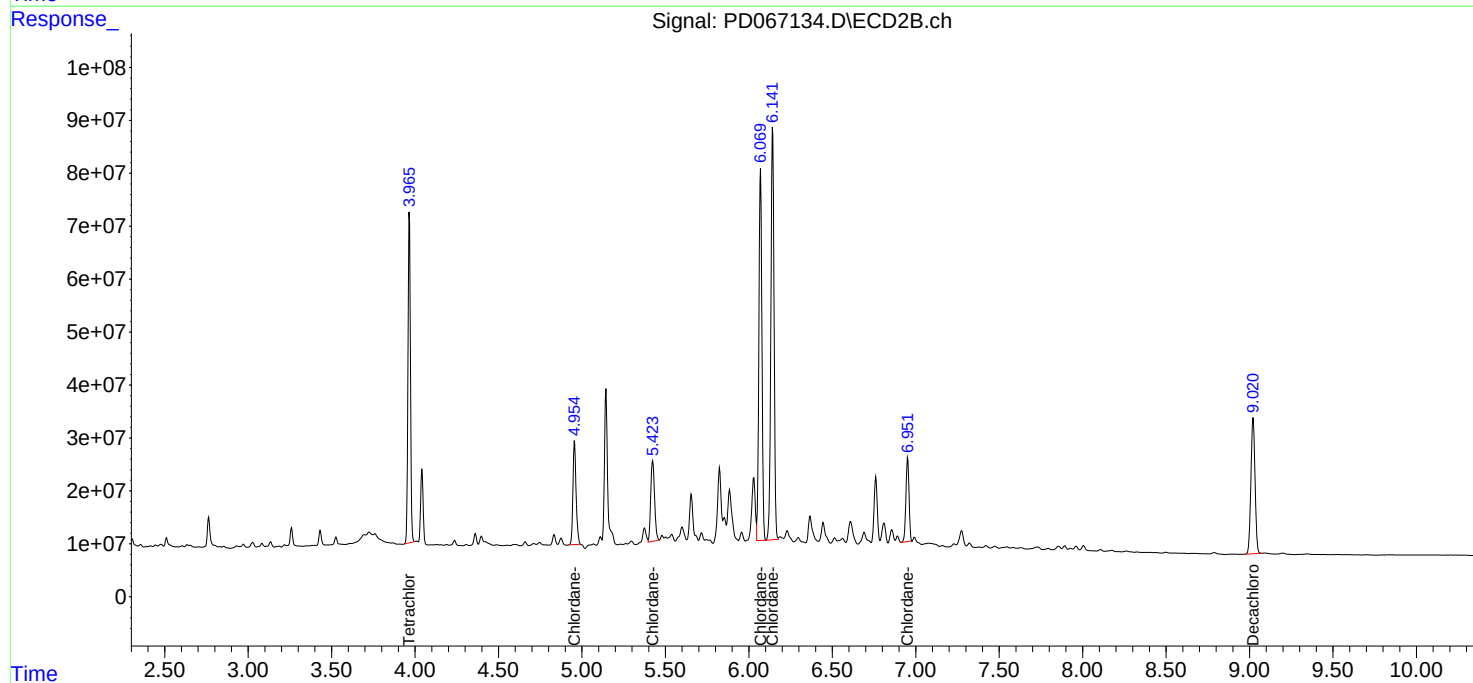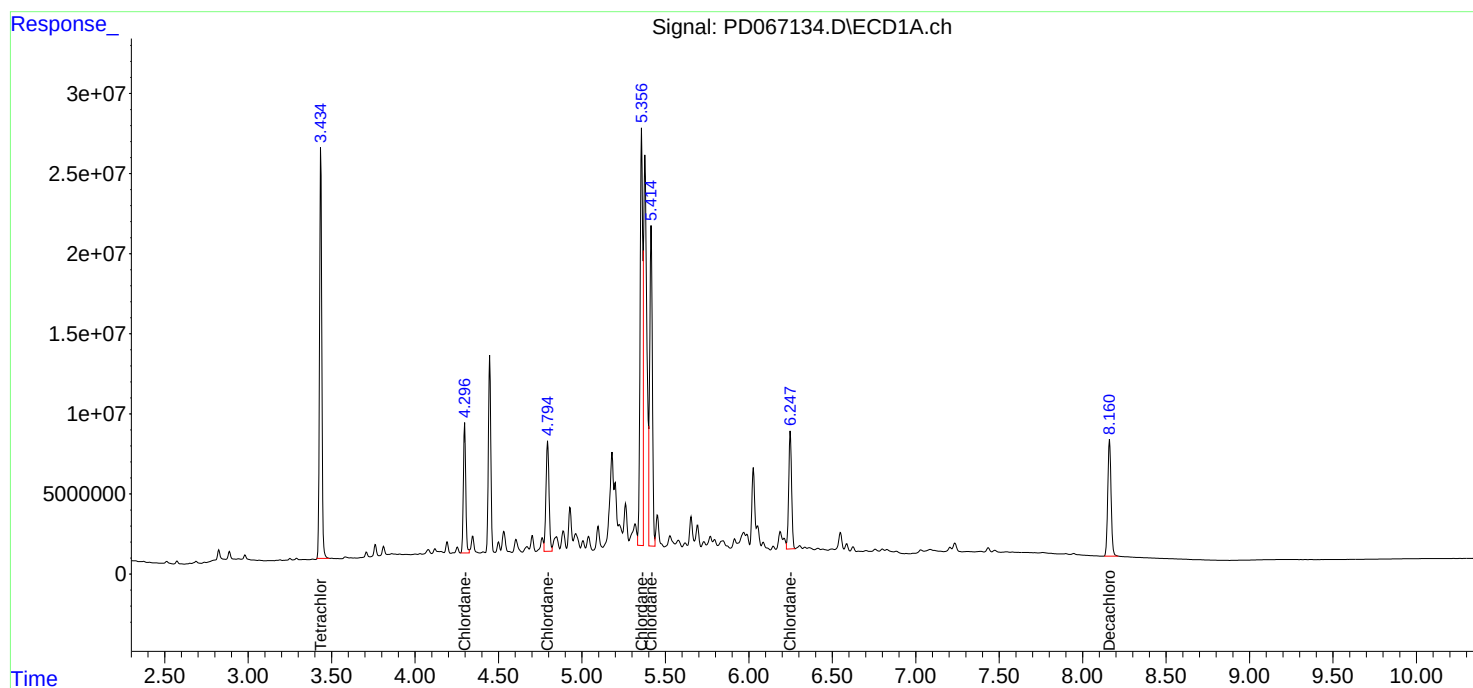


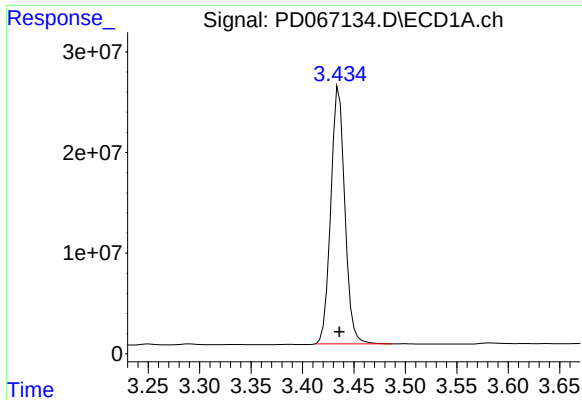

#1 Tetrachloro-m-xylene


R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 242935429
Conc: 100.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

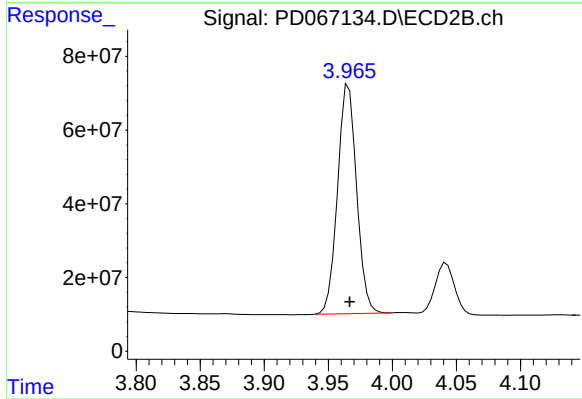


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 642899610
Conc: 93.93 ng/ml

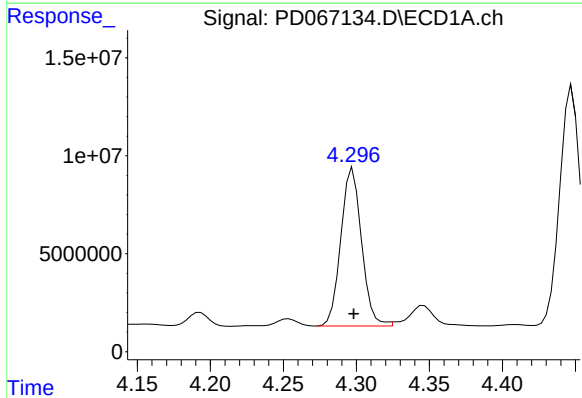


#23 Chlordane-1

R.T.: 4.298 min
Delta R.T.: 0.000 min
Response: 79416693
Conc: 987.25 ng/ml

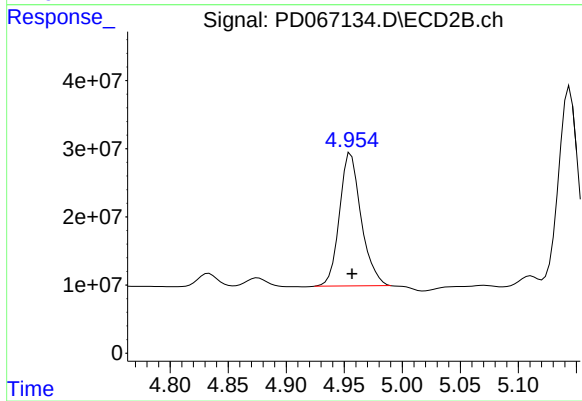

#23 Chlordane-1


R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 253707075
Conc: 969.53 ng/ml

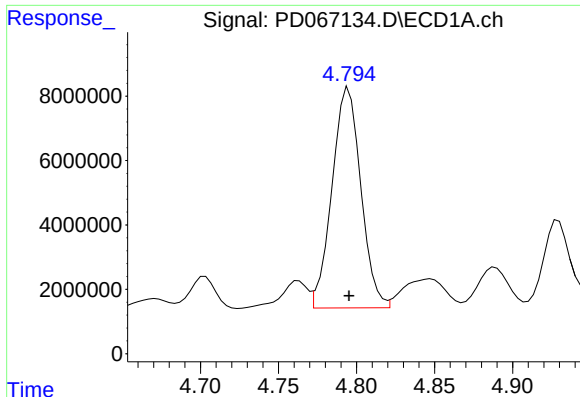

#24 Chlordane-2


R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 88088784
Conc: 913.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

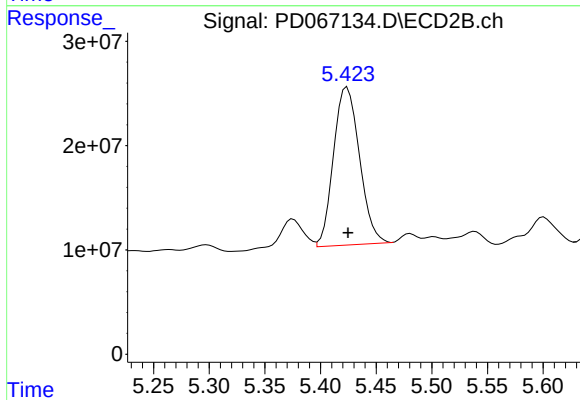


#24 Chlordane-2

R.T.: 5.424 min
Delta R.T.: 0.000 min
Response: 246193024
Conc: 927.30 ng/ml

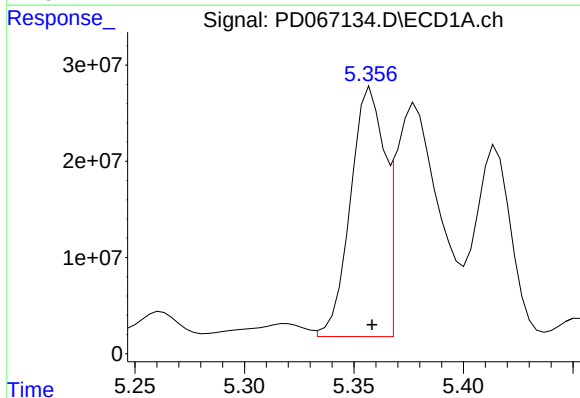


#25 Chlordane-3

R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 277947802
Conc: 1005.43 ng/ml

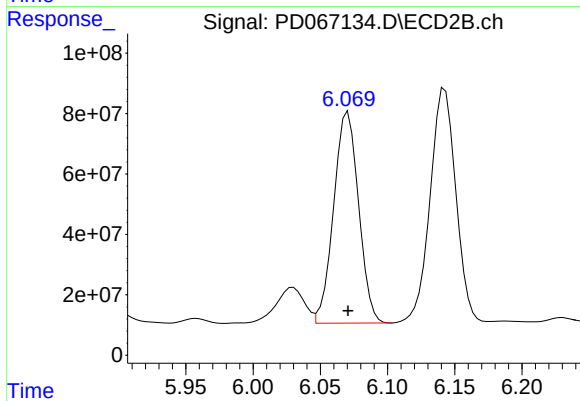

#25 Chlordane-3


R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 898701180
Conc: 964.98 ng/ml

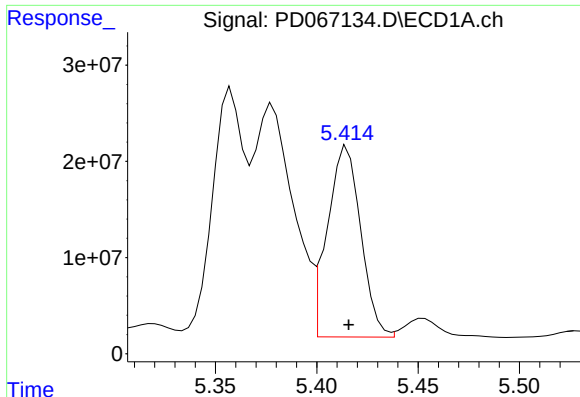

#26 Chlordane-4


R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 227683040
Conc: 1009.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

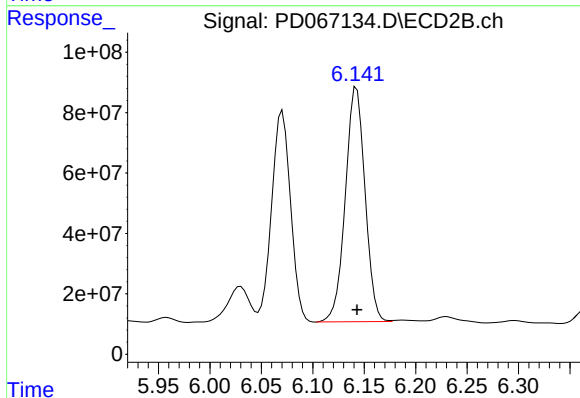


#26 Chlordane-4

R.T.: 6.143 min
Delta R.T.: 0.000 min
Response: 1035636156
Conc: 956.04 ng/ml

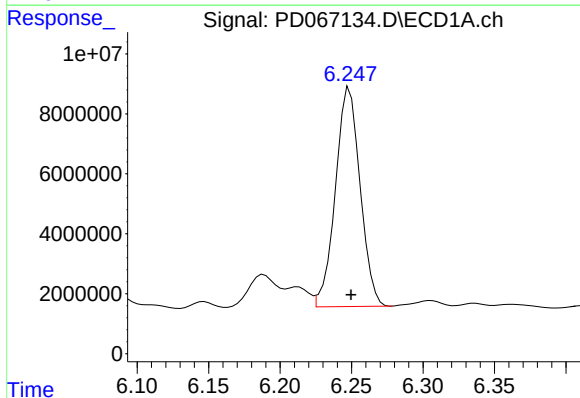


#27 Chlordane-5

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 87938646
Conc: 970.87 ng/ml

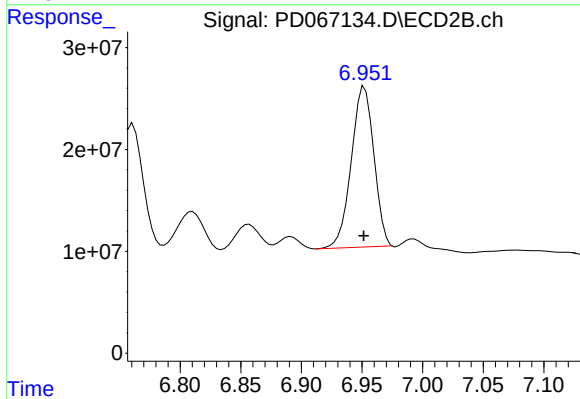

#27 Chlordane-5


R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 204613994
Conc: 950.05 ng/ml

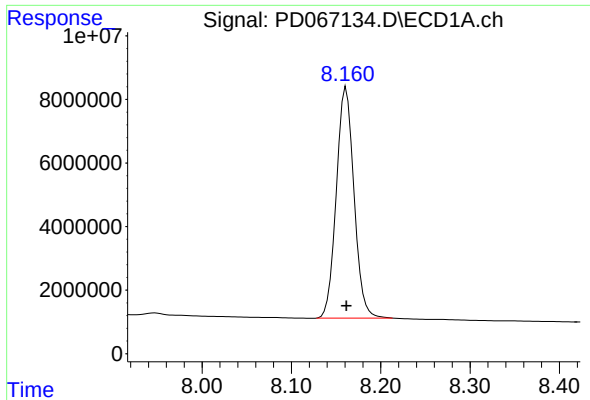

#28 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 99882916
Conc: 92.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

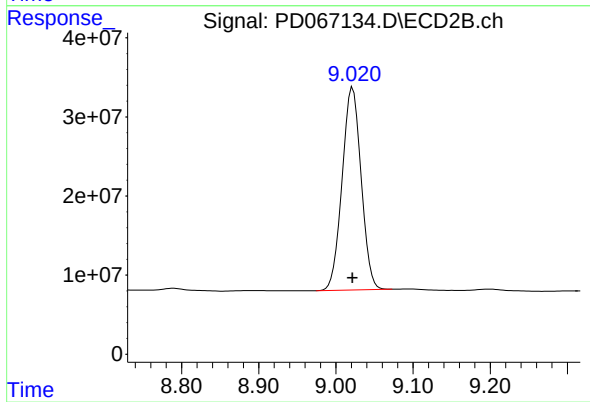

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 437053605
Conc: 91.71 ng/ml