

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113021\
 Data File : PD067135.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 06:34
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 07:47:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 07:45:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	3.966	176.6E6	478.3E6	72.999	69.886
28)	SA Decachlor...	8.162	9.021	75658608	333.1E6	69.941	69.886
Target Compounds							
23)	Chlordane-1	4.298	4.956	57299872	186.8E6	712.310	713.714
24)	Chlordane-2	4.795	5.424	65934292	184.5E6	684.107	695.064
25)	Chlordane-3	5.358	6.070	200.0E6	660.7E6	723.571	709.476
26)	Chlordane-4	5.416	6.143	163.6E6	764.9E6	725.174	706.151
27)	Chlordane-5	6.249	6.952	64956186	151.1E6	717.139	701.488



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113021\
Data File : PD067135.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 06:34
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 07:47:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 07:45:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

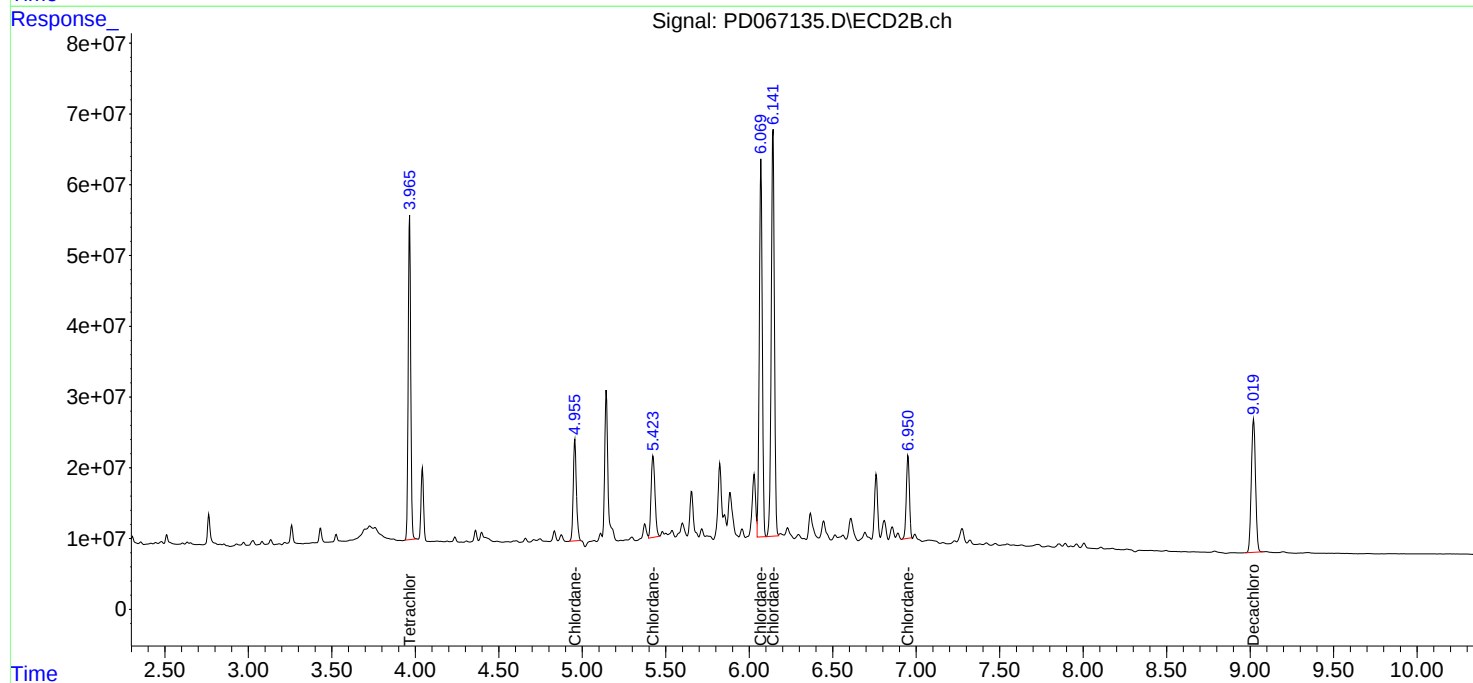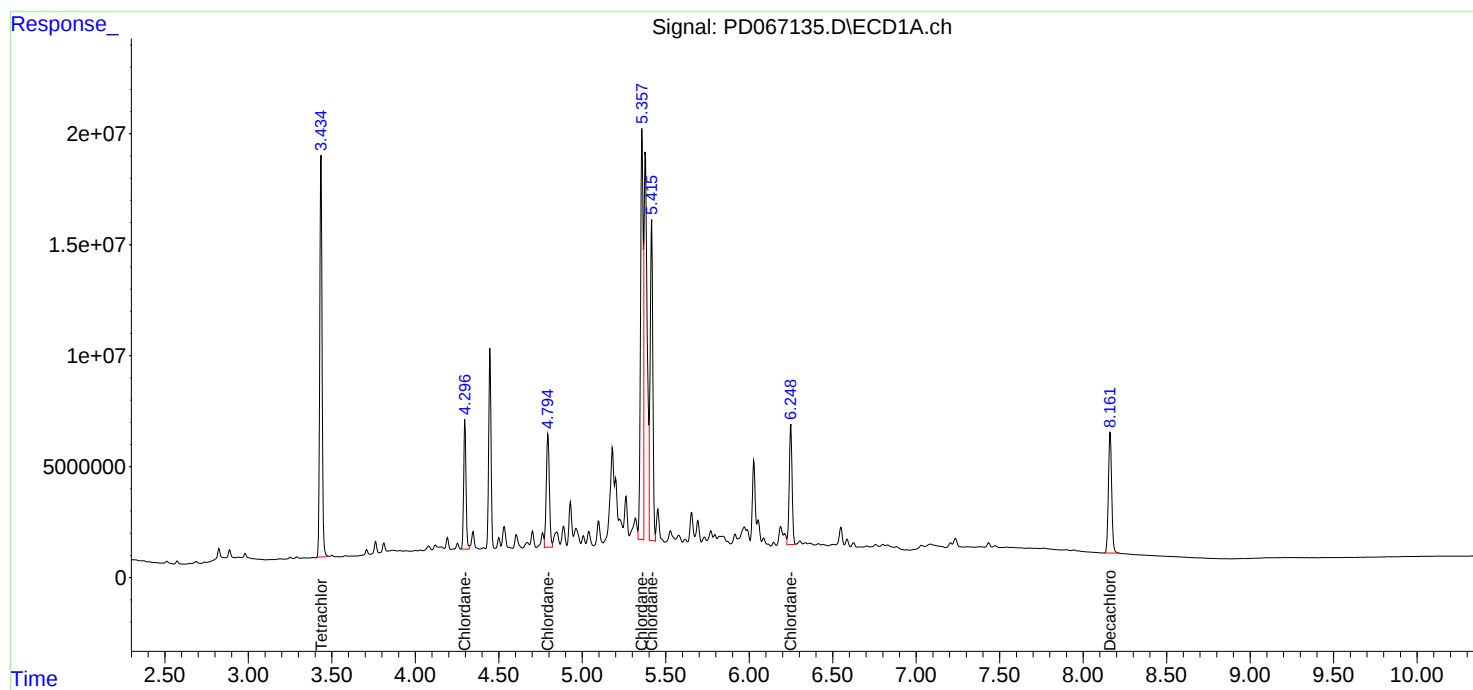


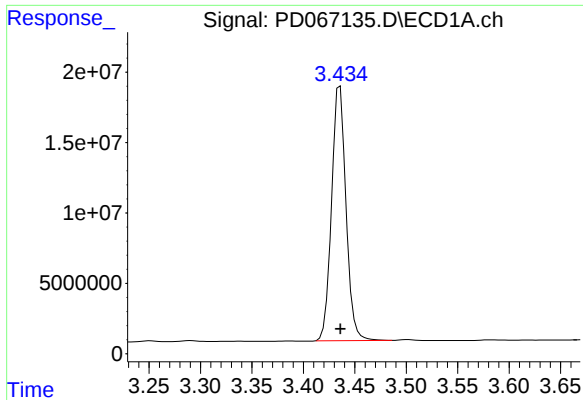

#1 Tetrachloro-m-xylene


R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 176648352
Conc: 73.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

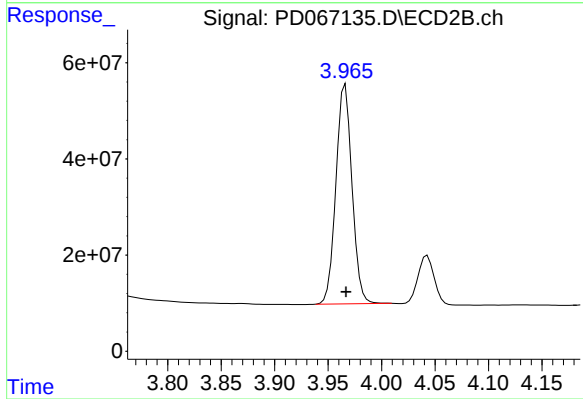


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 478312438
Conc: 69.89 ng/ml

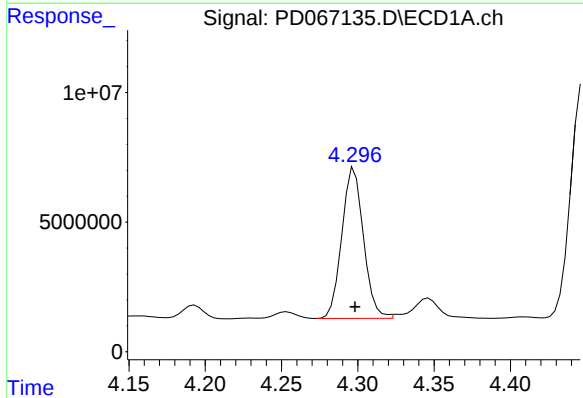


#23 Chlordane-1

R.T.: 4.298 min
Delta R.T.: 0.000 min
Response: 57299872
Conc: 712.31 ng/ml

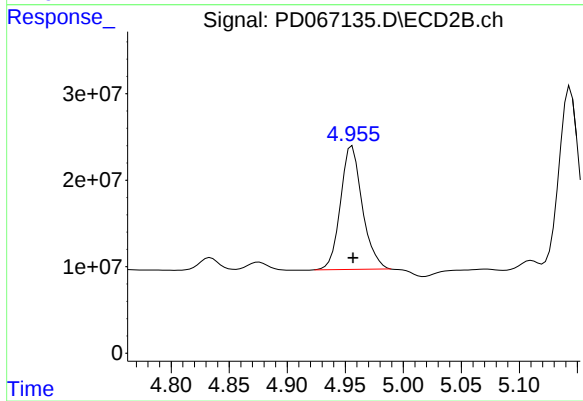

#23 Chlordane-1


R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 186765786
Conc: 713.71 ng/ml

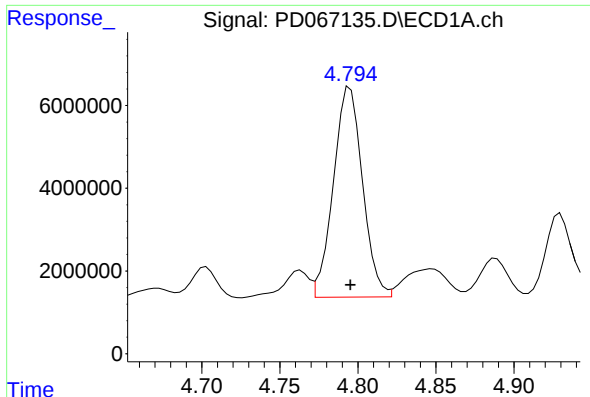

#24 Chlordane-2


R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 65934292
Conc: 684.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

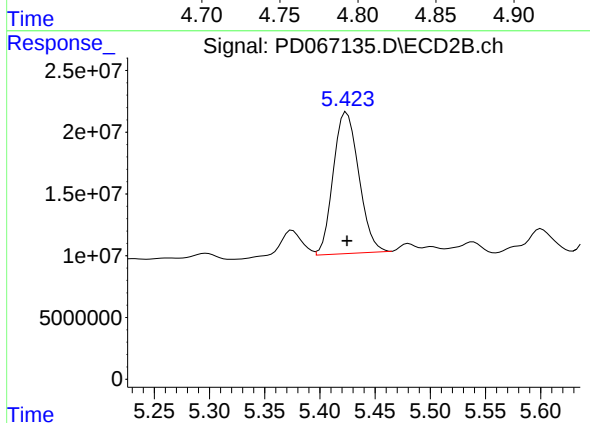


#24 Chlordane-2

R.T.: 5.424 min
Delta R.T.: 0.000 min
Response: 184535889
Conc: 695.06 ng/ml

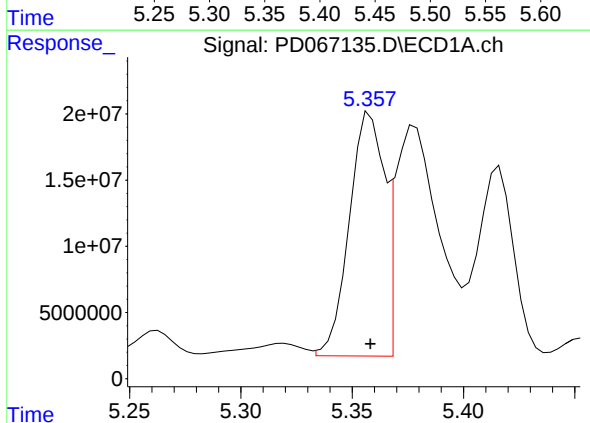


#25 Chlordane-3

R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 200029252
Conc: 723.57 ng/ml

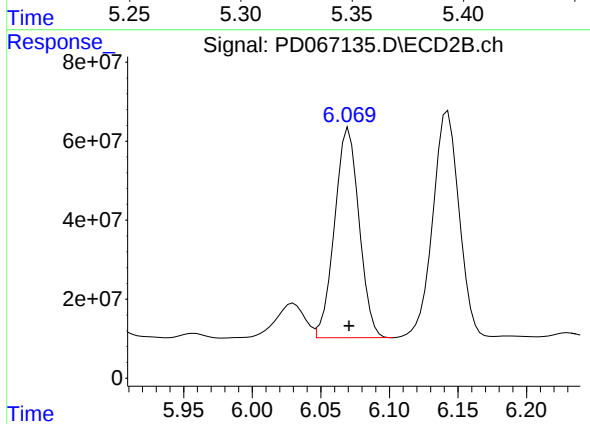

#25 Chlordane-3


R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 660745842
Conc: 709.48 ng/ml

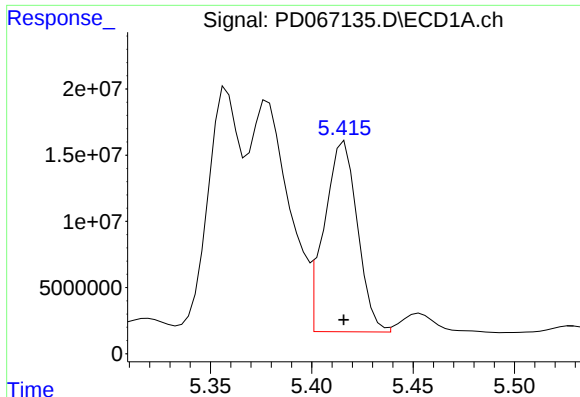

#26 Chlordane-4


R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 163610687
Conc: 725.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

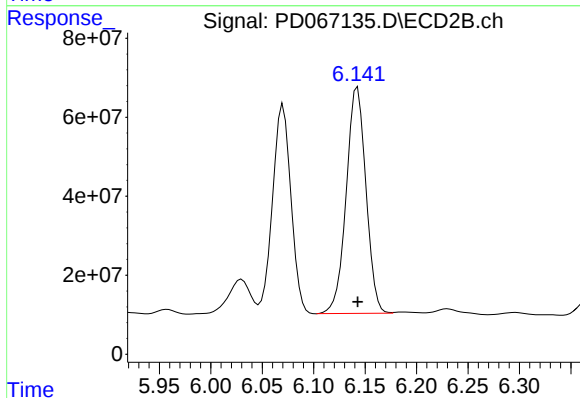


#26 Chlordane-4

R.T.: 6.143 min
Delta R.T.: 0.000 min
Response: 764942282
Conc: 706.15 ng/ml

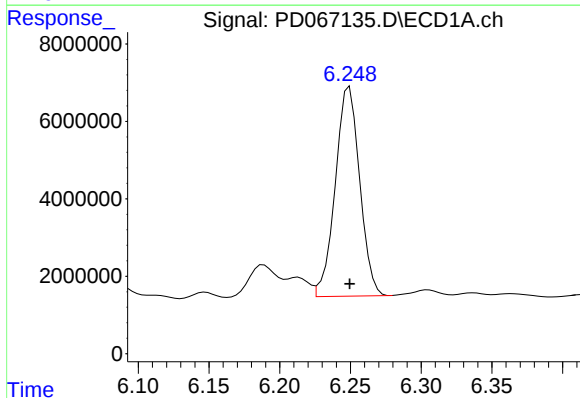


#27 Chlordane-5

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 64956186
Conc: 717.14 ng/ml

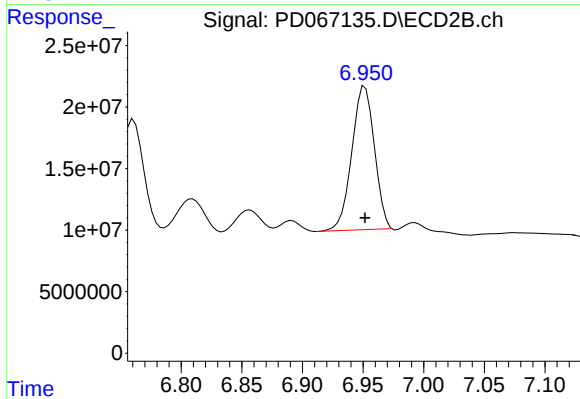

#27 Chlordane-5


R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 151080190
Conc: 701.49 ng/ml

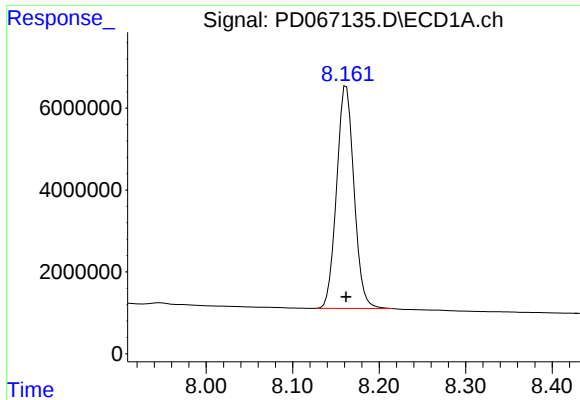

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 75658608
Conc: 69.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

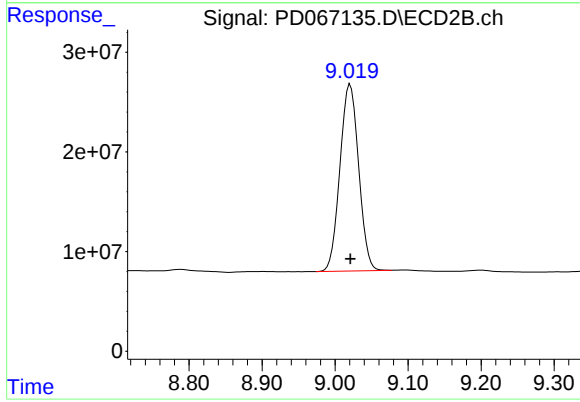

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 333057783
Conc: 69.89 ng/ml