

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113021\
 Data File : PD067136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 06:48
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 07:47:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 07:45:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	3.967	121.0E6	342.2E6	50.000	50.000
28)	SA Decachlor...	8.162	9.021	54087572	238.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.298	4.957	40221180	130.8E6	500.000	500.000
24)	Chlordane-2	4.795	5.425	48190063	132.7E6	500.000	500.000
25)	Chlordane-3	5.358	6.071	138.2E6	465.7E6	500.000	500.000
26)	Chlordane-4	5.416	6.143	112.8E6	541.6E6	500.000	500.000
27)	Chlordane-5	6.250	6.952	45288392	107.7E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113021\
Data File : PD067136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 06:48
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 07:47:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 07:45:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

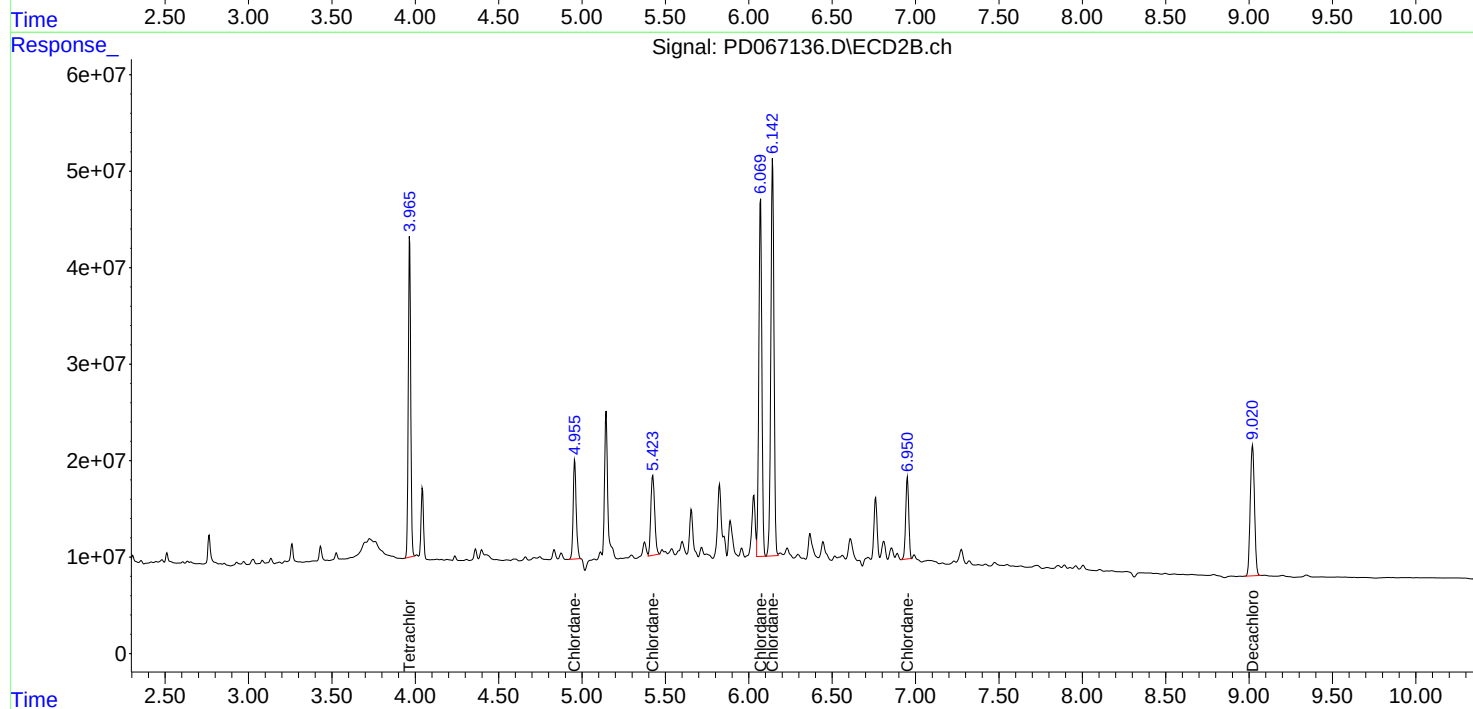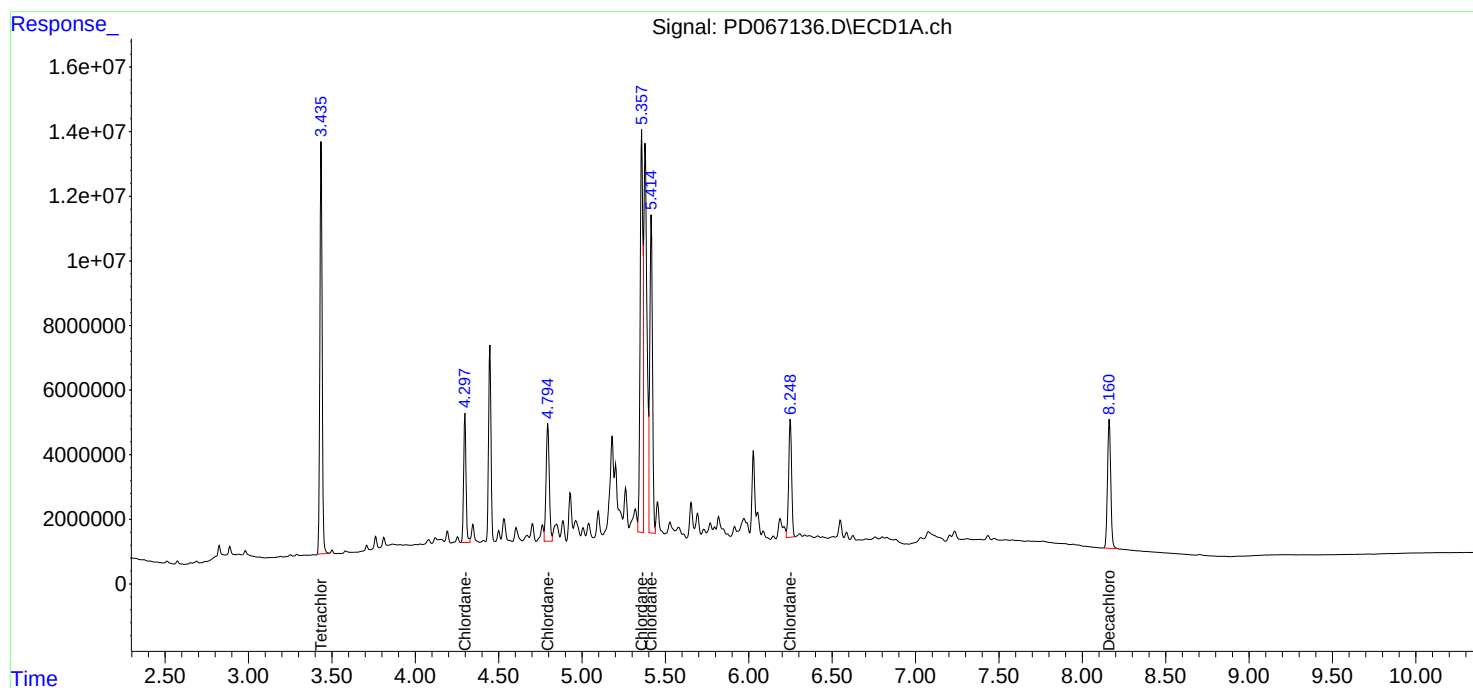


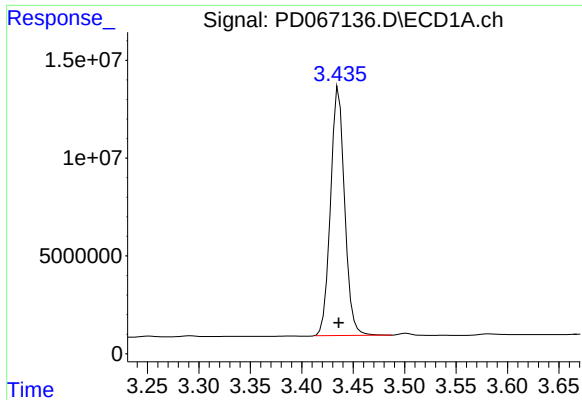

#1 Tetrachloro-m-xylene


R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 120993483
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

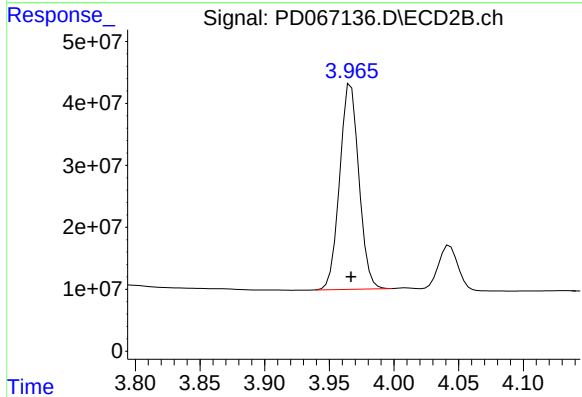


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 342208225
Conc: 50.00 ng/ml

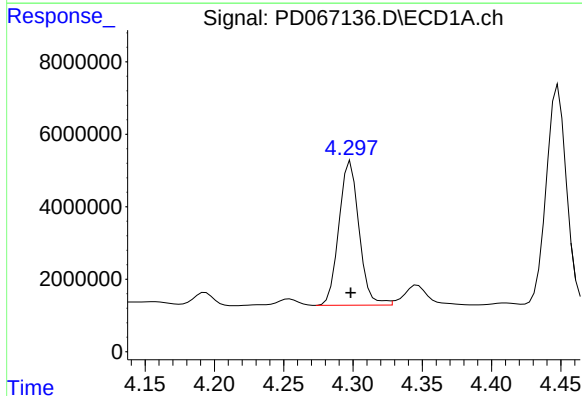


#23 Chlordane-1

R.T.: 4.298 min
Delta R.T.: 0.000 min
Response: 40221180
Conc: 500.00 ng/ml

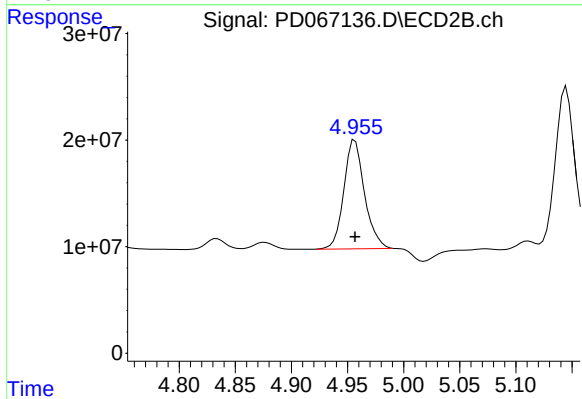

#23 Chlordane-1


R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 130840728
Conc: 500.00 ng/ml

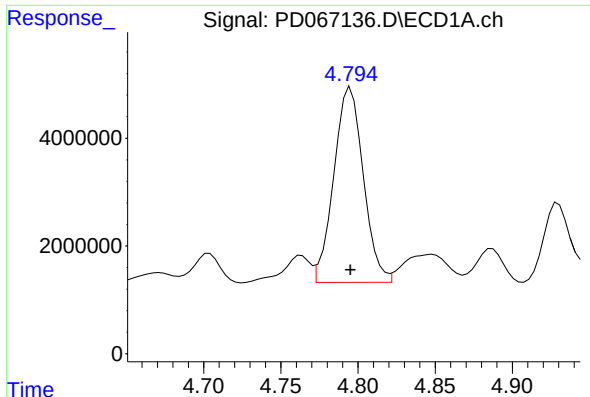

#24 Chlordane-2


R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 48190063
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

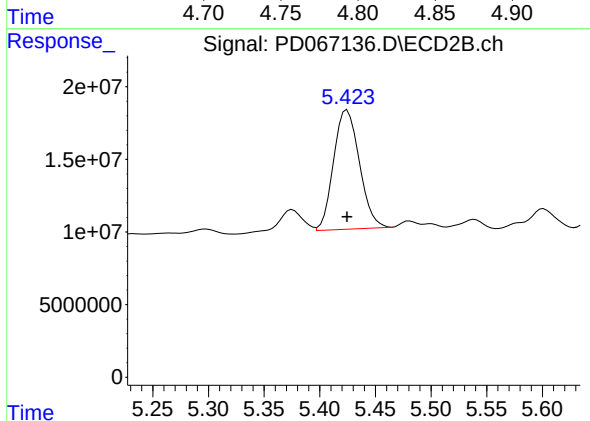


#24 Chlordane-2

R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 132747368
Conc: 500.00 ng/ml

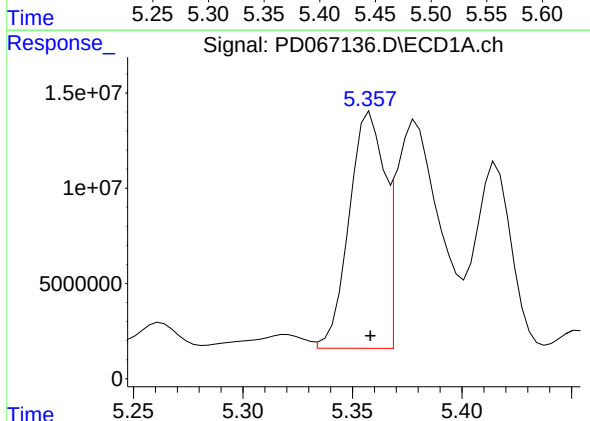


#25 Chlordane-3

R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 138223735
Conc: 500.00 ng/ml

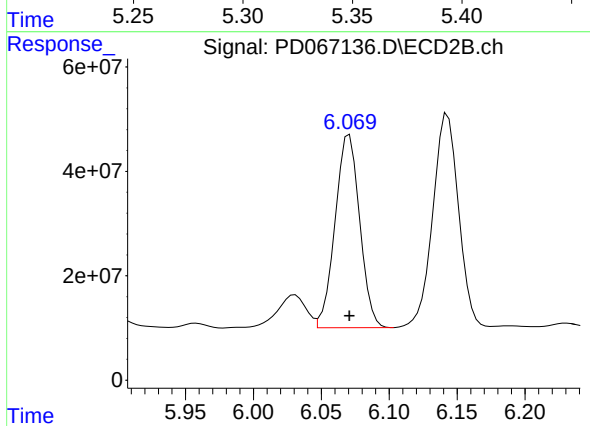

#25 Chlordane-3


R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 465657878
Conc: 500.00 ng/ml

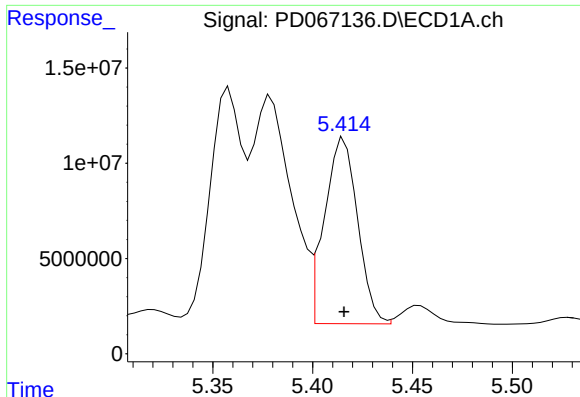

#26 Chlordane-4


R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 112807835
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

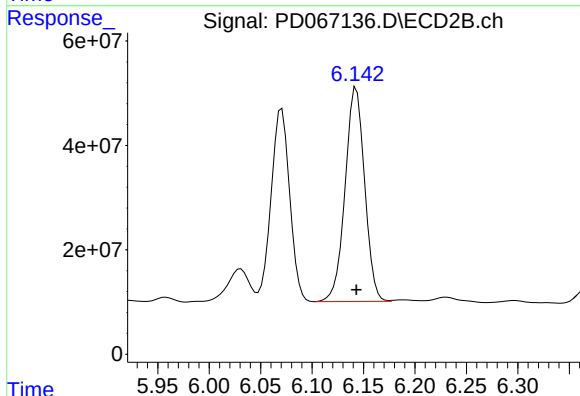


#26 Chlordane-4

R.T.: 6.143 min
Delta R.T.: 0.000 min
Response: 541628246
Conc: 500.00 ng/ml

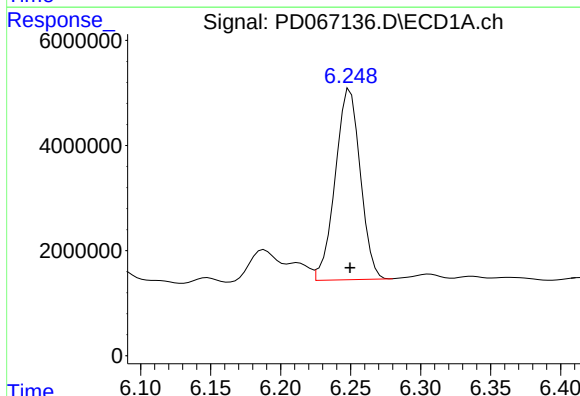


#27 Chlordane-5

R.T.: 6.250 min
Delta R.T.: 0.000 min
Response: 45288392
Conc: 500.00 ng/ml

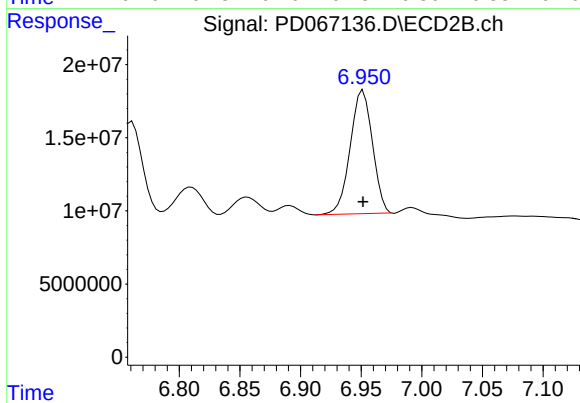

#27 Chlordane-5


R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 107685472
Conc: 500.00 ng/ml

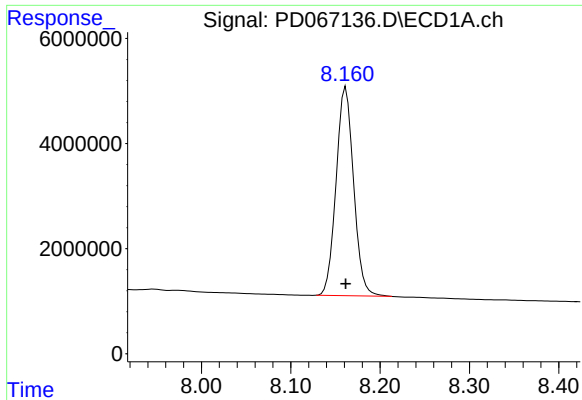

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 54087572
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

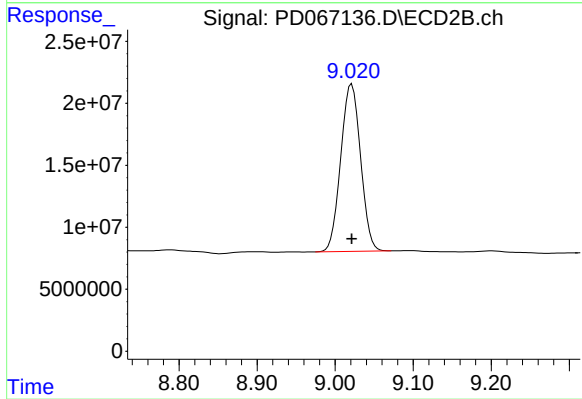

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 238286542
Conc: 50.00 ng/ml