

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113021\
 Data File : PD067137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 07:02
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 07:48:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 07:45:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	3.966	58067424	179.3E6	23.996	26.191
28)	SA Decachlor...	8.162	9.021	28343348	123.5E6	26.201	25.915
Target Compounds							
23)	Chlordane-1	4.297	4.956	19549189	64473382	243.021	246.381
24)	Chlordane-2	4.795	5.425	24776366	67973851	257.069	256.027
25)	Chlordane-3	5.358	6.070	65981757	233.8E6	238.677	251.004
26)	Chlordane-4	5.415	6.142	55089043	274.7E6	244.172	253.614
27)	Chlordane-5	6.249	6.952	22475017	53280281	248.132	247.388



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD113021\
Data File : PD067137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 07:02
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 07:48:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 07:45:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

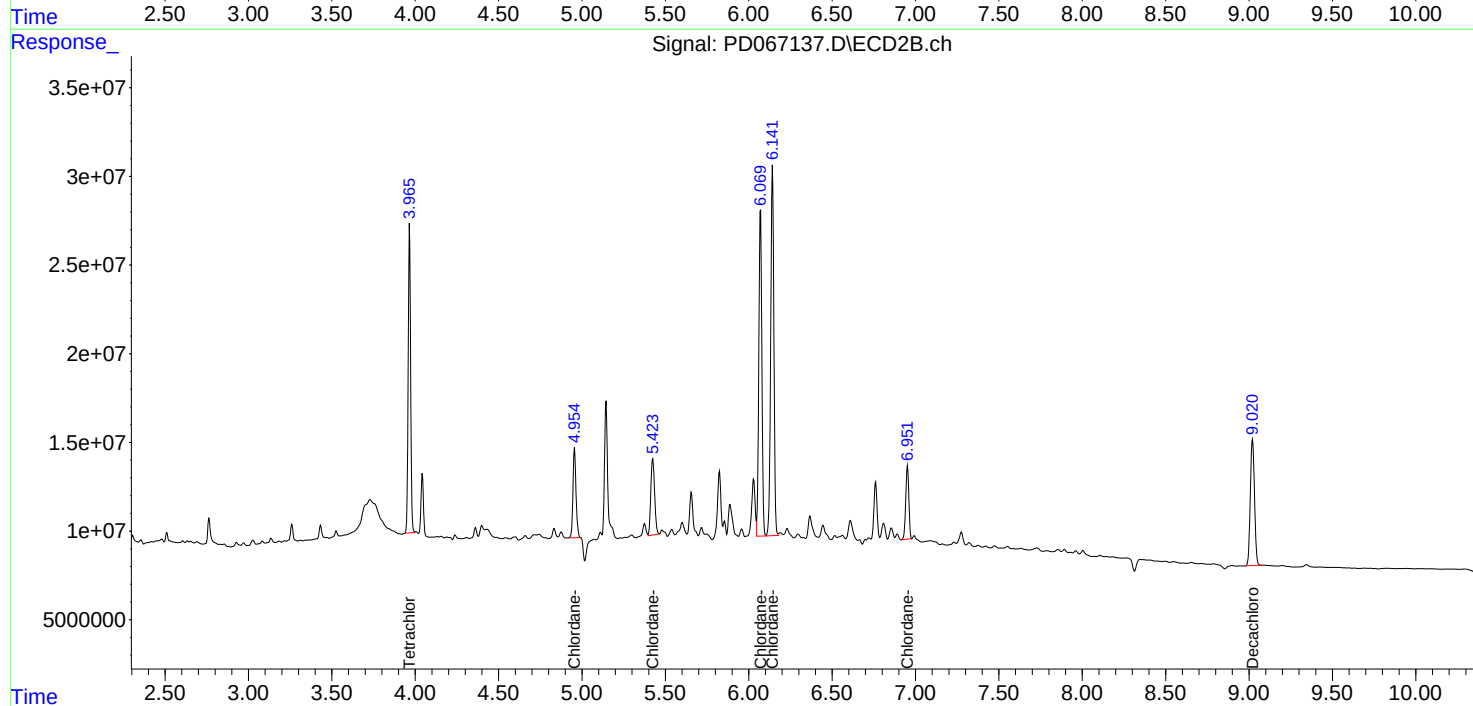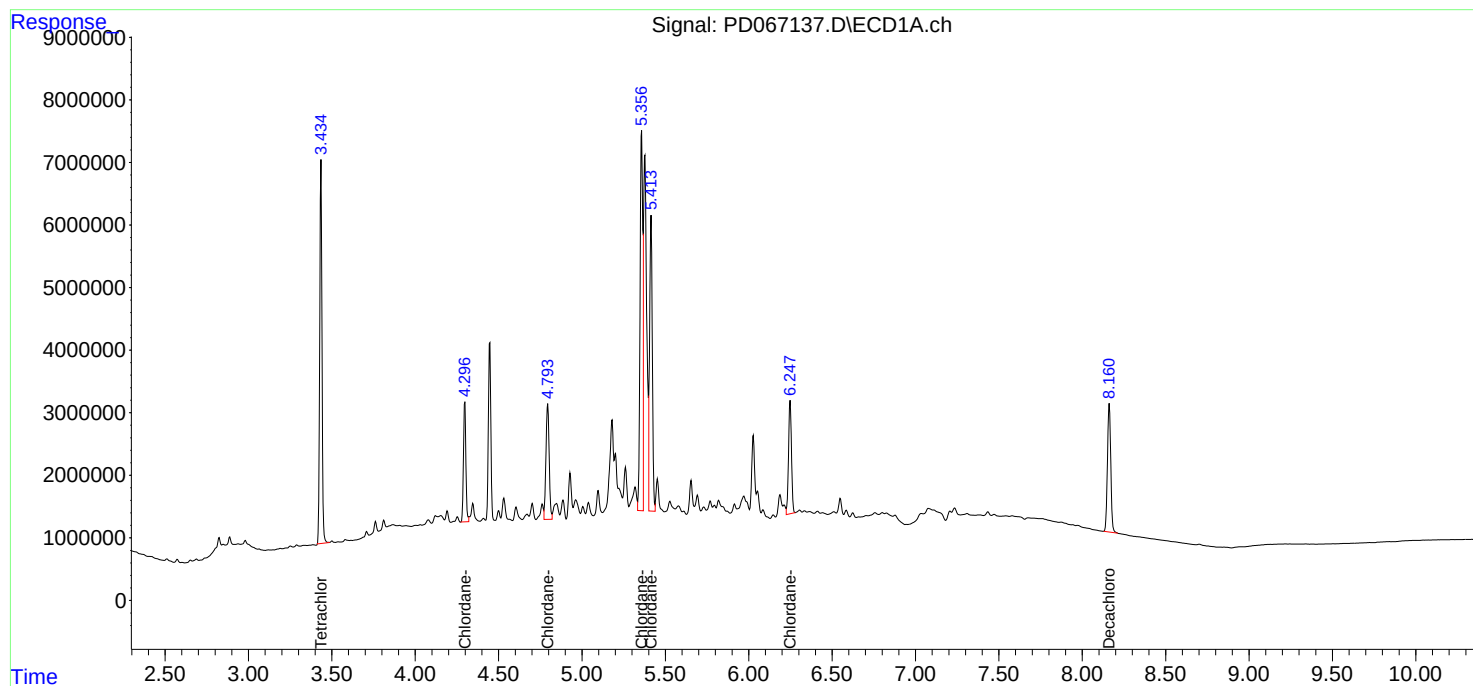


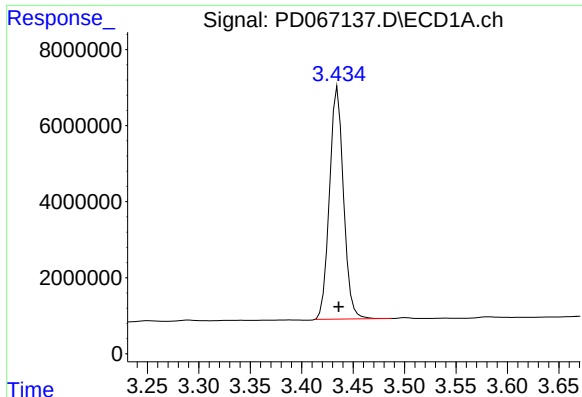

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 58067424
Conc: 24.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

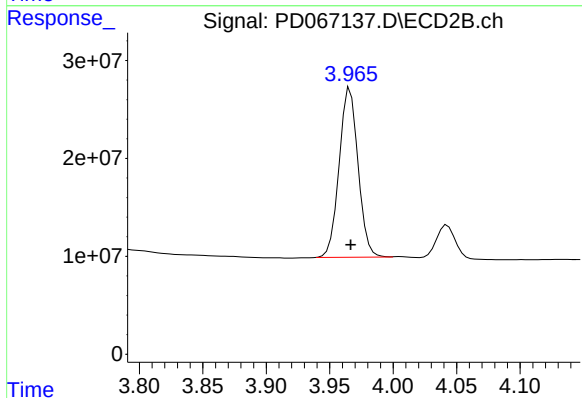


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 179255787
Conc: 26.19 ng/ml

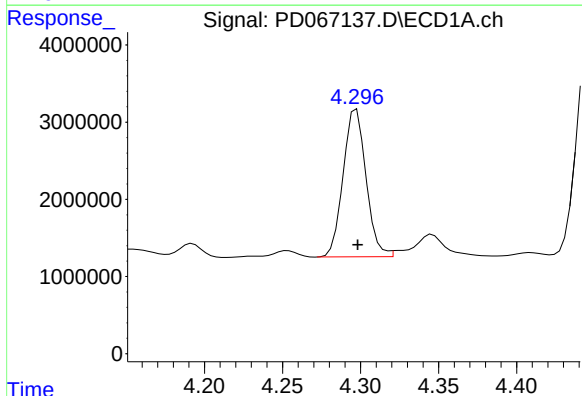


#23 Chlordane-1

R.T.: 4.297 min
Delta R.T.: 0.000 min
Response: 19549189
Conc: 243.02 ng/ml

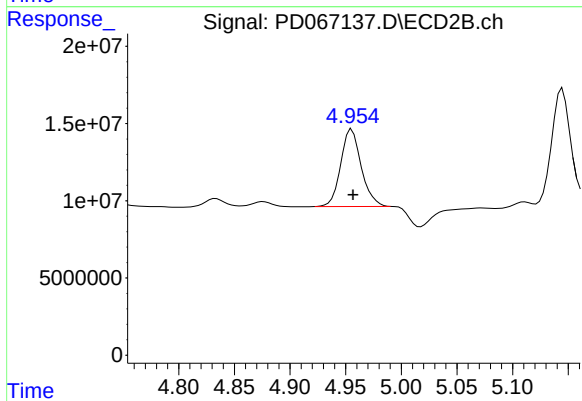

#23 Chlordane-1


R.T.: 4.956 min
Delta R.T.: -0.001 min
Response: 64473382
Conc: 246.38 ng/ml

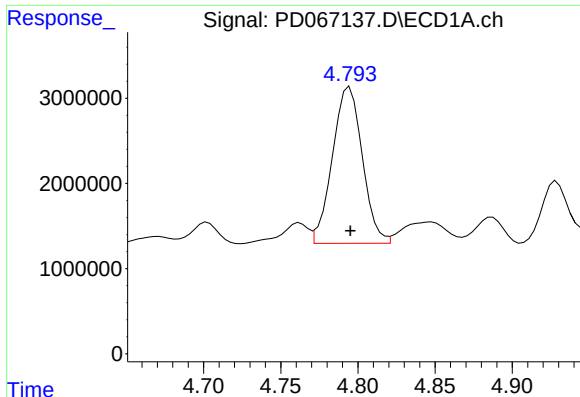

#24 Chlordane-2


R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 24776366
Conc: 257.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

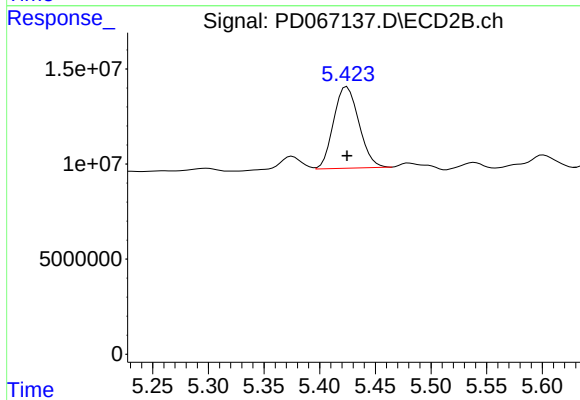


#24 Chlordane-2

R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 67973851
Conc: 256.03 ng/ml

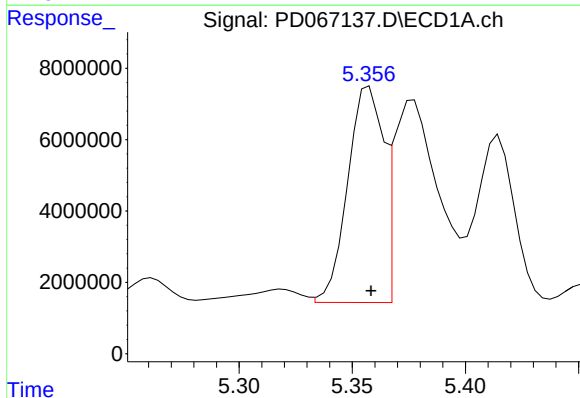


#25 Chlordane-3

R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 65981757
Conc: 238.68 ng/ml

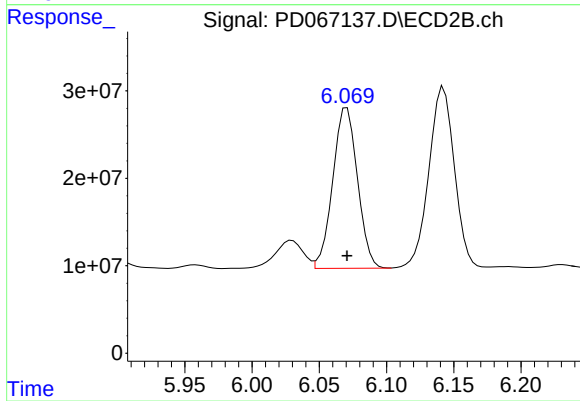

#25 Chlordane-3


R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 233763914
Conc: 251.00 ng/ml

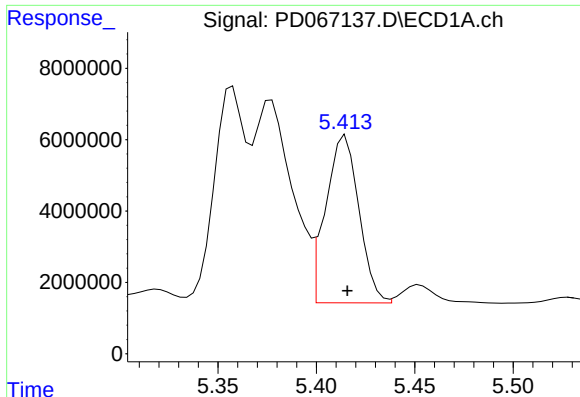

#26 Chlordane-4


R.T.: 5.415 min
Delta R.T.: -0.001 min
Response: 55089043
Conc: 244.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

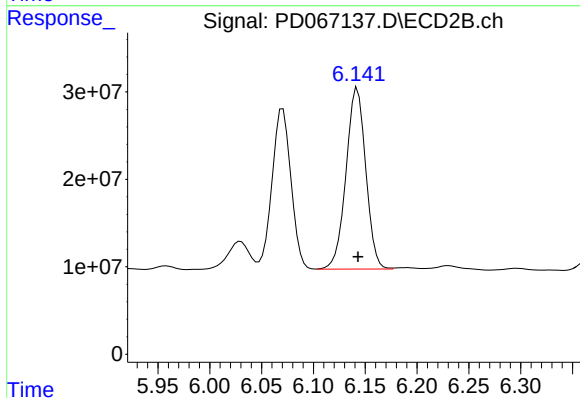


#26 Chlordane-4

R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 274729273
Conc: 253.61 ng/ml

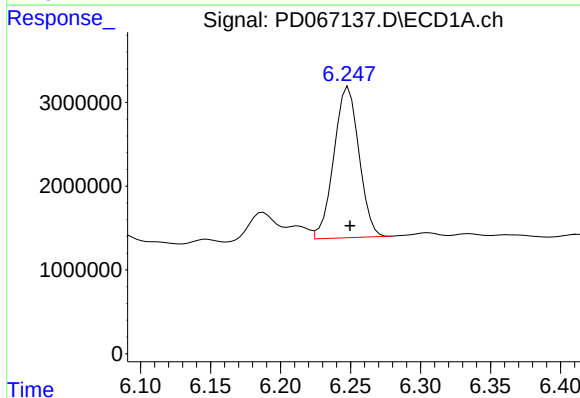


#27 Chlordane-5

R.T.: 6.249 min
Delta R.T.: -0.001 min
Response: 22475017
Conc: 248.13 ng/ml

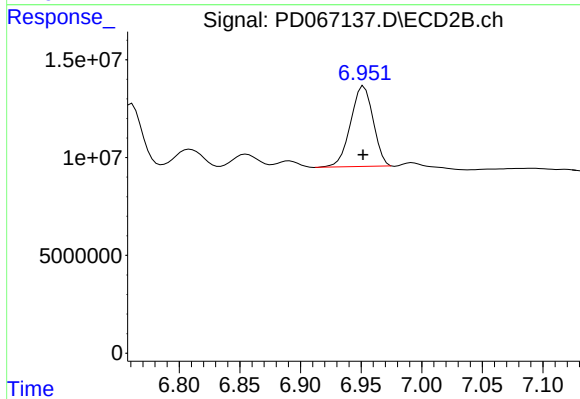

#27 Chlordane-5


R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 53280281
Conc: 247.39 ng/ml

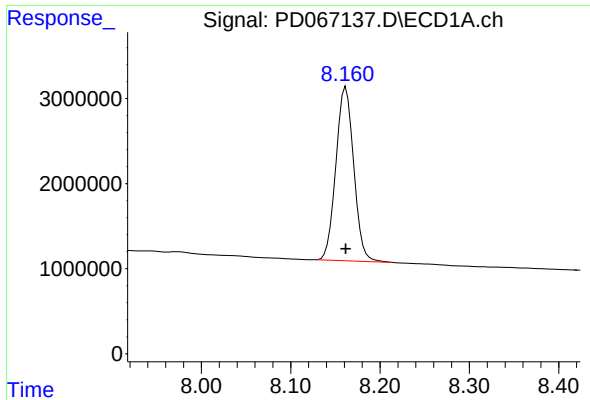

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 28343348
Conc: 26.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

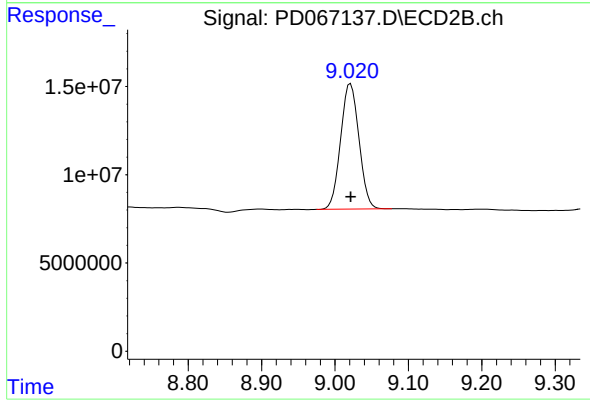

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 123502003
Conc: 25.91 ng/ml