

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120120\
 Data File : PD060502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2020 17:57
 Operator : DD\AJ
 Sample : L4862-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BB5

Manual Integrations
 APPROVED

Ankita
 12/2/2020 10:09:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 00:48:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.023	10324994	34242355	9.067	9.314
2)	SA Decachlor...	8.294	9.109	27779300	54899787	20.514	18.941
Target Compounds							
8)	B Heptachlo...	5.229	5.893	748315	26249085	0.525	7.023 #
10)	B trans-Chl...	5.459	6.137	17071377	35935786	11.391m	8.485m#
11)	B cis-Chlor...	5.521	6.213	18394036	75335205	12.477	18.273 #
12)	B 4,4'-DDE	5.685	6.366	17016055	55448798	11.907	13.956m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120120\
Data File : PD060502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2020 17:57
Operator : DD\AJ
Sample : L4862-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:48:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

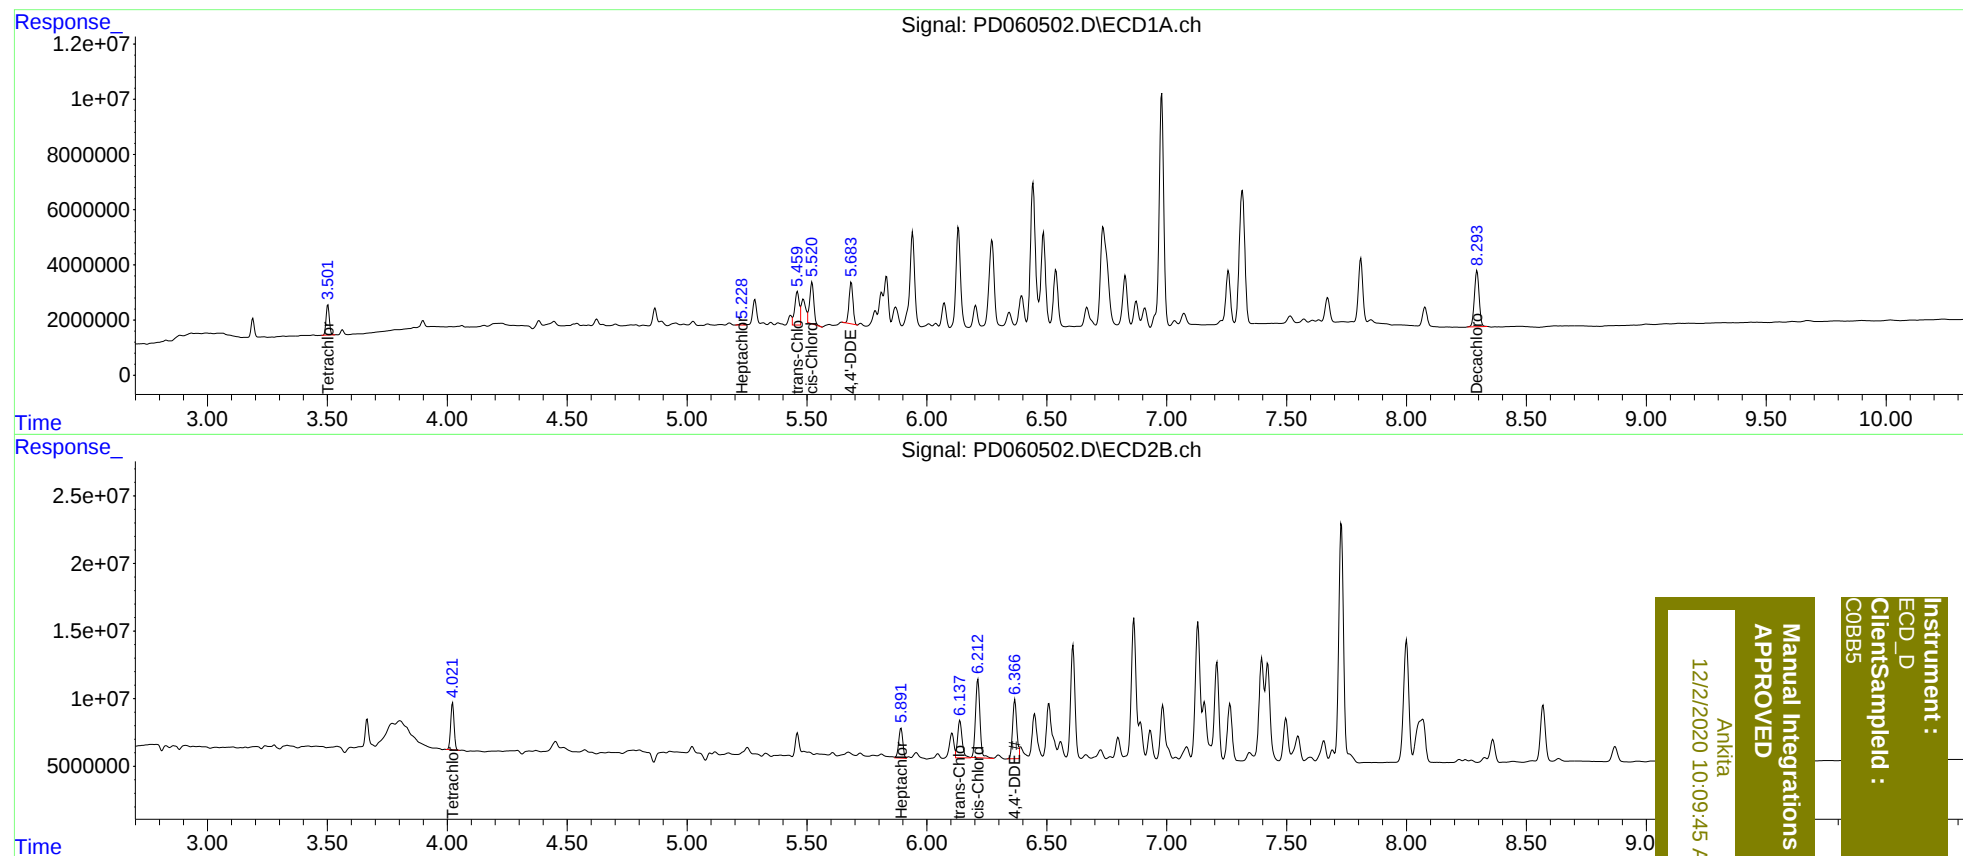

12/2/2020 10:09:45 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
C08B5