

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120120\
Data File : PD060490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2020 15:06
Operator : DD\AJ
Sample : INDA328
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
LabSampleId :
INDA328

Manual Integrations
APPROVED

Ankita
12/2/2020 10:09:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:42:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

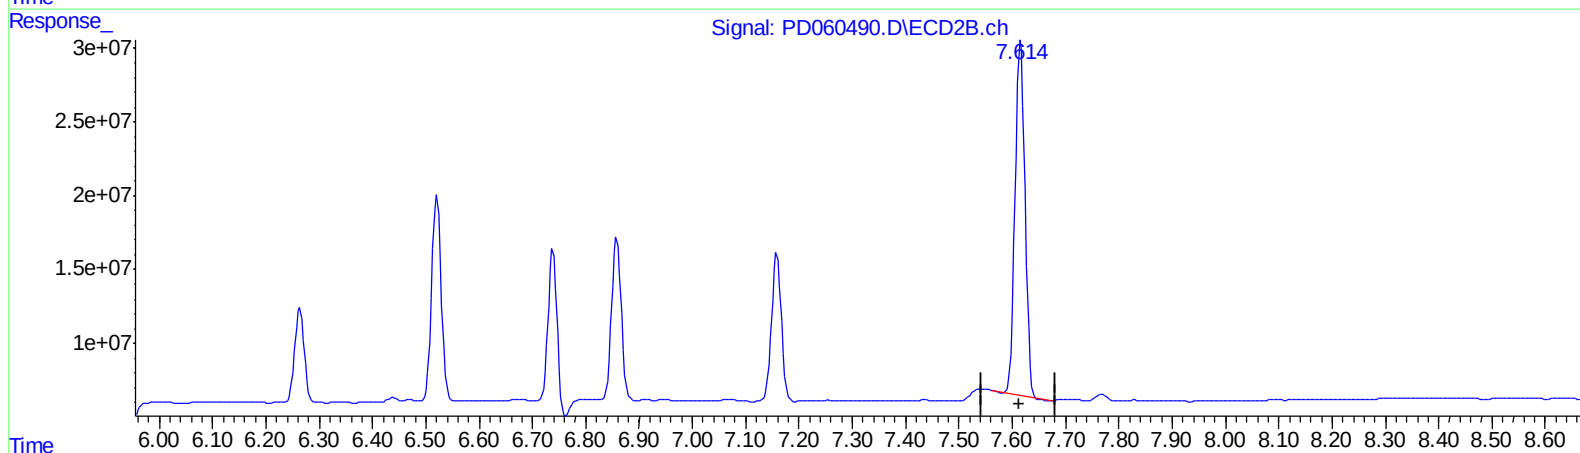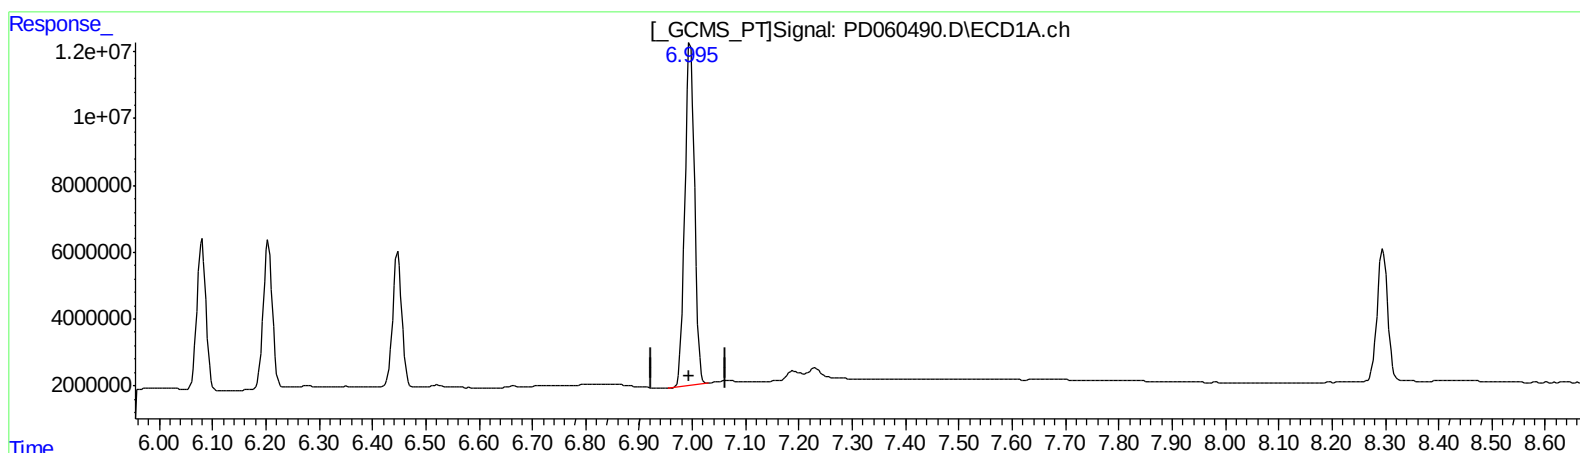

QEdit

(20) Methoxychlor (A)
6.996min 215.498 ng/ml
response 128728530

(20) Methoxychlor #2 (A)
7.616min 188.157 ng/ml
response 308440776

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120120\
Data File : PD060490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2020 15:06
Operator : DD\AJ
Sample : INDA328
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
LabSampleId :
INDA328

Manual Integrations
APPROVED

Ankita
12/2/2020 10:09:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:42:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

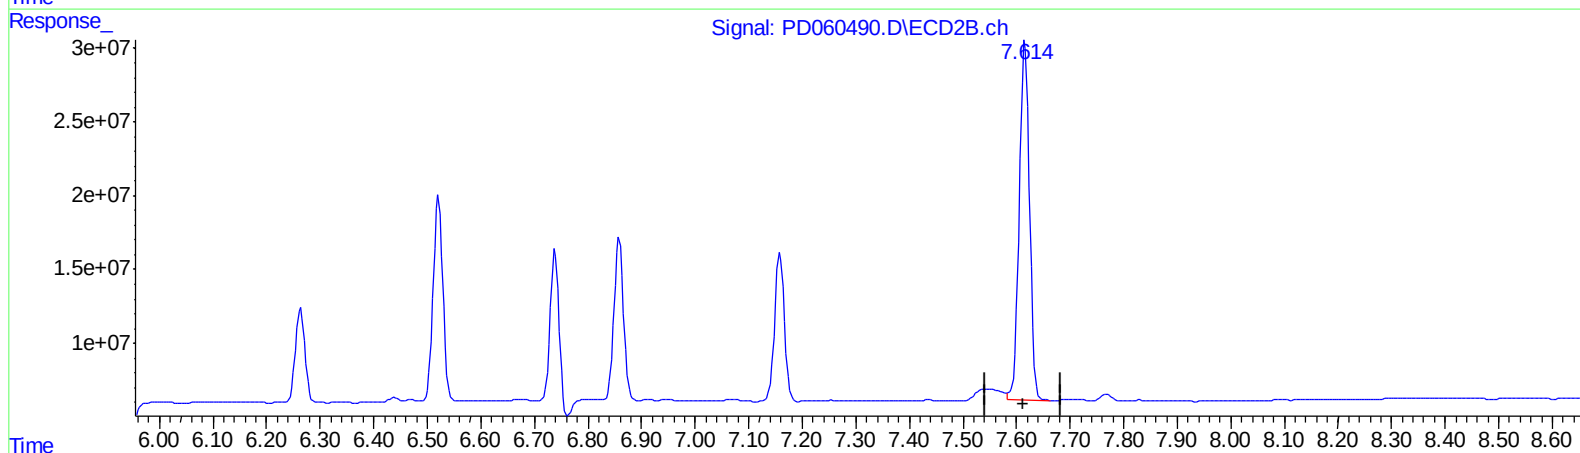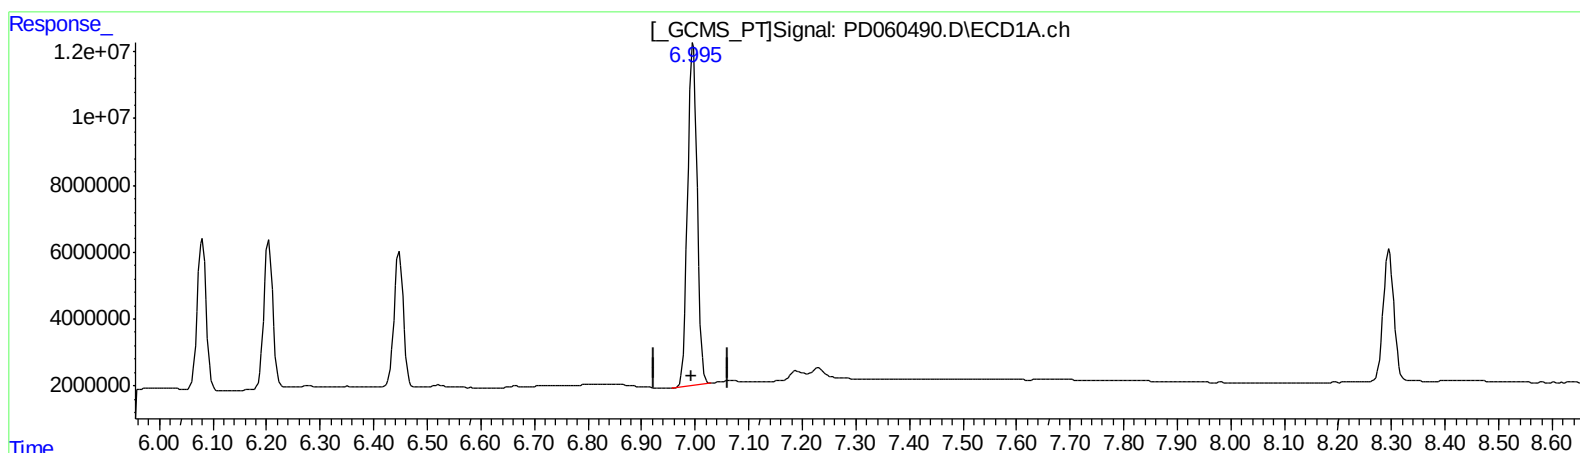

QEdit

(20) Methoxychlor (A)
6.996min 215.498 ng/ml
response 128728530

(20) Methoxychlor #2 (A)
7.614min 196.637 ng/ml m
response 322343235

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120120\
 Data File : PD060490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2020 15:06
 Operator : DD\AJ
 Sample : INDA328
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA328

Manual Integrations
 APPROVED

Ankita
 12/2/2020 10:09:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 00:42:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.503	4.024	23203048	75565913	20.376	20.554
27) SA Decachlor...	8.295	9.112	54524928	109.3E6	40.264	37.726
Target Compounds						
2) A alpha-BHC	3.945	4.414	33627737	113.0E6	20.503	20.734
3) MA gamma-BHC...	4.231	4.700	31833384	102.2E6	20.444	20.648
4) MA Heptachlor	4.537	5.212	33220764	99215471	21.278	20.479
9) A Endosulfan I	5.576	6.264	28788187	80954780	20.906	20.695
13) MA Dieldrin	5.822	6.521	62571339	173.2E6	41.110	40.836
14) MA Endrin	6.080	6.739	52845359	129.2E6	42.454	37.252
16) A 4,4'-DDD	6.204	6.858	52137656	138.1E6	42.860	41.673
17) MA 4,4'-DDT	6.448	7.159	49082678	128.0E6	40.182	38.988
20) A Methoxychlor	6.996	7.614	128.7E6	322.3E6	215.498	196.637m

AJ
 12/2/20

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.