

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120120\
 Data File : PD060485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2020 13:56
 Operator : DD\AJ
 Sample : L4862-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B04

Manual Integrations
 APPROVED

Ankita
 12/2/2020 10:09:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 06:51:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.503	4.024	14690766	46381885	12.901	12.616
2) SA Decachlor...	8.296	9.112	26186145	55139905	19.337	19.024
Target Compounds						
12) B 4,4'-DDE	5.684	6.367	1715583	6855501	1.200m	1.726m#
13) MA Dieldrin	5.811	6.511	8238791	3749412	5.413m	0.884 #
14) MA Endrin	6.072	6.729	3709840	29189839	2.980m	8.414 #
17) MA 4,4'-DDT	6.443	7.132	25903395	60392201	21.206m	18.396

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120120\
Data File : PD060485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2020 13:56
Operator : DD\AJ
Sample : L4862-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 06:51:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

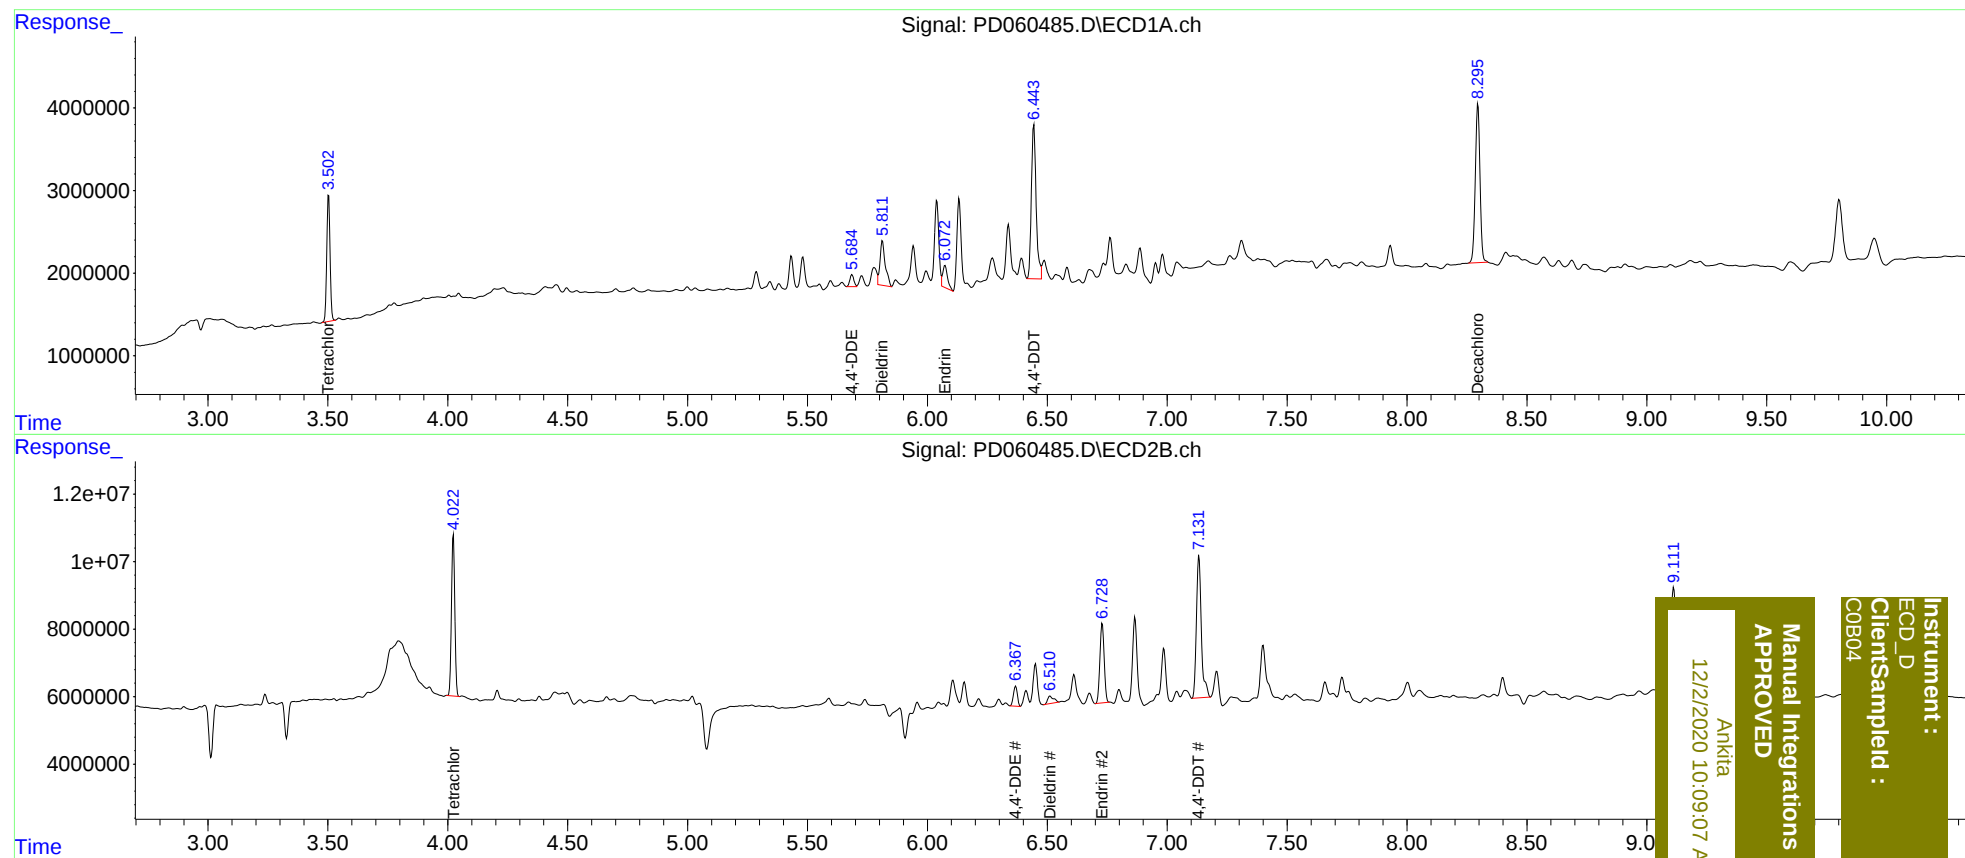

12/2/2020 10:09:07 AM
Ankitia

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
COB04