

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120120\
 Data File : PD060497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2020 16:47
 Operator : DD\AJ
 Sample : L4862-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B56

Manual Integrations
 APPROVED

Ankita
 12/2/2020 10:09:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 00:45:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.503	4.023	10011053	32735770	8.791	8.904
2) SA Decachlor...	8.294	9.110	15629733	29814132	11.542	10.286
Target Compounds						
4) MA Heptachlor	4.536	5.212	1377433	3487657	0.882	0.720
10) B trans-Chl...	5.463	6.138	3092202	27102233	2.063m	6.399m#
11) B cis-Chlor...	5.521	6.216	5785039	85625958	3.924	20.769 #
12) B 4,4'-DDE	5.685	6.366	863119	5150016	0.604	1.296 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120120\
Data File : PD060497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2020 16:47
Operator : DD\AJ
Sample : L4862-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:45:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

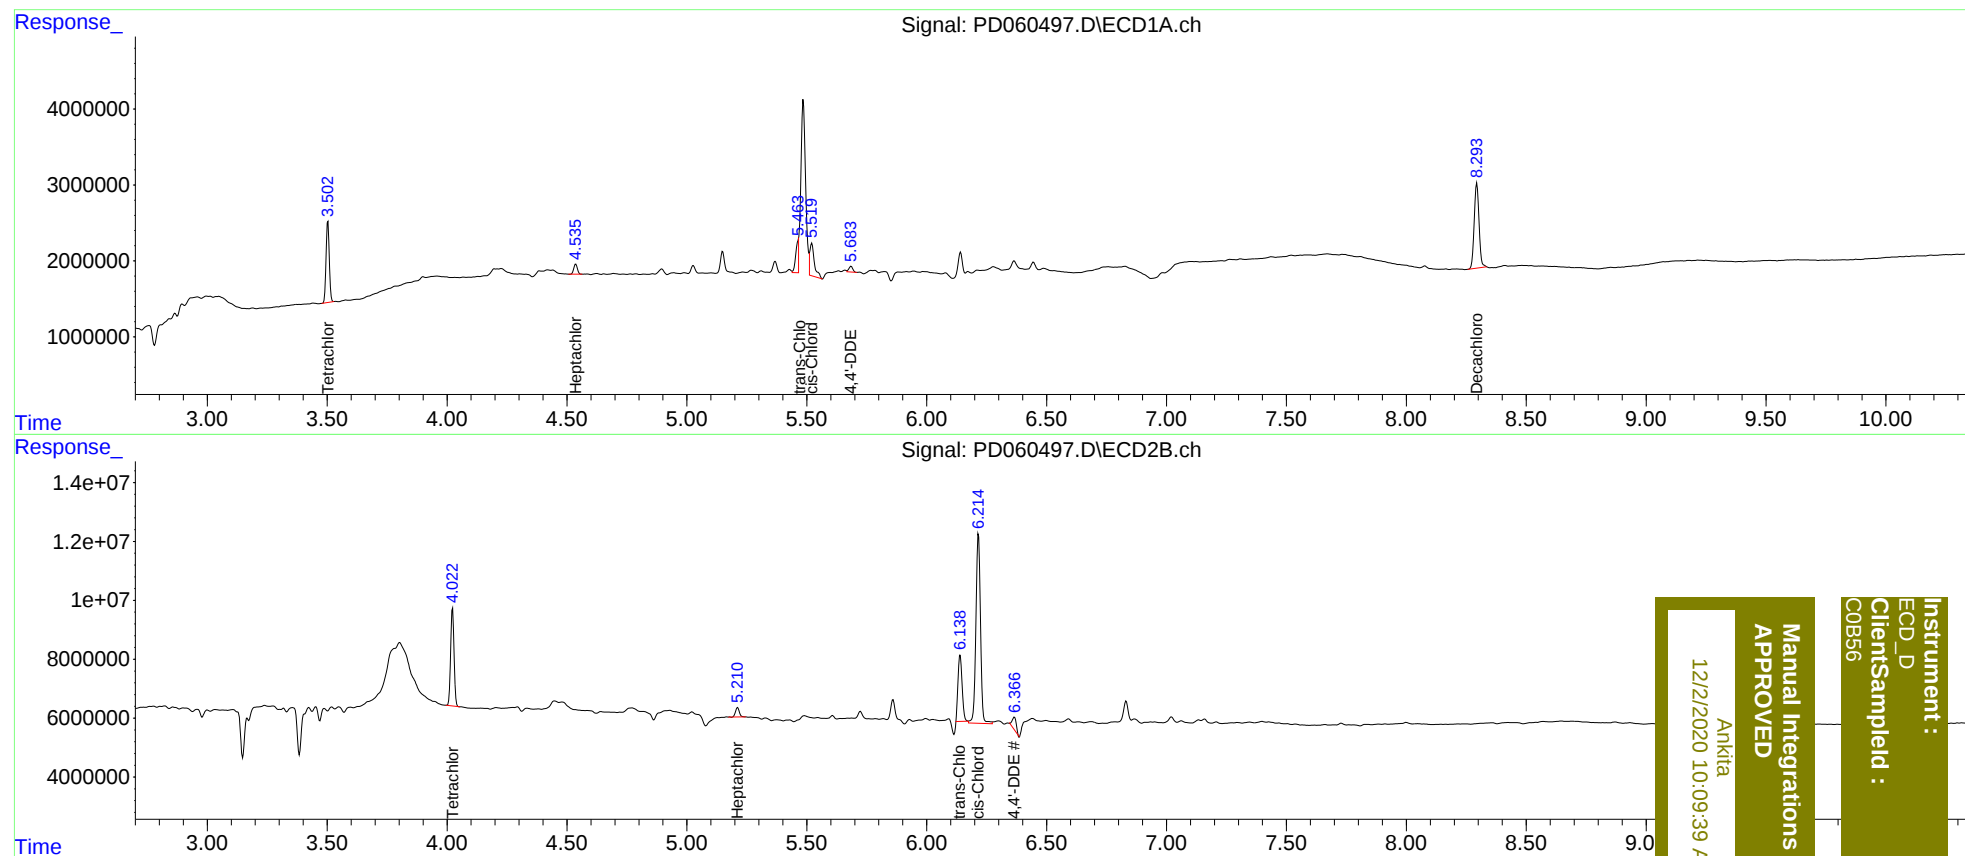

12/2/2020 10:09:39 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
COB56