

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120121\
 Data File : PD067164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2021 15:10
 Operator : AR\AJ
 Sample : PB141025BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 21:57:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:28:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	3.966	38212080	137.1E6	17.500	17.113
2)	SA Decachlor...	8.161	9.022	39143911	175.5E6	34.478	34.611
Target Compounds							
6)	B beta-BHC	0.000	4.844	0	1372711	N.D.	0.298


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120121\
Data File : PD067164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2021 15:10
Operator : AR\AJ
Sample : PB141025BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 21:57:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

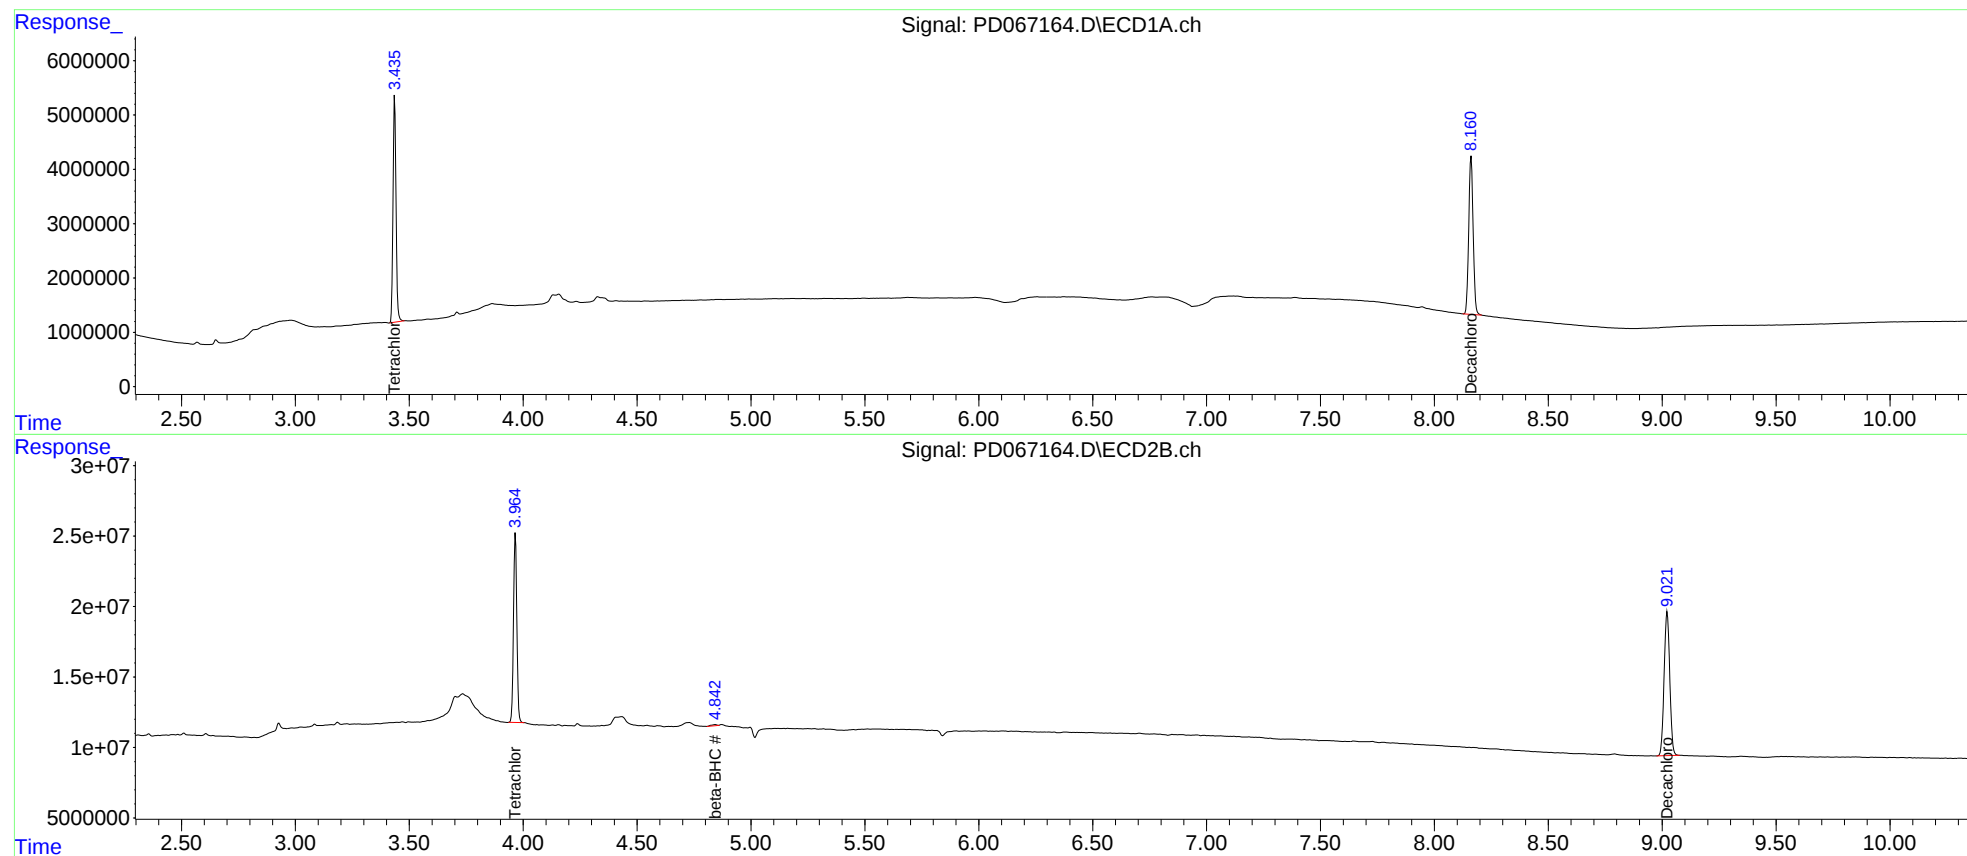

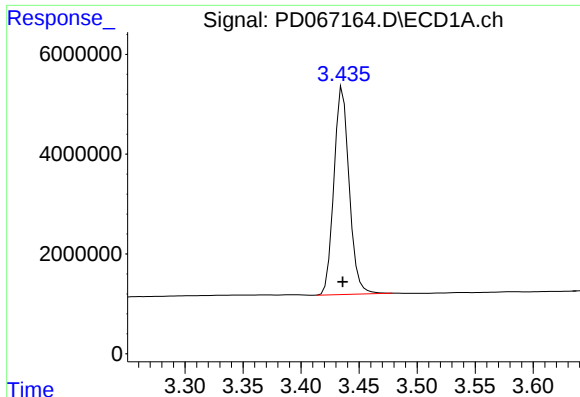


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 38212080
Conc: 17.50 ng/ml

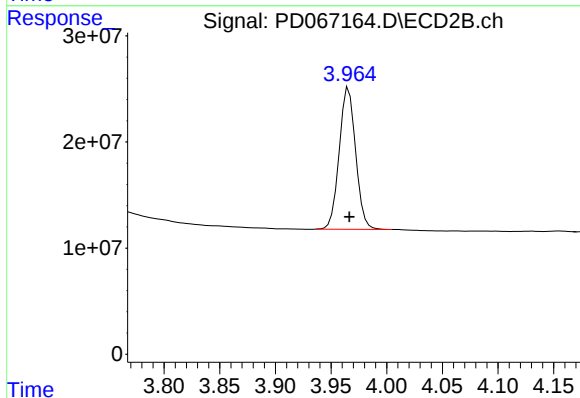


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 137101624
Conc: 17.11 ng/ml

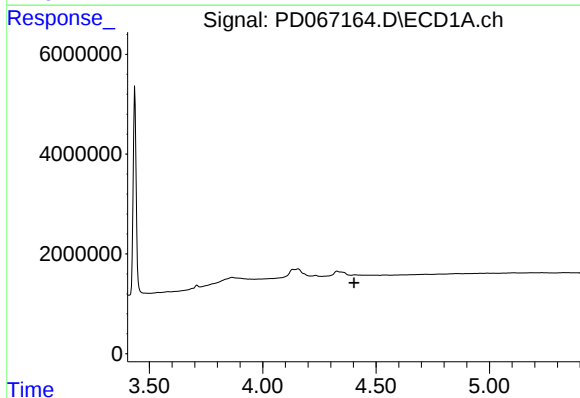


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.403 min
Response: 0
Conc: N.D.

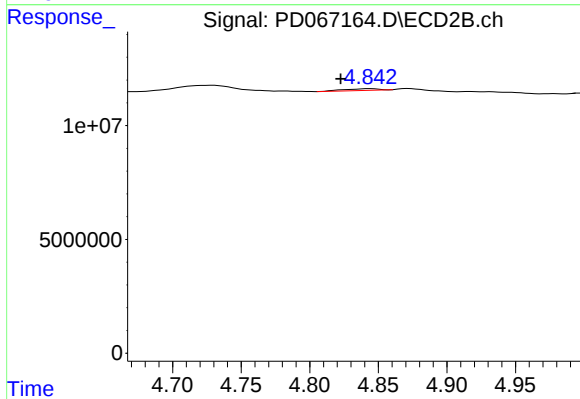


#6 beta-BHC

R.T.: 4.844 min
Delta R.T.: 0.021 min
Response: 1372711
Conc: 0.30 ng/ml

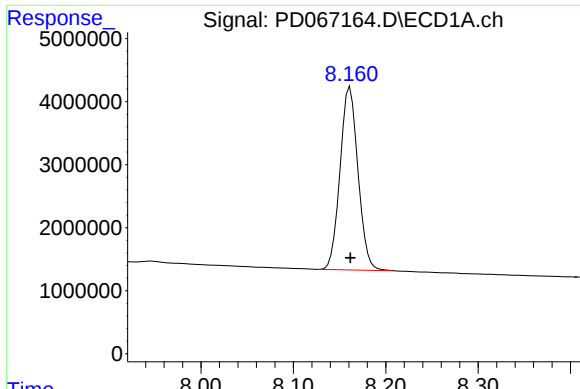

#27 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 39143911
Conc: 34.48 ng/ml

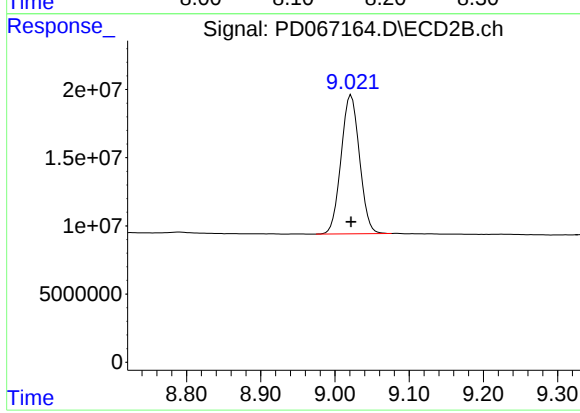

#27 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 175508492
Conc: 34.61 ng/ml