

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120123\
 Data File : PD079892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2023 13:06
 Operator : AR\AJ
 Sample : 05459-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/01/2023
 Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 21:59:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.568	2.802	18615595	29085945	12.747	12.716
27) SA Decachlor...	9.113	7.944	21079942	26717597	11.879	11.191
Target Compounds						
9) A Endosulfan I	6.136	5.152	5437529	12299352	2.630m	4.437m#
13) MA Dieldrin	6.399	5.396	1863725	6103283	0.847	1.917m#
16) A 4,4'-DDD	6.730	5.811	2235527	1784333	1.380	0.758m#
17) MA 4,4'-DDT	7.033	6.060	1520957	1405863	0.893m	0.585 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120123\
Data File : PD079892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2023 13:06
Operator : AR\AJ
Sample : 05459-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 21:59:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

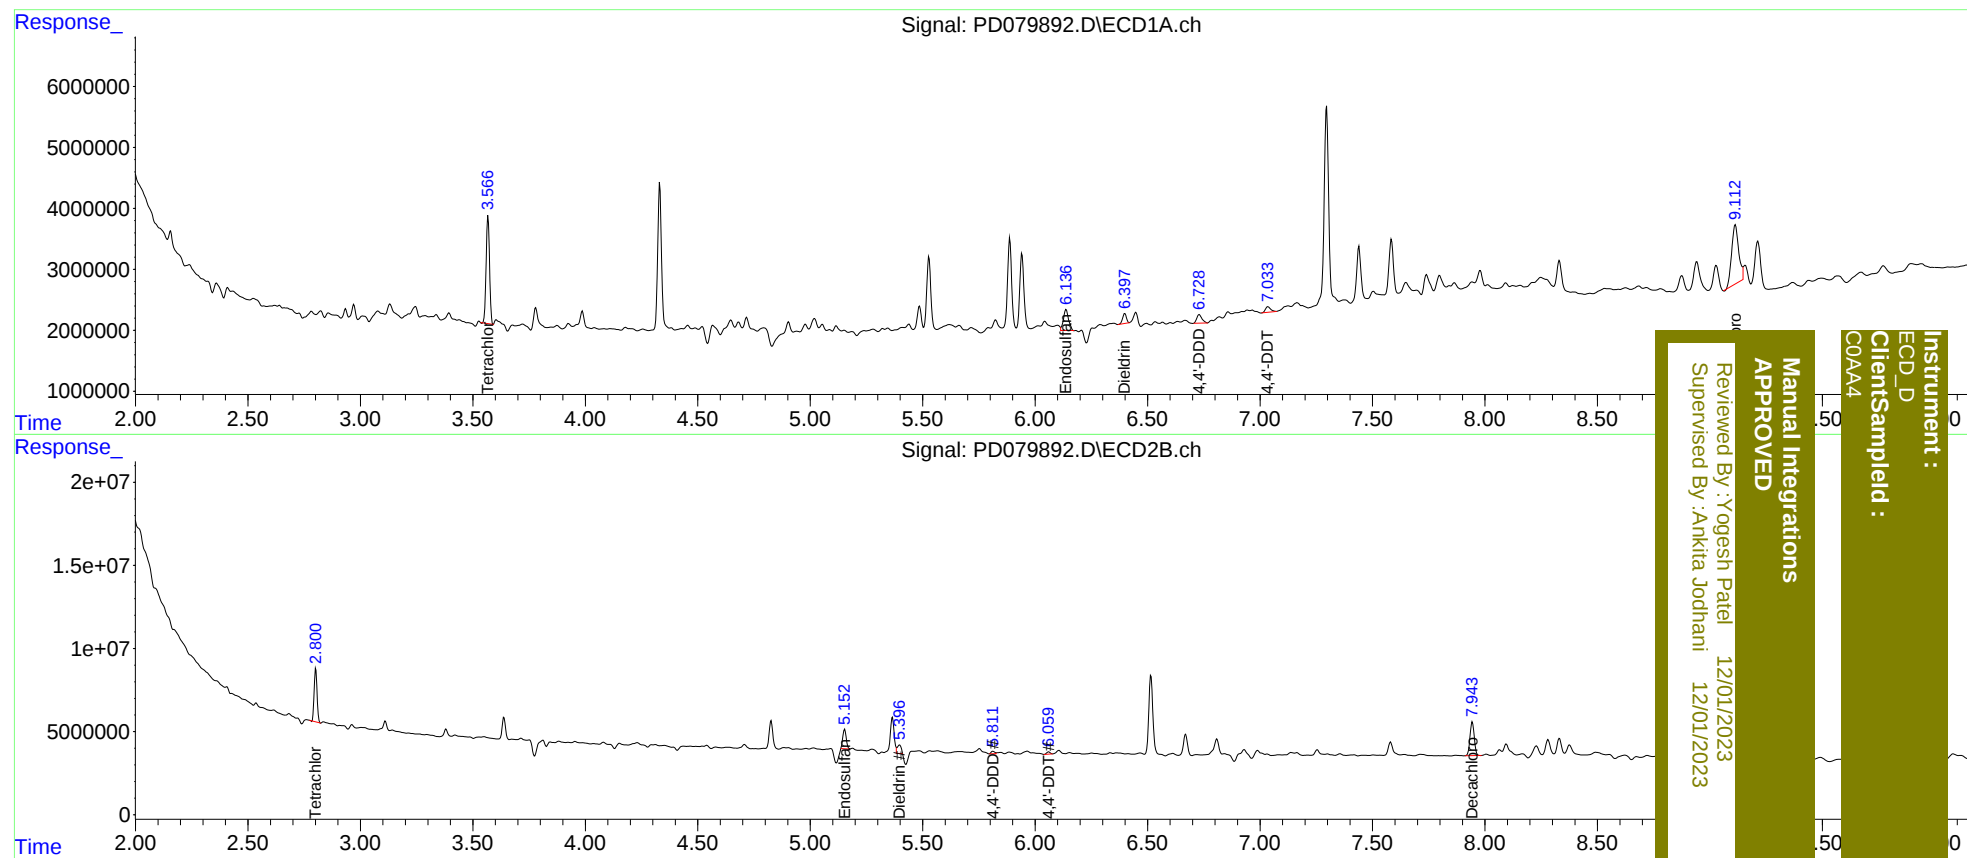

Instrument :
ECD_D
ClientSampled :
COAA4

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 12/01/2023
Supervised By : Ankita Jodhani 12/01/2023