

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120123\
 Data File : PD079903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2023 15:33
 Operator : AR\AJ
 Sample : 05459-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/01/2023
 Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 03:57:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.800	17531386	27048685	12.005m	11.826m
2)	SA Decachlor...	9.115	7.945	42157519	30260992	23.757m	12.675 #
Target Compounds							
9)	A Endosulfan I	6.137	5.153	8401145	17012977	4.064m	6.137m#
13)	MA Dieldrin	6.398	5.395	5663899	10558885	2.575m	3.316m#
16)	A 4,4'-DDD	6.727	5.810	5077006	3400646	3.134m	1.445m#
17)	MA 4,4'-DDT	7.033	6.061	2622079	3273173	1.539	1.363

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120123\
Data File : PD079903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2023 15:33
Operator : AR\AJ
Sample : 05459-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 03:57:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

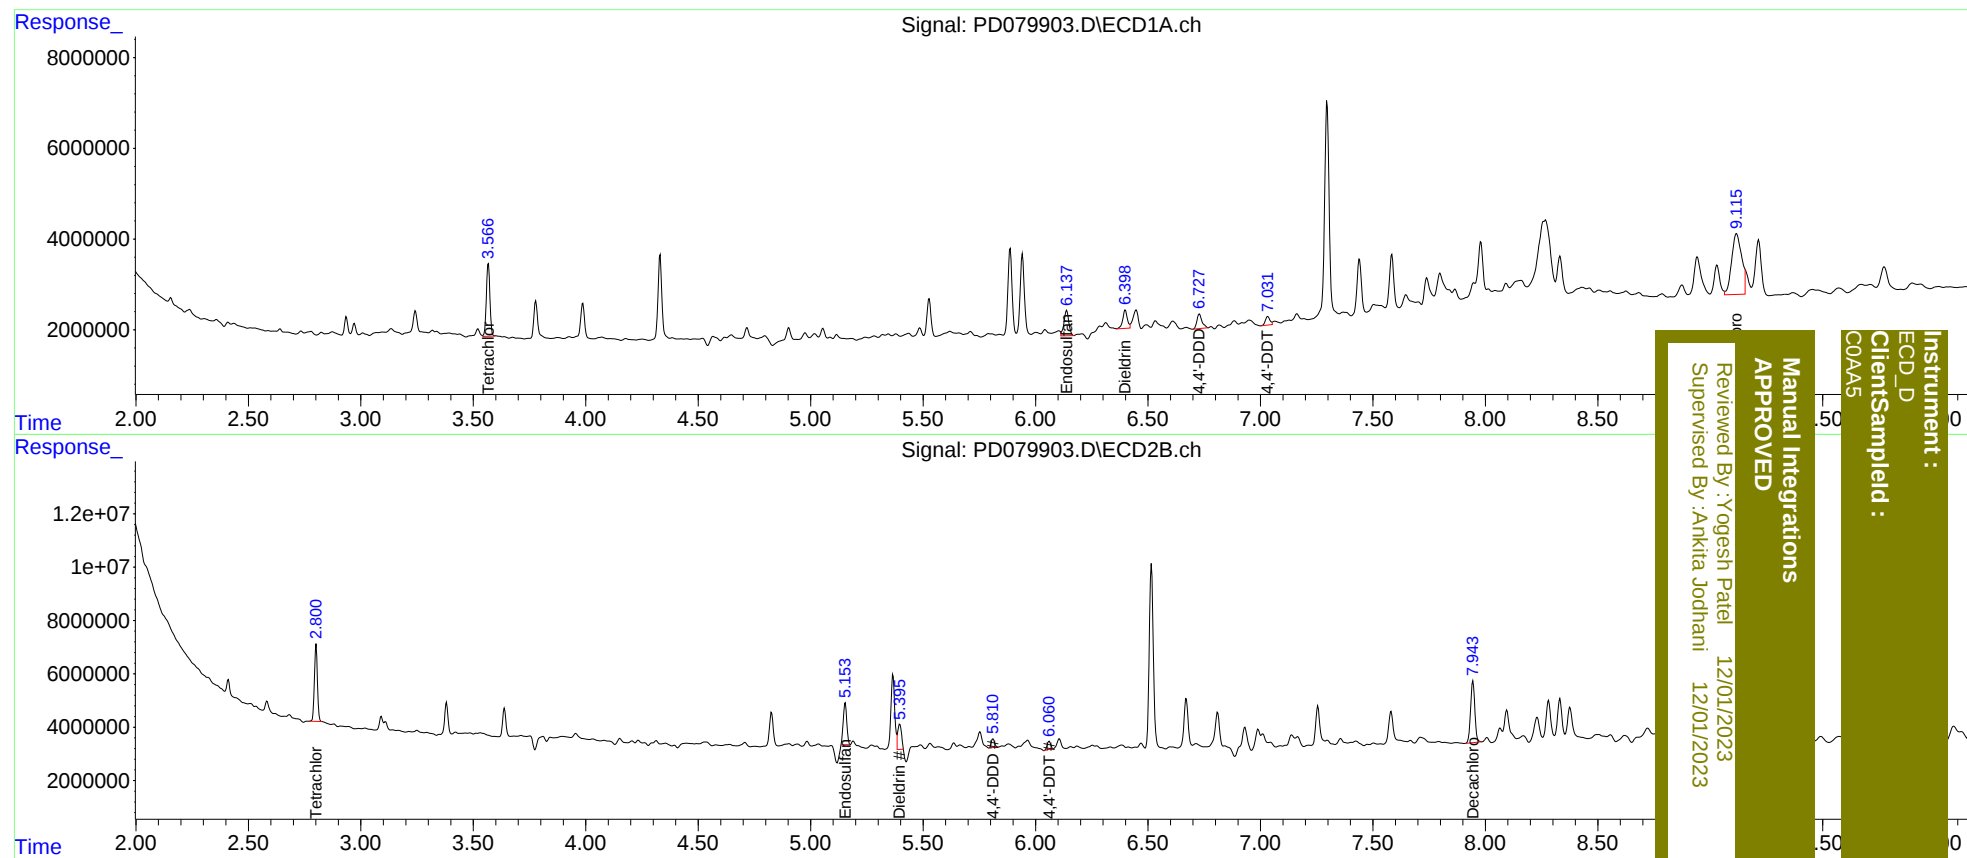

Instrument :
ECD_D
ClientSampled :
COAAS

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 12/01/2023
Supervised By : Ankita Jodhani 12/01/2023