

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120125\
 Data File : PD091408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2025 13:12
 Operator : AR\AJ
 Sample : Q3732-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HD-01-11-26-2025

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/02/2025
 Supervised By : mohammad ahmed 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 02:12:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:46:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.872	74692104	754.8E6	21.659m	20.607
28) SA Decachlor...	9.057	8.054	72155731	520.2E6	14.484	13.146

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120125\
Data File : PD091408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2025 13:12
Operator : AR\AJ
Sample : Q3732-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
HD-01-11-26-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/02/2025
Supervised By :mohammad ahmed 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 02:12:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:46:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

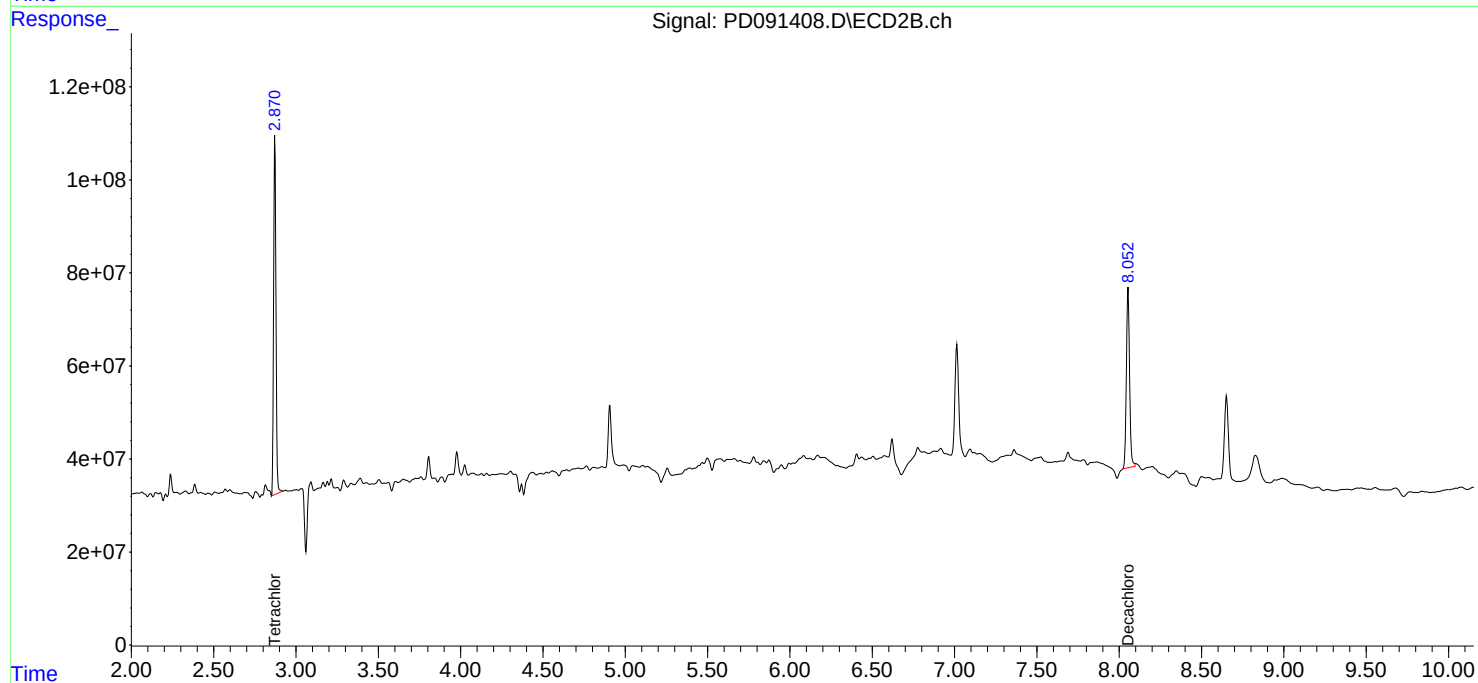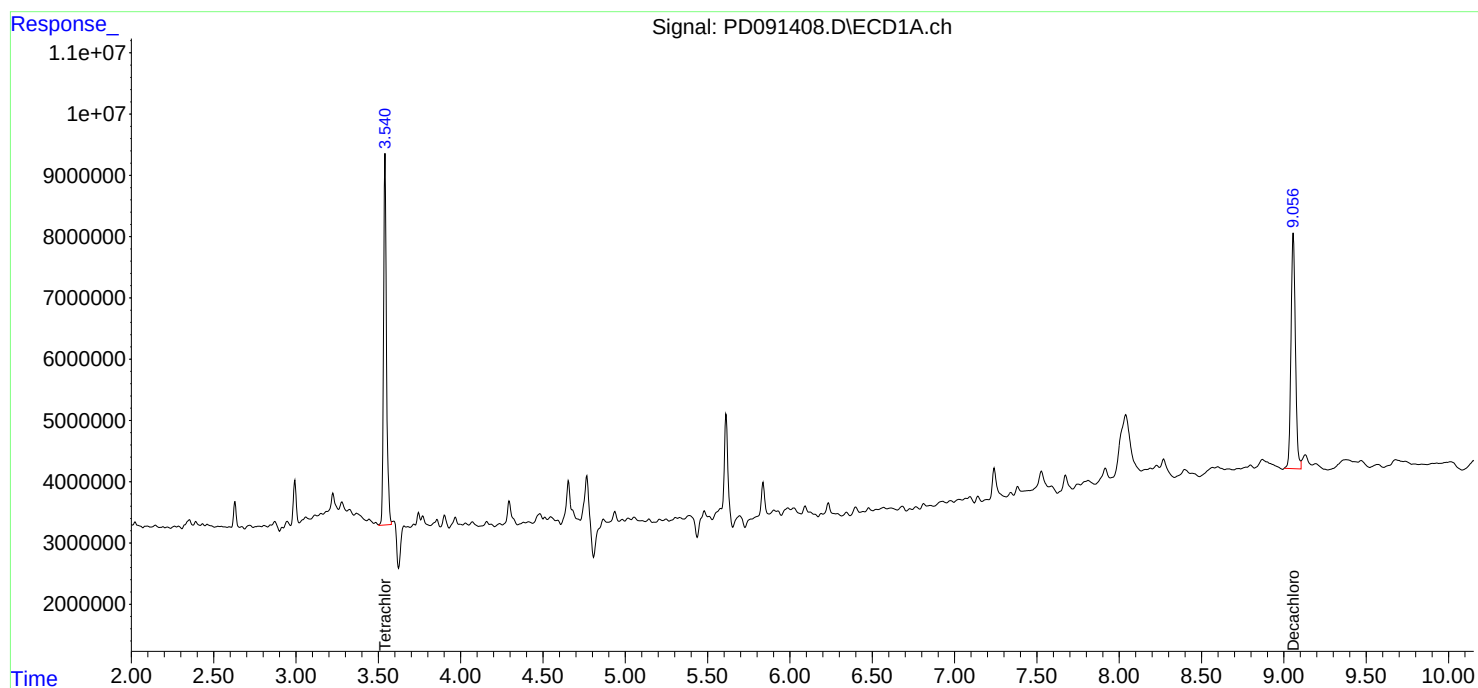

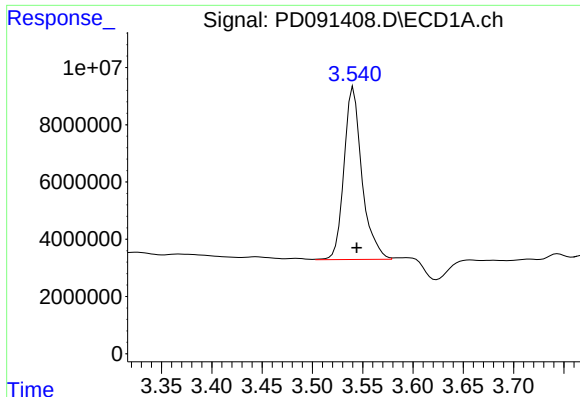


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.005 min
Response: 74692104
Conc: 21.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
HD-01-11-26-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/02/2025
Supervised By :mohammad ahmed 12/03/2025

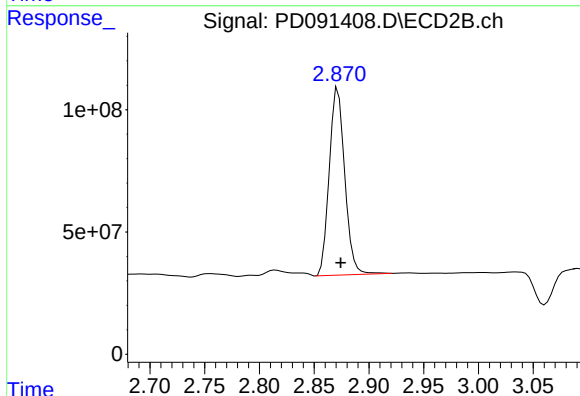


#1 Tetrachloro-m-xylene

R.T.: 2.872 min
Delta R.T.: -0.002 min
Response: 754837633
Conc: 20.61 ng/ml

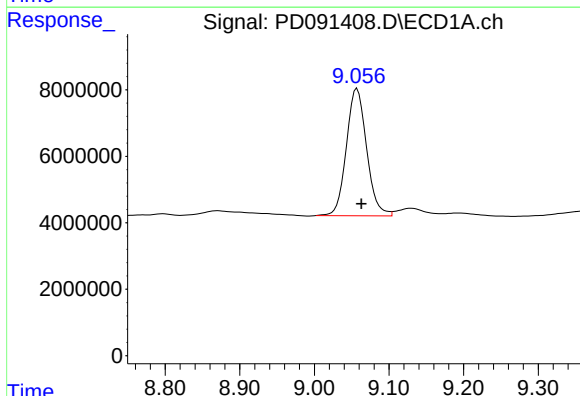

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.006 min
Response: 72155731
Conc: 14.48 ng/ml

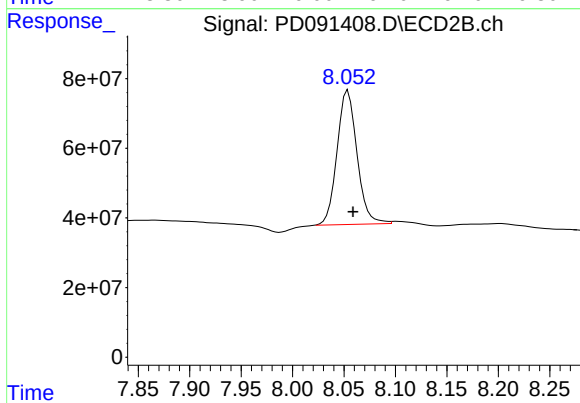

#28 Decachlorobiphenyl

R.T.: 8.054 min
Delta R.T.: -0.005 min
Response: 520231858
Conc: 13.15 ng/ml