

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120220\
 Data File : PD060548.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2020 20:02
 Operator : DD\AJ
 Sample : L4865-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BH1

Manual Integrations
 APPROVED

Ankita
 12/3/2020 10:22:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 03:40:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.022	11422946	37271842	10.031	10.138
27)	SA Decachlor...	8.291	9.106	25075034	49724398	18.517	17.156
Target Compounds							
8)	B Heptachlo...	5.230	5.888	1468056	5282914	1.029m	1.414 #
10)	B trans-Chl...	5.459	6.136	11209811	37687407	7.480m	8.899m
11)	B cis-Chlor...	5.520	6.212	9956235	49766980	6.753	12.071 #
15)	B Endosulfa...	6.361	6.948	3000970	1871266	2.525	0.586m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120220\
Data File : PD060548.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2020 20:02
Operator : DD\AJ
Sample : L4865-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 03:40:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

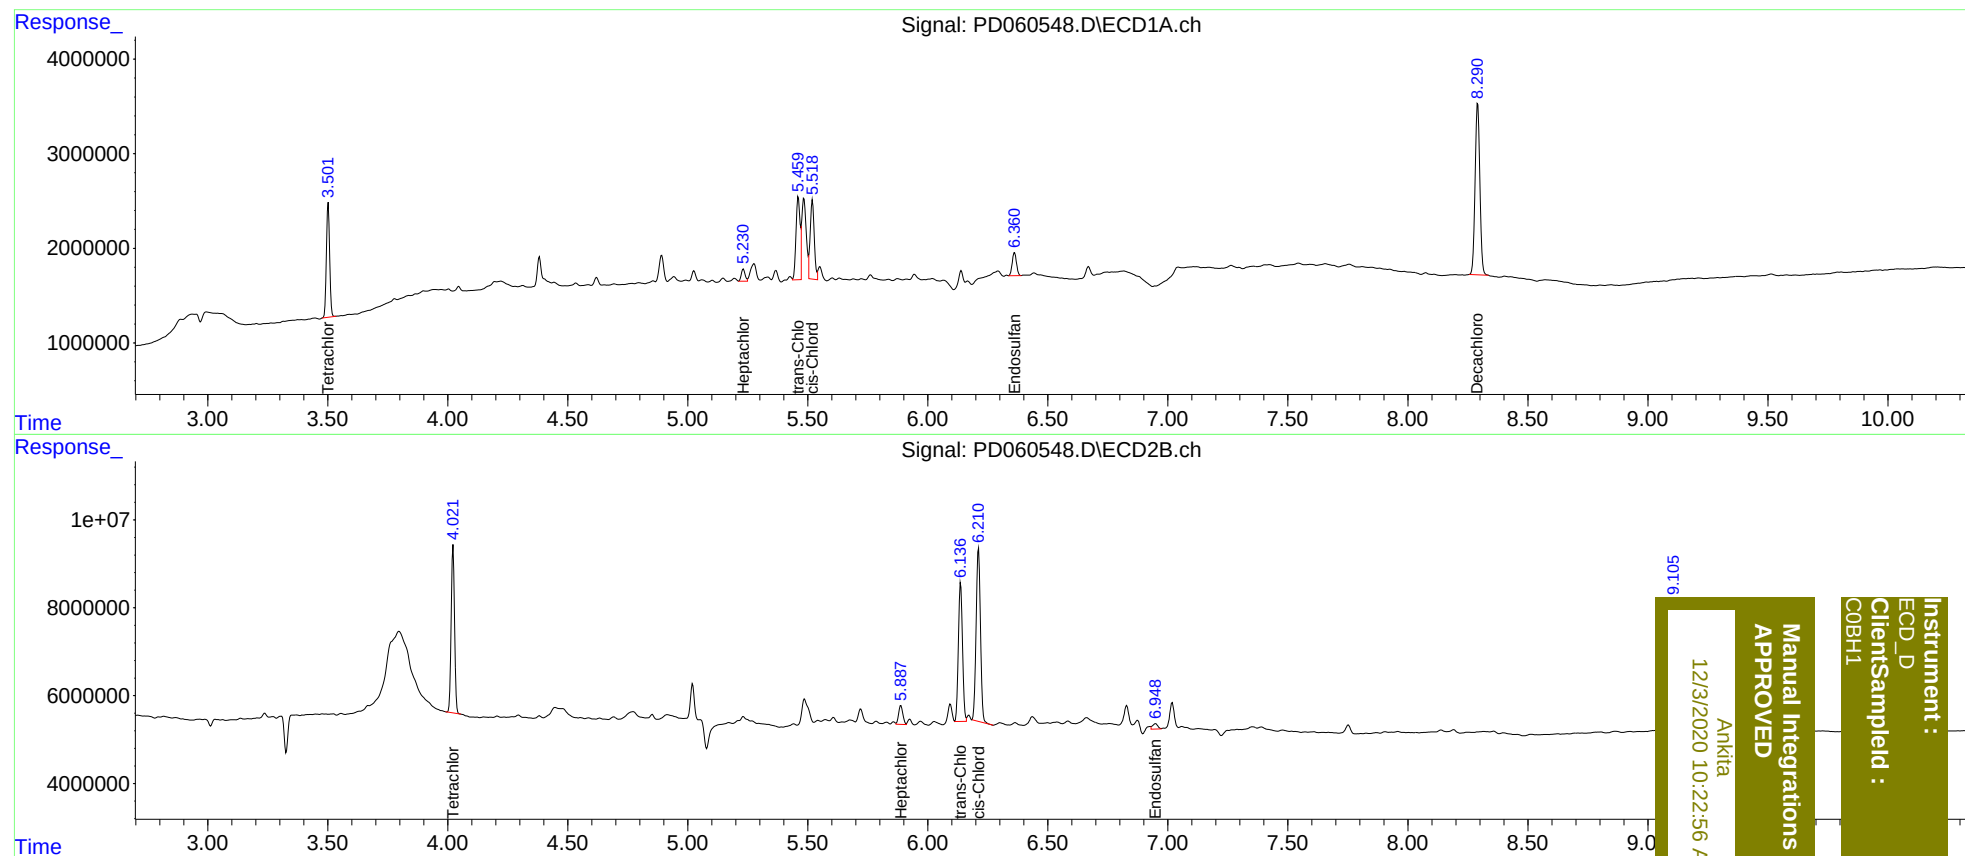

12/3/2020 10:22:56 AM

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSample :
COBH1