

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120225\
 Data File : PD091424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2025 16:11
 Operator : AR\AJ
 Sample : Q3748-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 AU-05-12-1-2025

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 01:08:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:46:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.872	46814227	547.2E6	13.575	14.938
28) SA Decachlor...	9.063	8.059	66503379	498.2E6	13.349m	12.589
Target Compounds						
12) B 4,4'-DDE	6.187	5.362	2545113	35347567	0.439	0.661 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120225\
Data File : PD091424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2025 16:11
Operator : AR\AJ
Sample : Q3748-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
AU-05-12-1-2025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/03/2025
Supervised By : Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 01:08:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:46:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

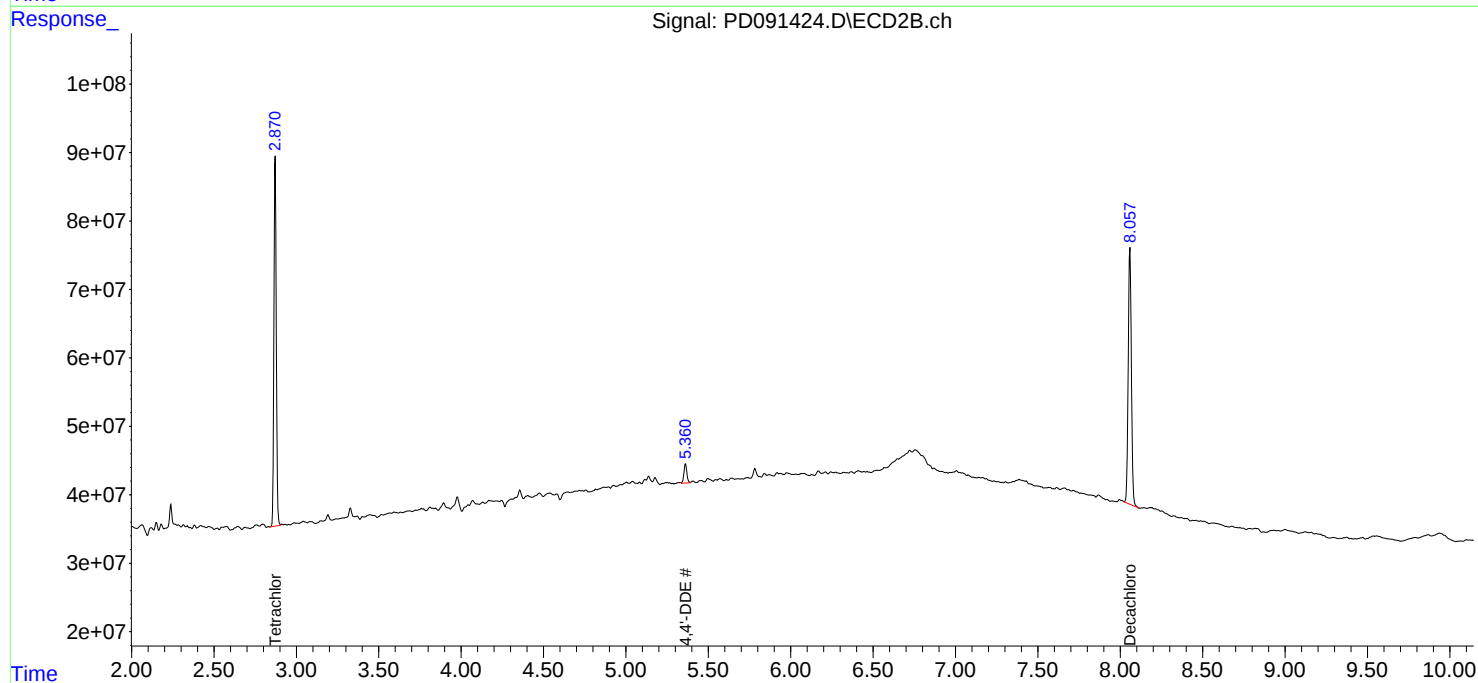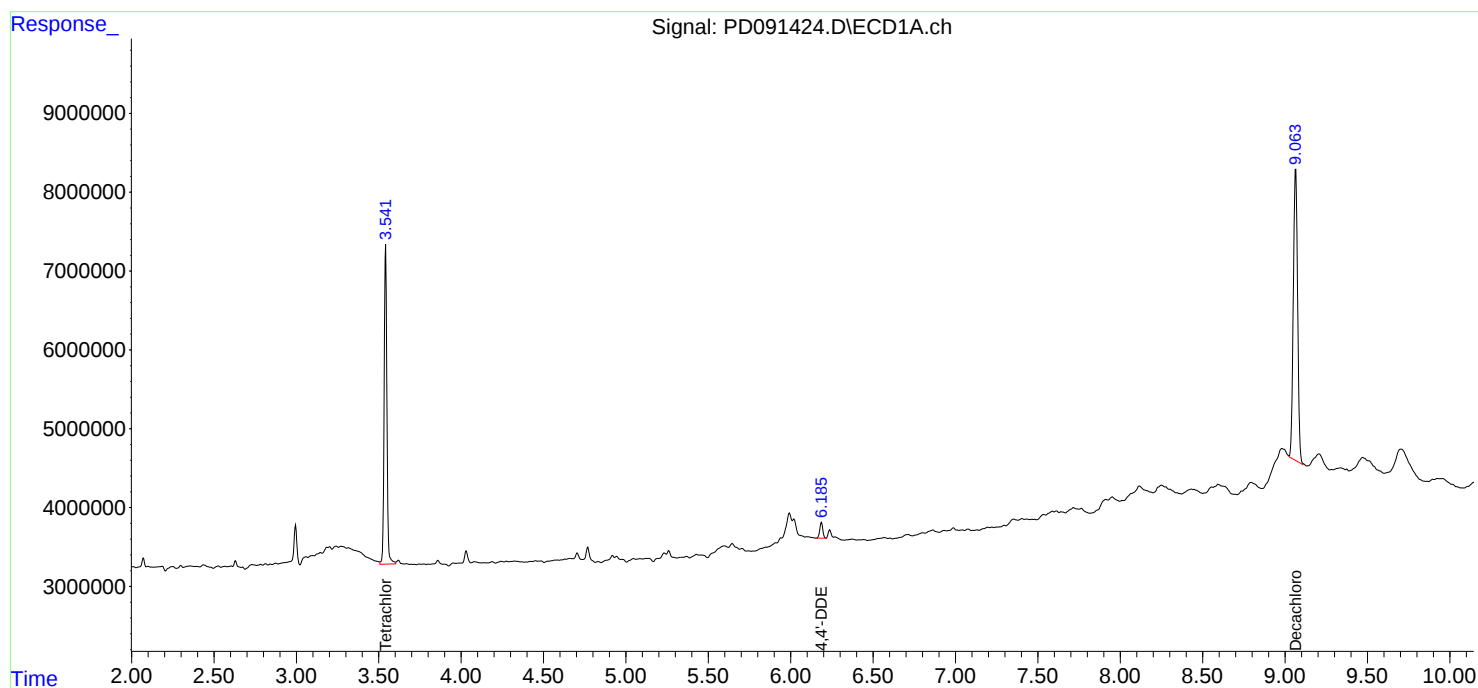

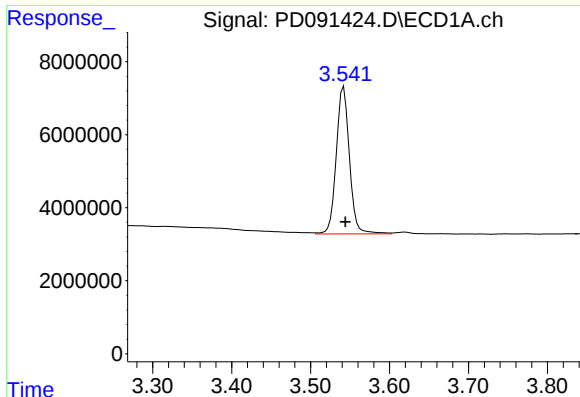


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 46814227
Conc: 13.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-05-12-1-2025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

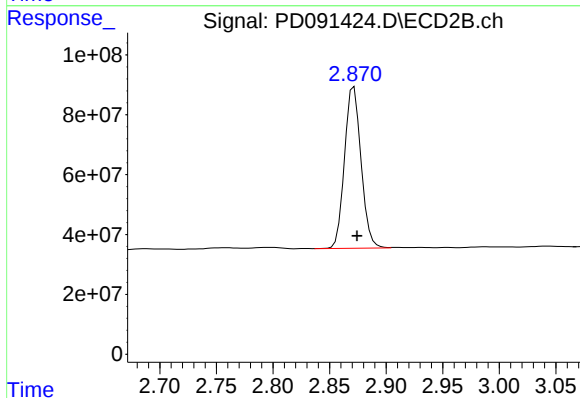


#1 Tetrachloro-m-xylene

R.T.: 2.872 min
Delta R.T.: -0.003 min
Response: 547189320
Conc: 14.94 ng/ml

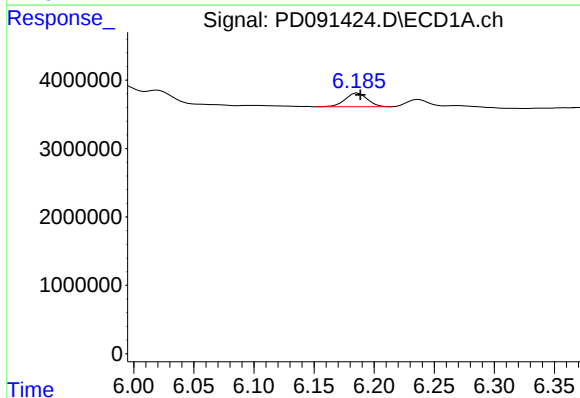


#12 4,4'-DDE

R.T.: 6.187 min
Delta R.T.: -0.002 min
Response: 2545113
Conc: 0.44 ng/ml

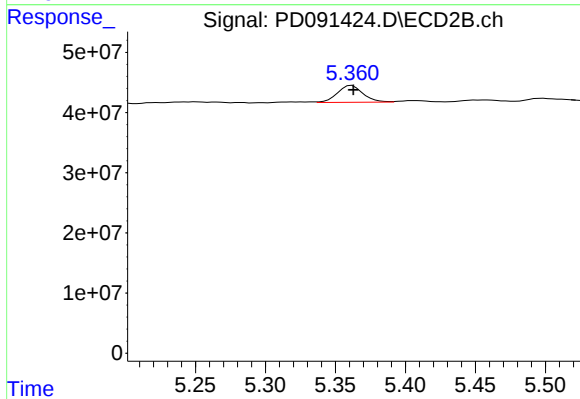

#12 4,4'-DDE

R.T.: 5.362 min
Delta R.T.: -0.001 min
Response: 35347567
Conc: 0.66 ng/ml

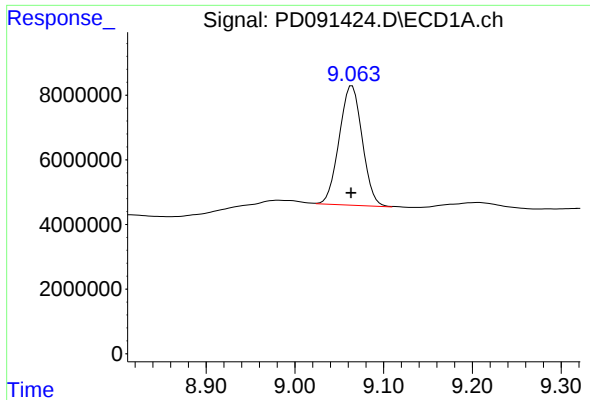


#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: 0.000 min
Response: 66503379
Conc: 13.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-05-12-1-2025

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

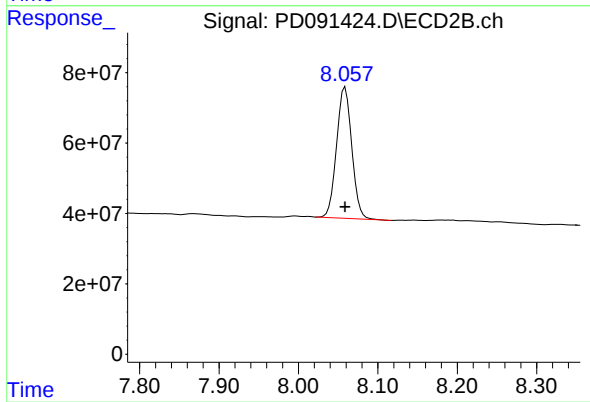

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: 0.000 min
Response: 498204049
Conc: 12.59 ng/ml