

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120318\
 Data File : PD050616.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2018 19:54
 Operator : AJ\SJ
 Sample : PB115220BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 01:10:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120318CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 04 00:43:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	4.045	30983565	572.7E6	20.315	20.198
27)	SA Decachlor...	7.835	9.153	67167155	905.5E6	40.831	41.838
Target Compounds							
6)	B beta-BHC	0.000	4.940f	0 33781011	N.D.	2.099	
7)	B delta-BHC	0.000	5.089	0 23477895	N.D.	0.589	
8)	B Heptachlo...	0.000	5.925	0 56709609	N.D.	1.569	
10)	B trans-Chl...	0.000	6.114f	0 7413636	N.D.	0.229	
16)	A 4,4'-DDD	0.000	6.846f	0 17008157	N.D.	0.699	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120318\
Data File : PD050616.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2018 19:54
Operator : AJ\SJ
Sample : PB115220BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 01:10:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120318CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 04 00:43:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

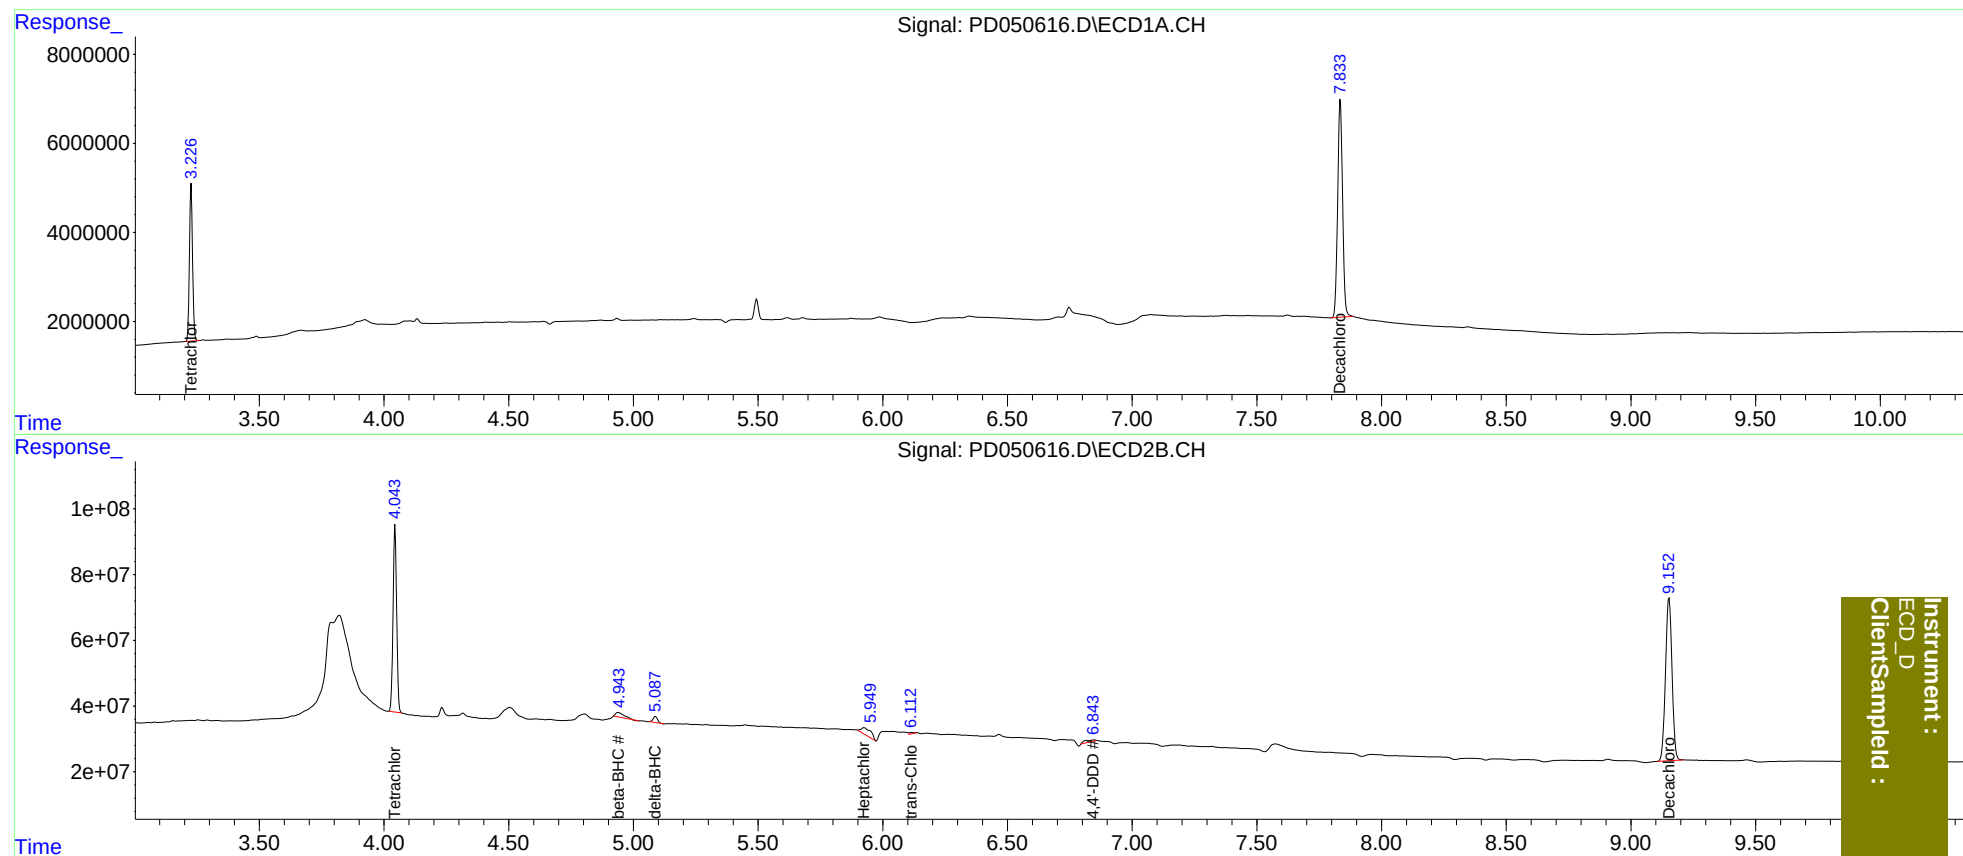

Instrument :
ECD_D
ClientSampleId :