

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120318\
 Data File : PD050615.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2018 19:40
 Operator : AJ\SJ
 Sample : PB115035BS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS35

Manual Integrations
 APPROVED

apatel
 12/4/2018 8:24:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 01:10:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120318CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 04 00:43:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	4.045	30006813	560.0E6	19.674	19.752
27)	SA Decachlor...	7.835	9.153	66450891	879.5E6	40.396	40.638
Target Compounds							
3)	MA gamma-BHC...	3.917	4.724	112.9E6	1752.2E6	48.489	44.341
8)	B Heptachlo...	4.856	5.933	111.4E6	1607.5E6	54.041	44.483
10)	B trans-Chl...	5.074	6.167	112.0E6	1548.9E6	53.235	47.804
12)	B 4,4'-DDE	5.300	6.396	218.7E6	2847.5E6	110.879	97.915
13)	MA Dieldrin	5.414	6.550	241.0E6	2931.5E6	104.230	93.113
14)	MA Endrin	5.661	6.768	217.0E6	2358.4E6	110.197	99.434
19)	B Endosulfa...	6.306	7.323	156.6E6	1999.8E6	91.803	84.205m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120318\
Data File : PD050615.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2018 19:40
Operator : AJ\SJ
Sample : PB115035BS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 01:10:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120318CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 04 00:43:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

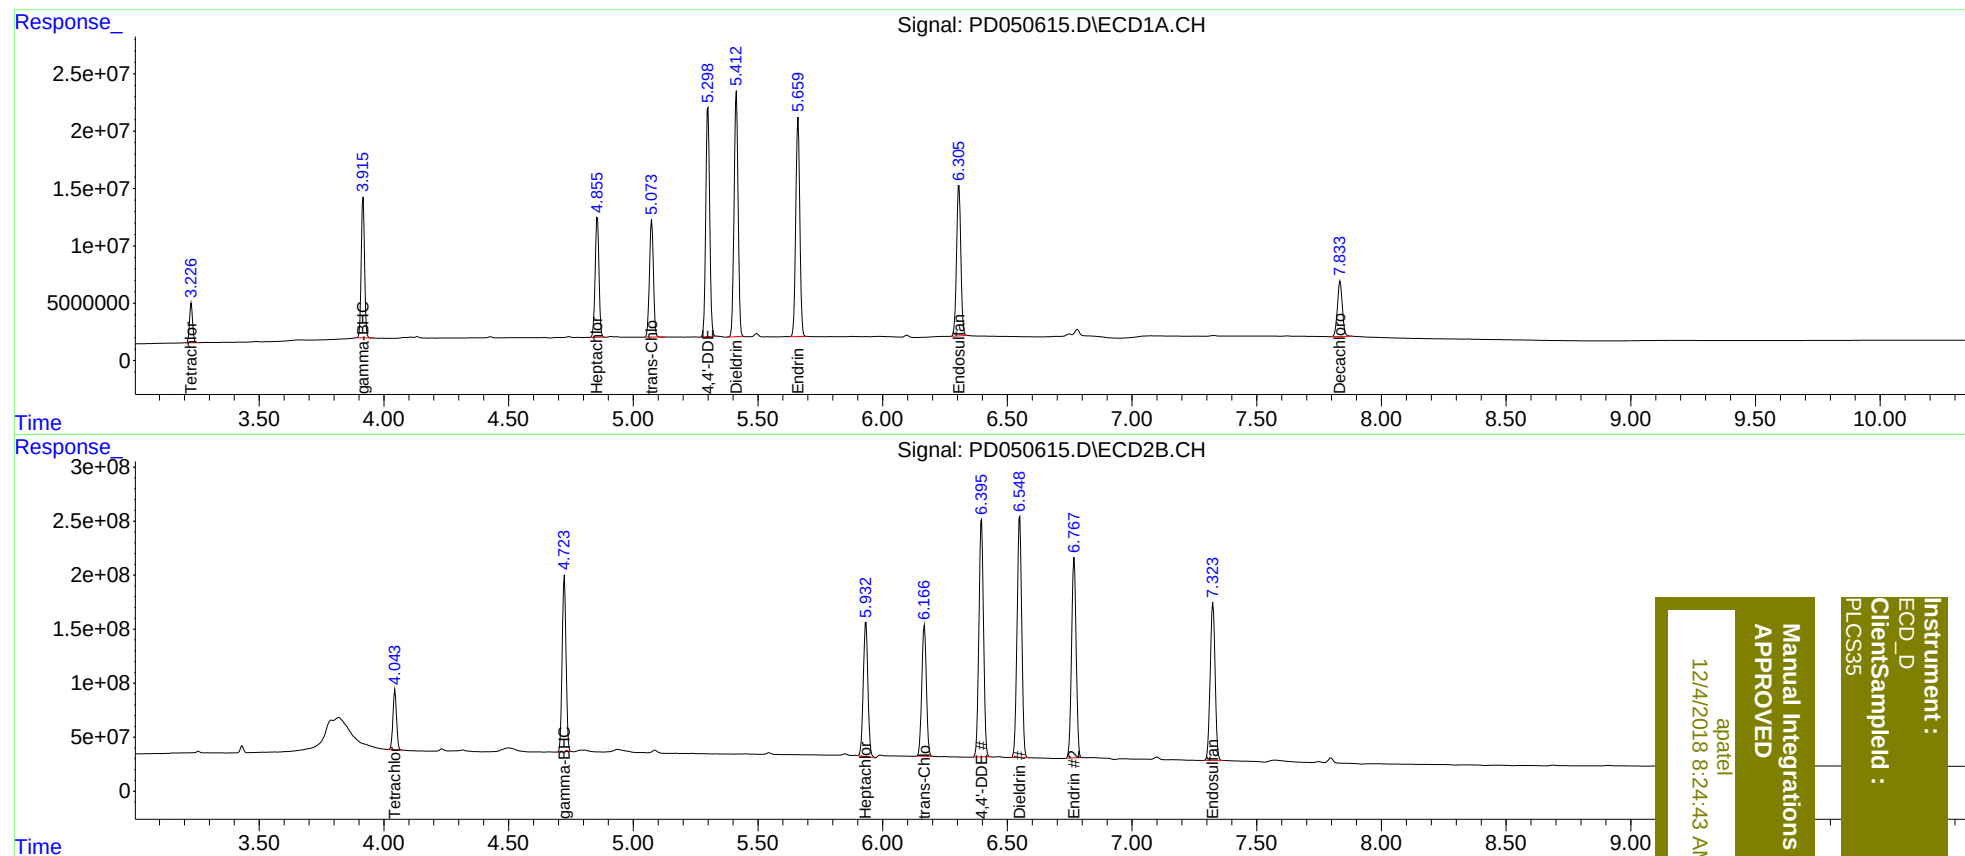

12/4/2018 8:24:43 AM

Manual Integrations
APPROVED

apatel

Instrument :
ECD_D
ClientSampled :
PLCS35

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120318\
 Data File : PD050615.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2018 19:40
 Operator : AJ\SJ
 Sample : PB115035BS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS35

Manual Integrations
 APPROVED

apatel
 12/4/2018 8:24:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 01:10:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120318CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 04 00:43:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.228	4.045	30006813	560.0E6	19.674	19.752
27) SA Decachlor...	7.835	9.153	66450891	879.5E6	40.396	40.638
Target Compounds						
3) MA gamma-BHC...	3.917	4.724	112.9E6	1752.2E6	48.489	44.341
8) B Heptachlo...	4.856	5.933	111.4E6	1607.5E6	54.041	44.483
10) B trans-Chl...	5.074	6.167	112.0E6	1548.9E6	53.235	47.804
12) B 4,4'-DDE	5.300	6.396	218.7E6	2847.5E6	110.879	97.915
13) MA Dieldrin	5.414	6.550	241.0E6	2931.5E6	104.230	93.113
14) MA Endrin	5.661	6.768	217.0E6	2358.4E6	110.197	99.434
19) B Endosulfa...	6.306	7.323	156.6E6	1999.8E6	91.803	84.205m

> D. D 12/04/18

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.