

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120318\
 Data File : PD050617.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2018 20:08
 Operator : AJ\SJ
 Sample : PB115220BS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS20

Manual Integrations
 APPROVED

apatel
 12/4/2018 8:24:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 01:10:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120318CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 04 00:43:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	4.044	30521613	562.7E6	20.012	19.846
27)	SA Decachlor...	7.834	9.152	67119287	905.7E6	40.802	41.846
Target Compounds							
3)	MA gamma-BHC...	3.916	4.724	115.5E6	1777.0E6	49.570	44.970
8)	B Heptachlo...	4.856	5.933	114.6E6	1603.0E6	55.578	44.359
10)	B trans-Chl...	5.074	6.167	114.8E6	1584.8E6	54.590	48.914
12)	B 4,4'-DDE	5.300	6.396	223.3E6	2924.6E6	113.206	100.565
13)	MA Dieldrin	5.414	6.549	245.7E6	2991.4E6	106.273	95.015
14)	MA Endrin	5.661	6.768	221.2E6	2449.2E6	112.369	103.263
19)	B Endosulfa...	6.307	7.323	158.5E6	2056.2E6	92.923	86.581m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120318\
Data File : PD050617.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2018 20:08
Operator : AJ\SJ
Sample : PB115220BS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 01:10:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120318CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 04 00:43:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

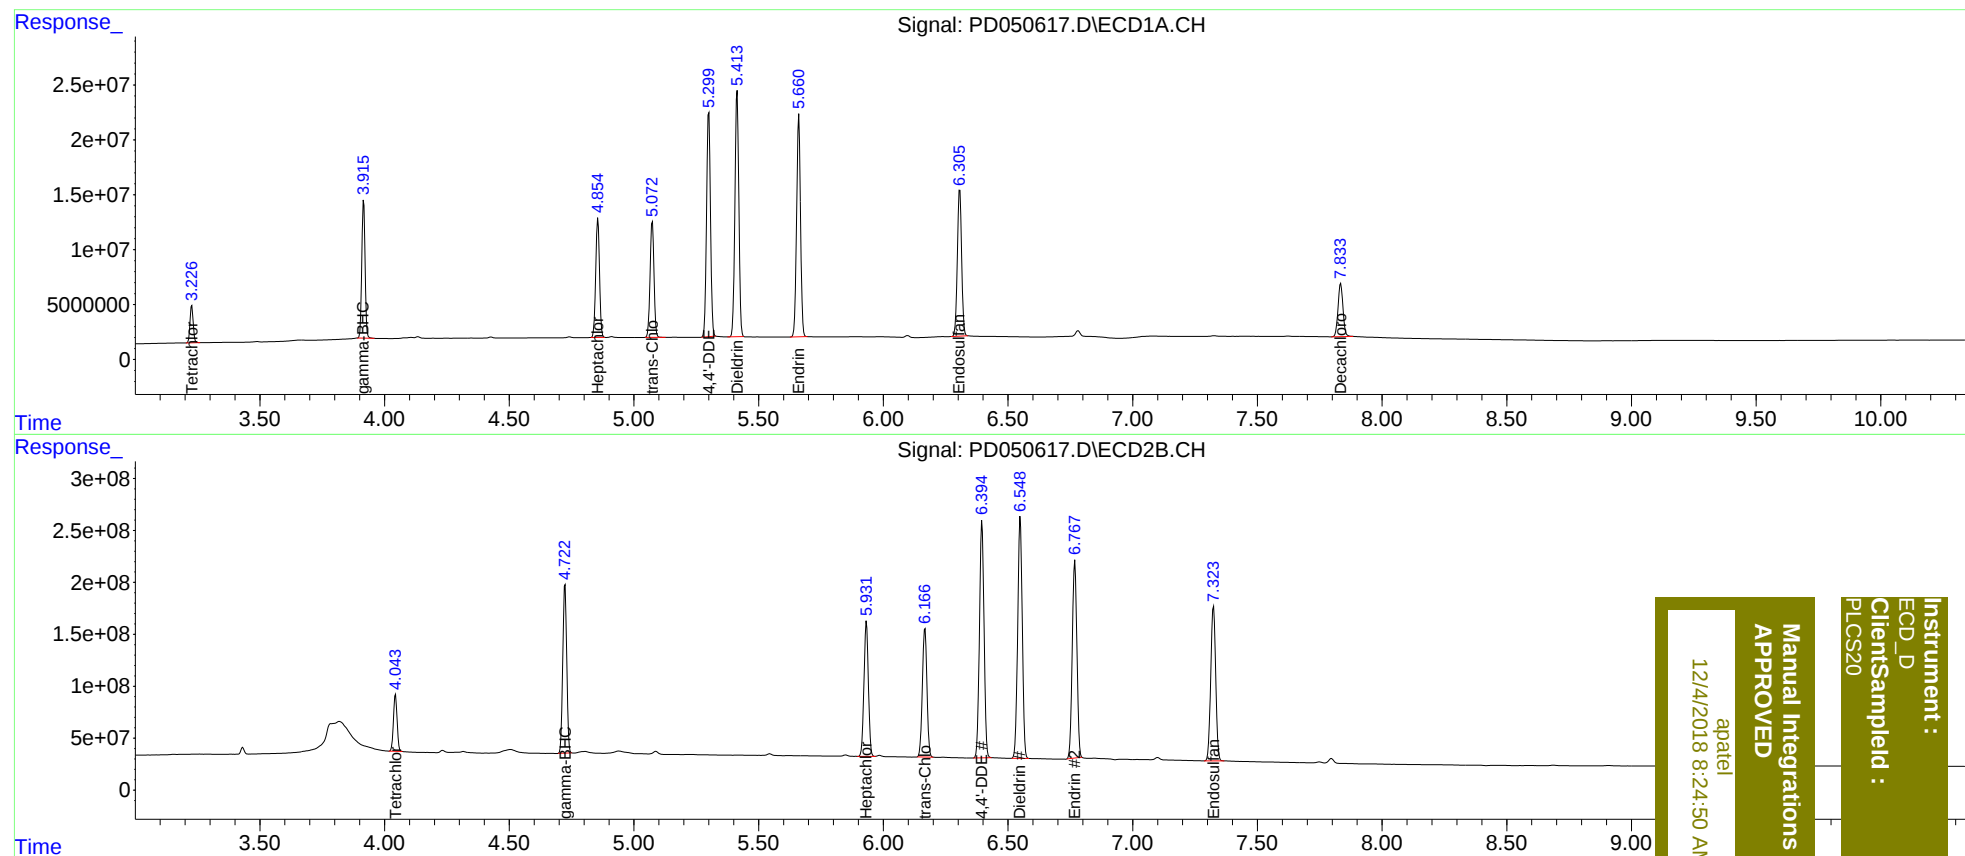

Manual Integrations
APPROVED

apatel
12/4/2018 8:24:50 AM

Instrument :
ECD_D
ClientSampled :
PLCS20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120318\
 Data File : PD050617.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2018 20:08
 Operator : AJ\SJ
 Sample : PB115220BS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS20

Manual Integrations
 APPROVED

apatel
 12/4/2018 8:24:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 01:10:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120318CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 04 00:43:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.227	4.044	30521613	562.7E6	20.012	19.846
27) SA Decachlor...	7.834	9.152	67119287	905.7E6	40.802	41.846
Target Compounds						
3) MA gamma-BHC...	3.916	4.724	115.5E6	1777.0E6	49.570	44.970
8) B Heptachlo...	4.856	5.933	114.6E6	1603.0E6	55.578	44.359
10) B trans-Chl...	5.074	6.167	114.8E6	1584.8E6	54.590	48.914
12) B 4,4'-DDE	5.300	6.396	223.3E6	2924.6E6	113.206	100.565
13) MA Dieldrin	5.414	6.549	245.7E6	2991.4E6	106.273	95.015
14) MA Endrin	5.661	6.768	221.2E6	2449.2E6	112.369	103.263
19) B Endosulfa...	6.307	7.323	158.5E6	2056.2E6	92.923	86.581m

> D.D 12/04/18

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.