

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
 Data File : PD056218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2019 08:59
 Operator : SG\AJ
 Sample : PIBLK42
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK42

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:43:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.289	3.962	17779643	27018759	21.468	22.473
27) SA Decachlor...	7.967	9.002	36275723	49336568	40.174	41.006
Target Compounds						
6) B beta-BHC	0.000	4.847f	0	1541686	N.D.	1.871


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
Data File : PD056218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2019 08:59
Operator : SG\AJ
Sample : PIBLK42
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK42

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:43:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

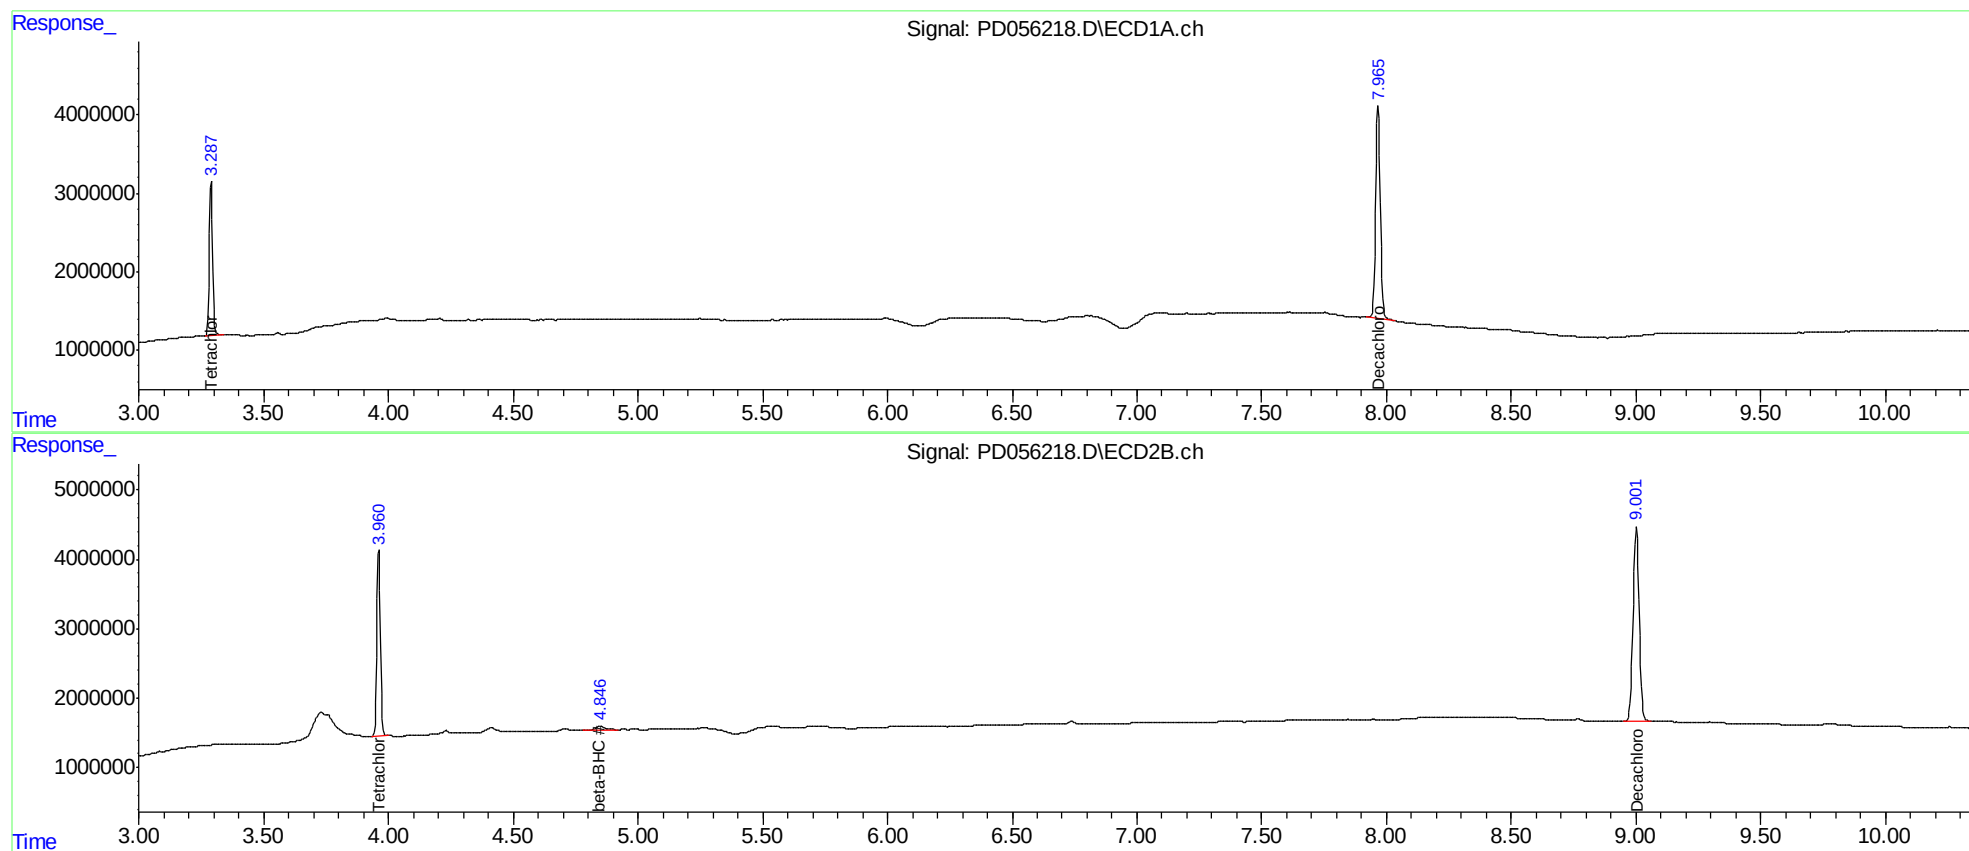


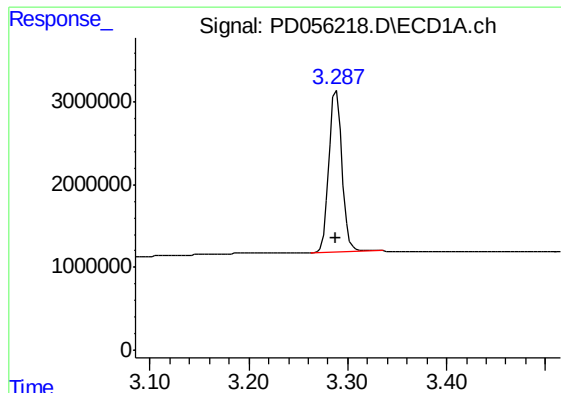

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 17779643
Conc: 21.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK42

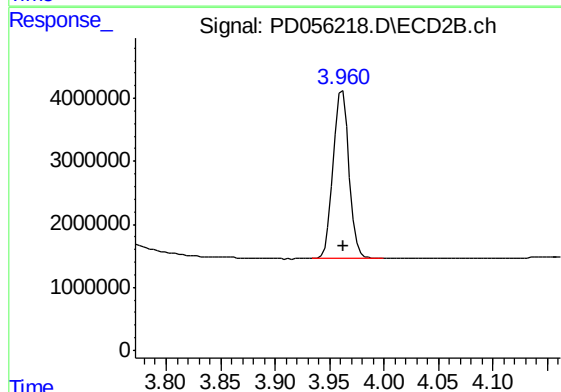


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 27018759
Conc: 22.47 ng/ml

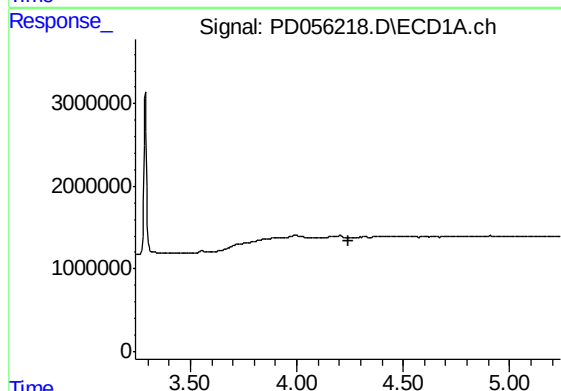


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

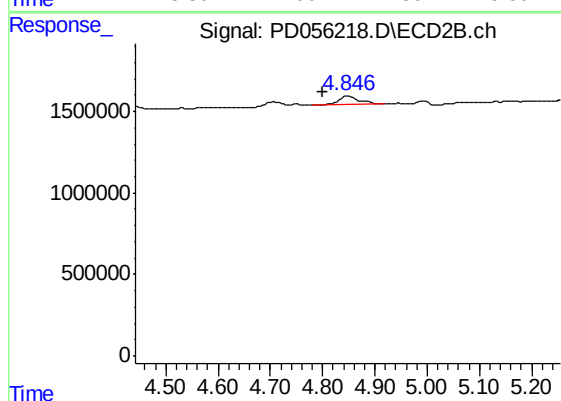

#6 beta-BHC


R.T.: 4.847 min
Delta R.T.: 0.047 min
Response: 1541686
Conc: 1.87 ng/ml

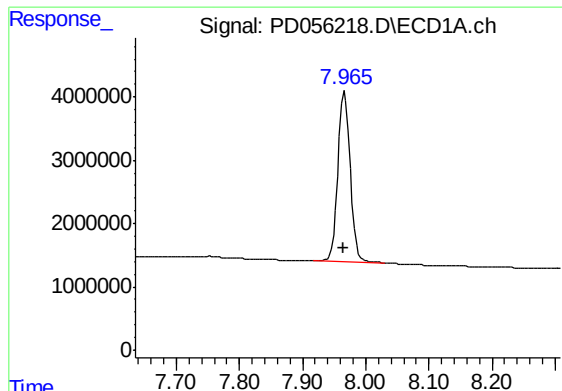

#27 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: 0.001 min
Response: 36275723
Conc: 40.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK42

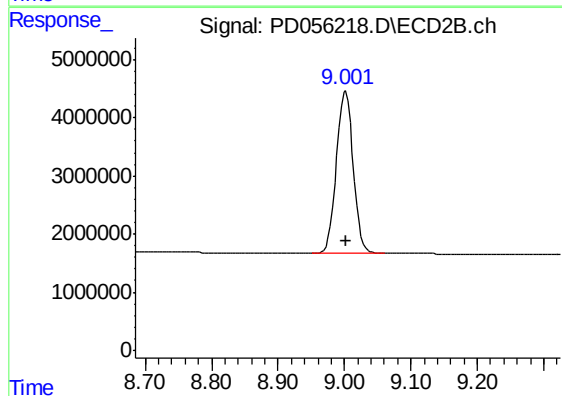

#27 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: 0.000 min
Response: 49336568
Conc: 41.01 ng/ml