

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
 Data File : PD056226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2019 12:20
 Operator : SG\AJ
 Sample : PB125113BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:45:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.295	3.961	16731490	25616613	20.202	21.307
27)	SA Decachlor...	7.975	9.006	33547401	46114873	37.152	38.329
Target Compounds							
16)	A 4,4'-DDD	0.000	6.726f	0	2073832	N.D.	1.762


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
Data File : PD056226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2019 12:20
Operator : SG\AJ
Sample : PB125113BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:45:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

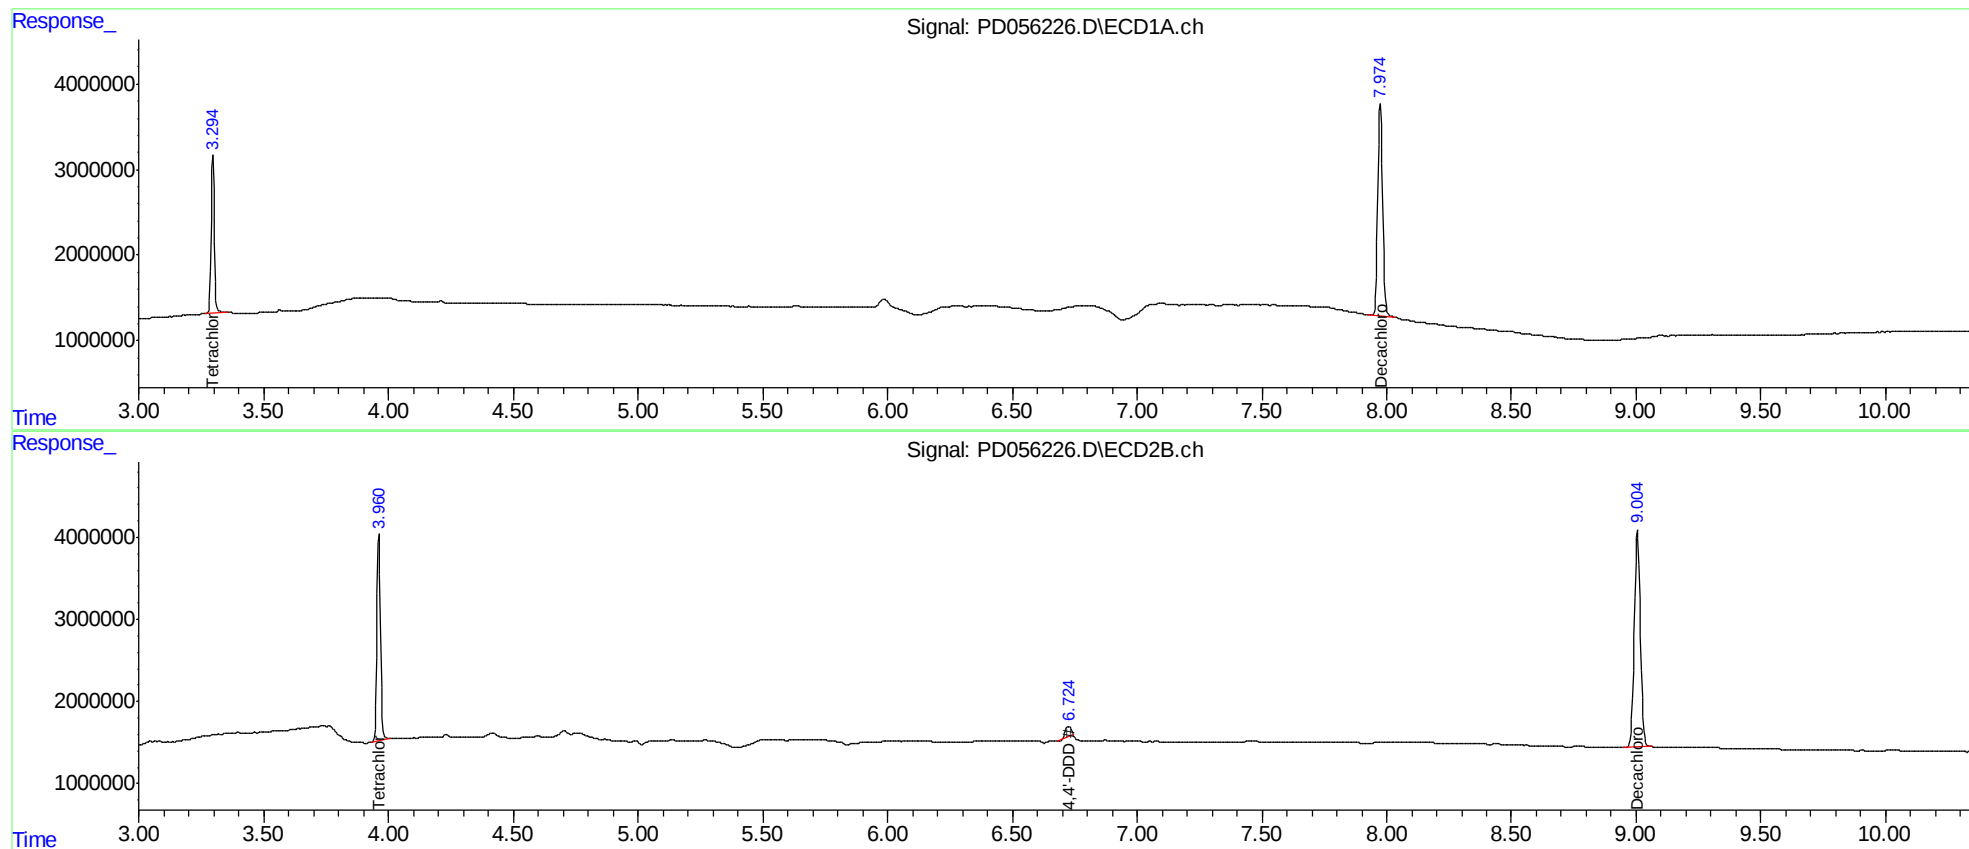


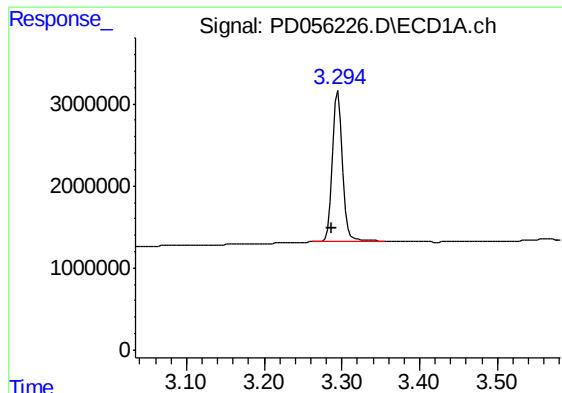

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.007 min
Response: 16731490
Conc: 20.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK13

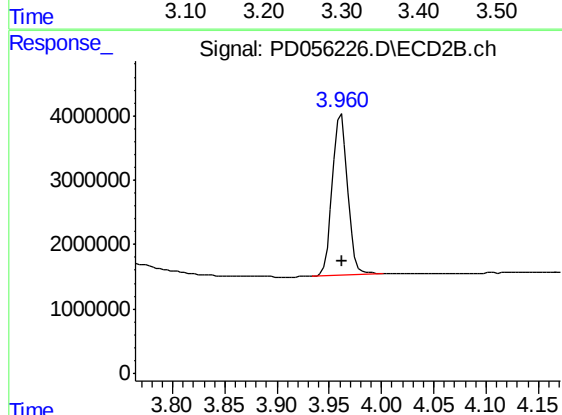


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.001 min
Response: 25616613
Conc: 21.31 ng/ml

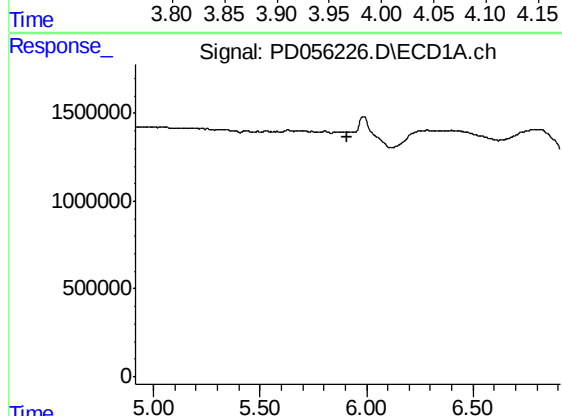


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.912 min
Response: 0
Conc: N.D.

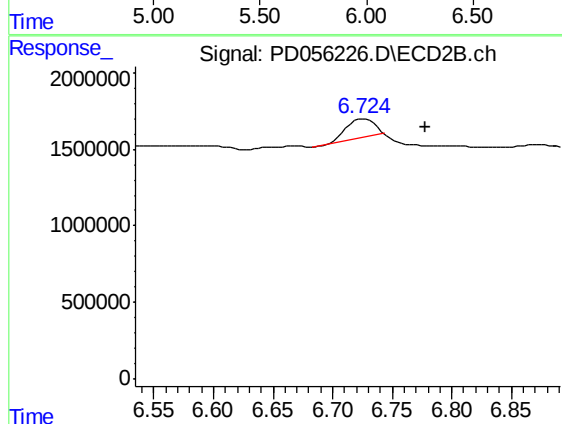

#16 4,4'-DDD


R.T.: 6.726 min
Delta R.T.: -0.052 min
Response: 2073832
Conc: 1.76 ng/ml

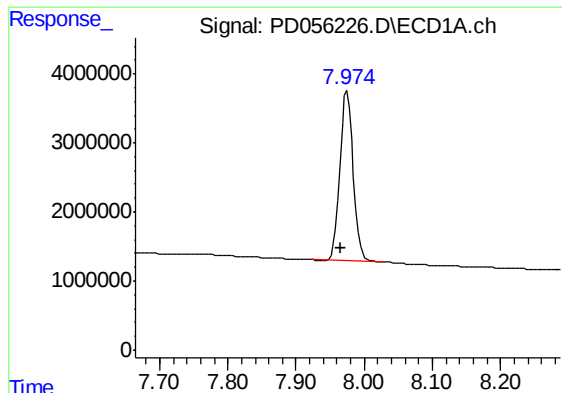

#27 Decachlorobiphenyl

R.T.: 7.975 min
Delta R.T.: 0.010 min
Response: 33547401
Conc: 37.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK13

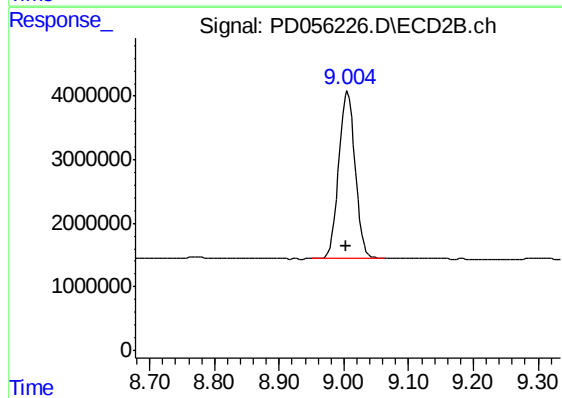

#27 Decachlorobiphenyl

R.T.: 9.006 min
Delta R.T.: 0.003 min
Response: 46114873
Conc: 38.33 ng/ml