

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
 Data File : PD056228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2019 12:47
 Operator : SG\AJ
 Sample : K6007-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BL3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:45:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.288	3.962	20504503	31233067	24.758	25.979
27) SA Decachlor...	7.966	9.002	28951756	39500801	32.063	32.831
Target Compounds						
2) A alpha-BHC	0.000	4.390f	0	762382	N.D.	0.457
4) MA Heptachlor	0.000	5.119	0	760700	N.D.	0.467
6) B beta-BHC	0.000	4.845f	0	2917560	N.D.	3.540


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
Data File : PD056228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2019 12:47
Operator : SG\AJ
Sample : K6007-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BL3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:45:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

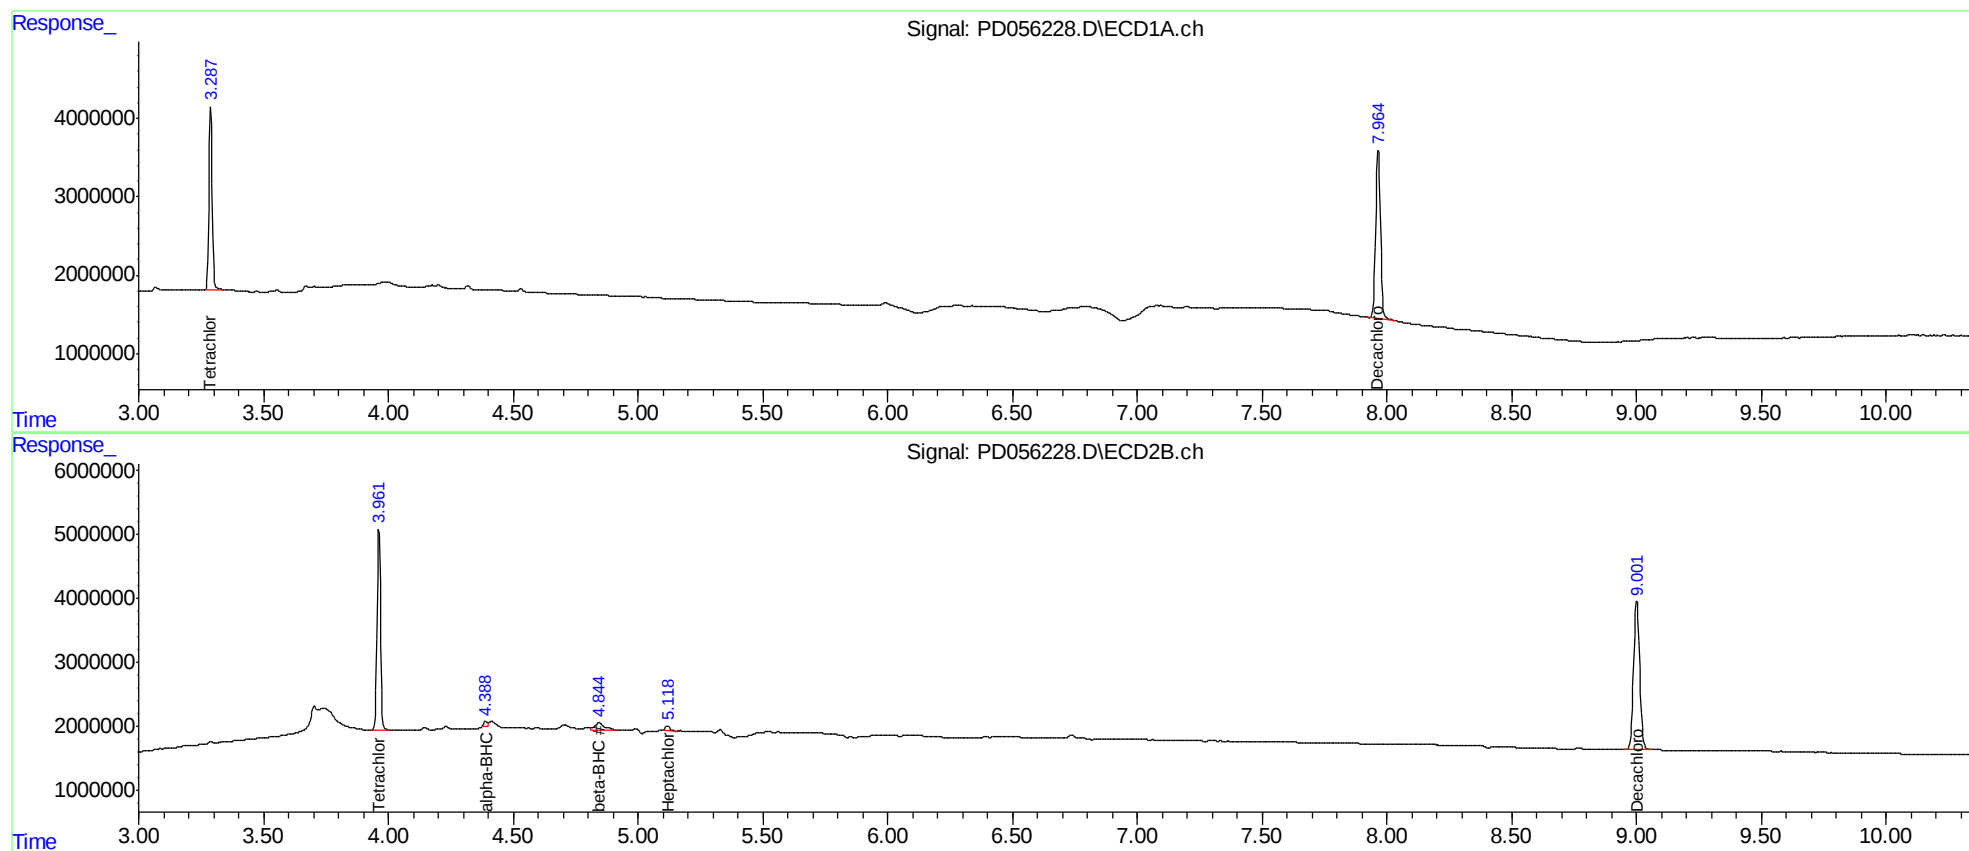


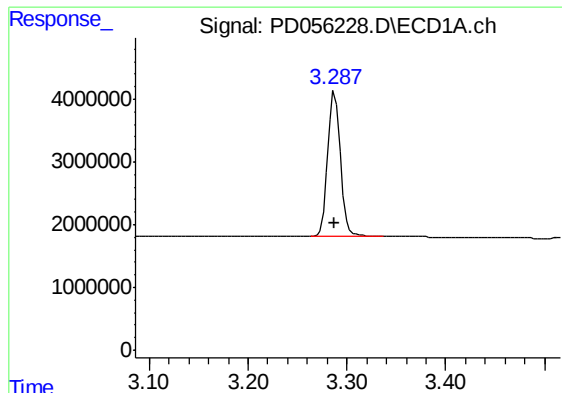

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 20504503
Conc: 24.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BL3

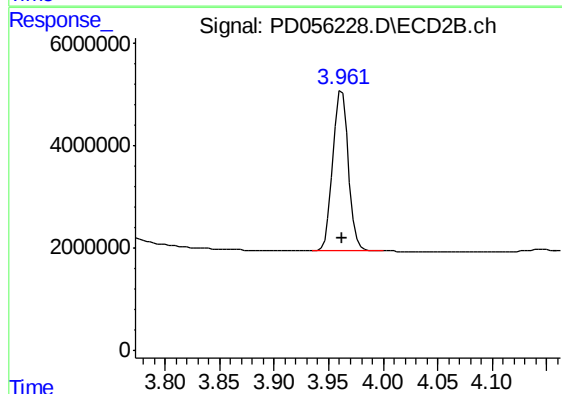


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 31233067
Conc: 25.98 ng/ml

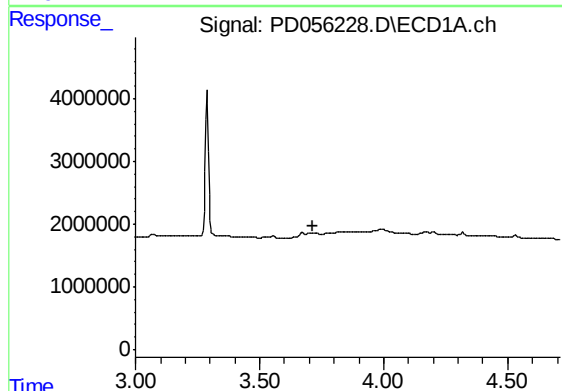


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.715 min
Response: 0
Conc: N.D.

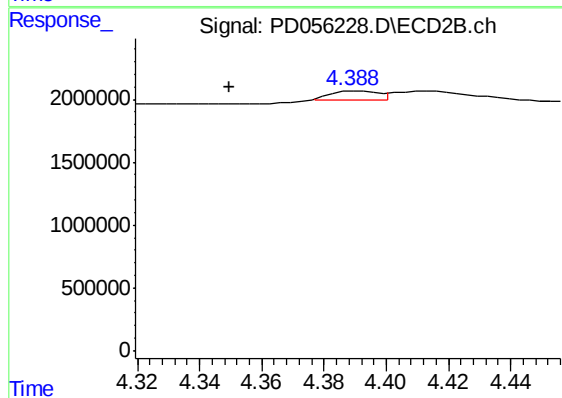

#2 alpha-BHC


R.T.: 4.390 min
Delta R.T.: 0.040 min
Response: 762382
Conc: 0.46 ng/ml

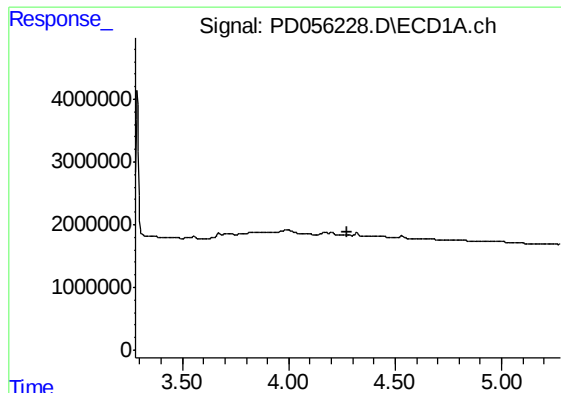

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BL3

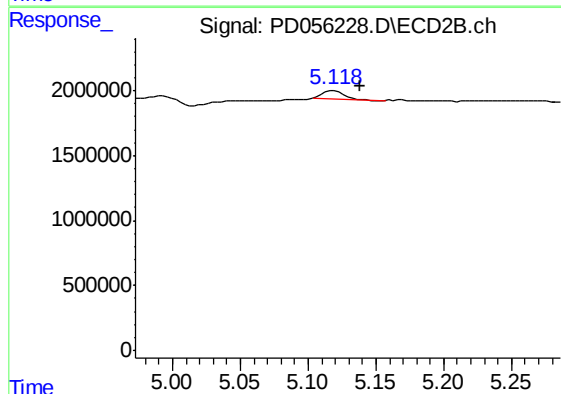


#4 Heptachlor

R.T.: 5.119 min
Delta R.T.: -0.019 min
Response: 760700
Conc: 0.47 ng/ml

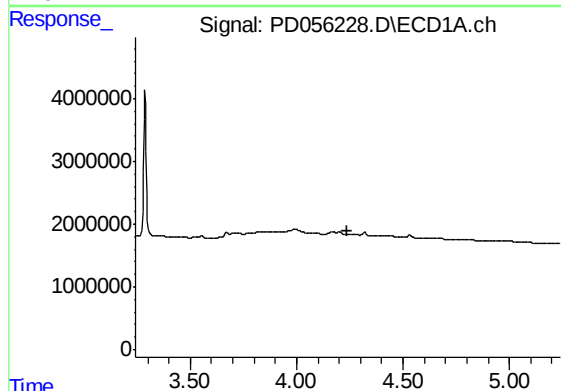


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

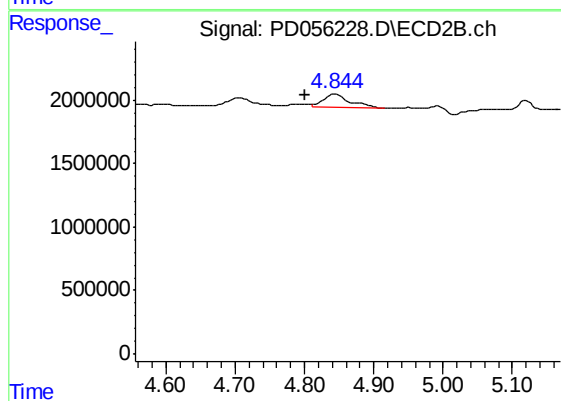

#6 beta-BHC


R.T.: 4.845 min
Delta R.T.: 0.044 min
Response: 2917560
Conc: 3.54 ng/ml

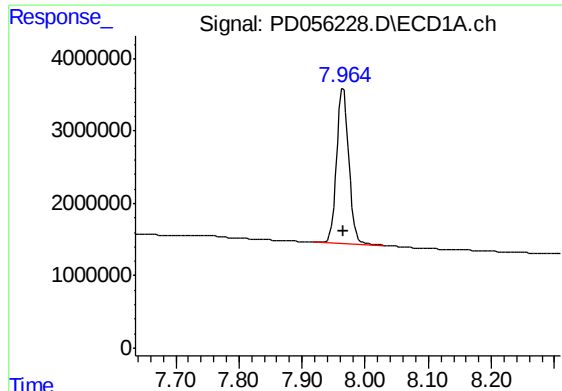

#27 Decachlorobiphenyl

R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 28951756
Conc: 32.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BL3

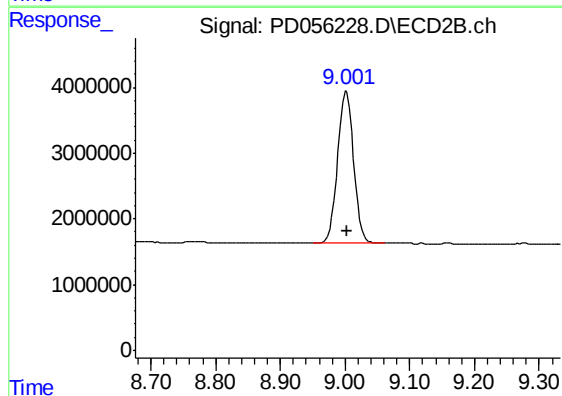

#27 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: 0.000 min
Response: 39500801
Conc: 32.83 ng/ml