

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
 Data File : PD056233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2019 13:57
 Operator : SG\AJ
 Sample : K6086-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFLZ0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:47:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.288	3.963	18502903	27800274	22.341	23.123
27) SA Decachlor...	7.965	9.001	29201403	38907037	32.339	32.338
Target Compounds						
4) MA Heptachlor	0.000	5.158	0	527014	N.D.	0.323
10) B trans-Chl...	0.000	5.991f	0	6792520	N.D.	4.108


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
Data File : PD056233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2019 13:57
Operator : SG\AJ
Sample : K6086-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFLZ0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:47:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

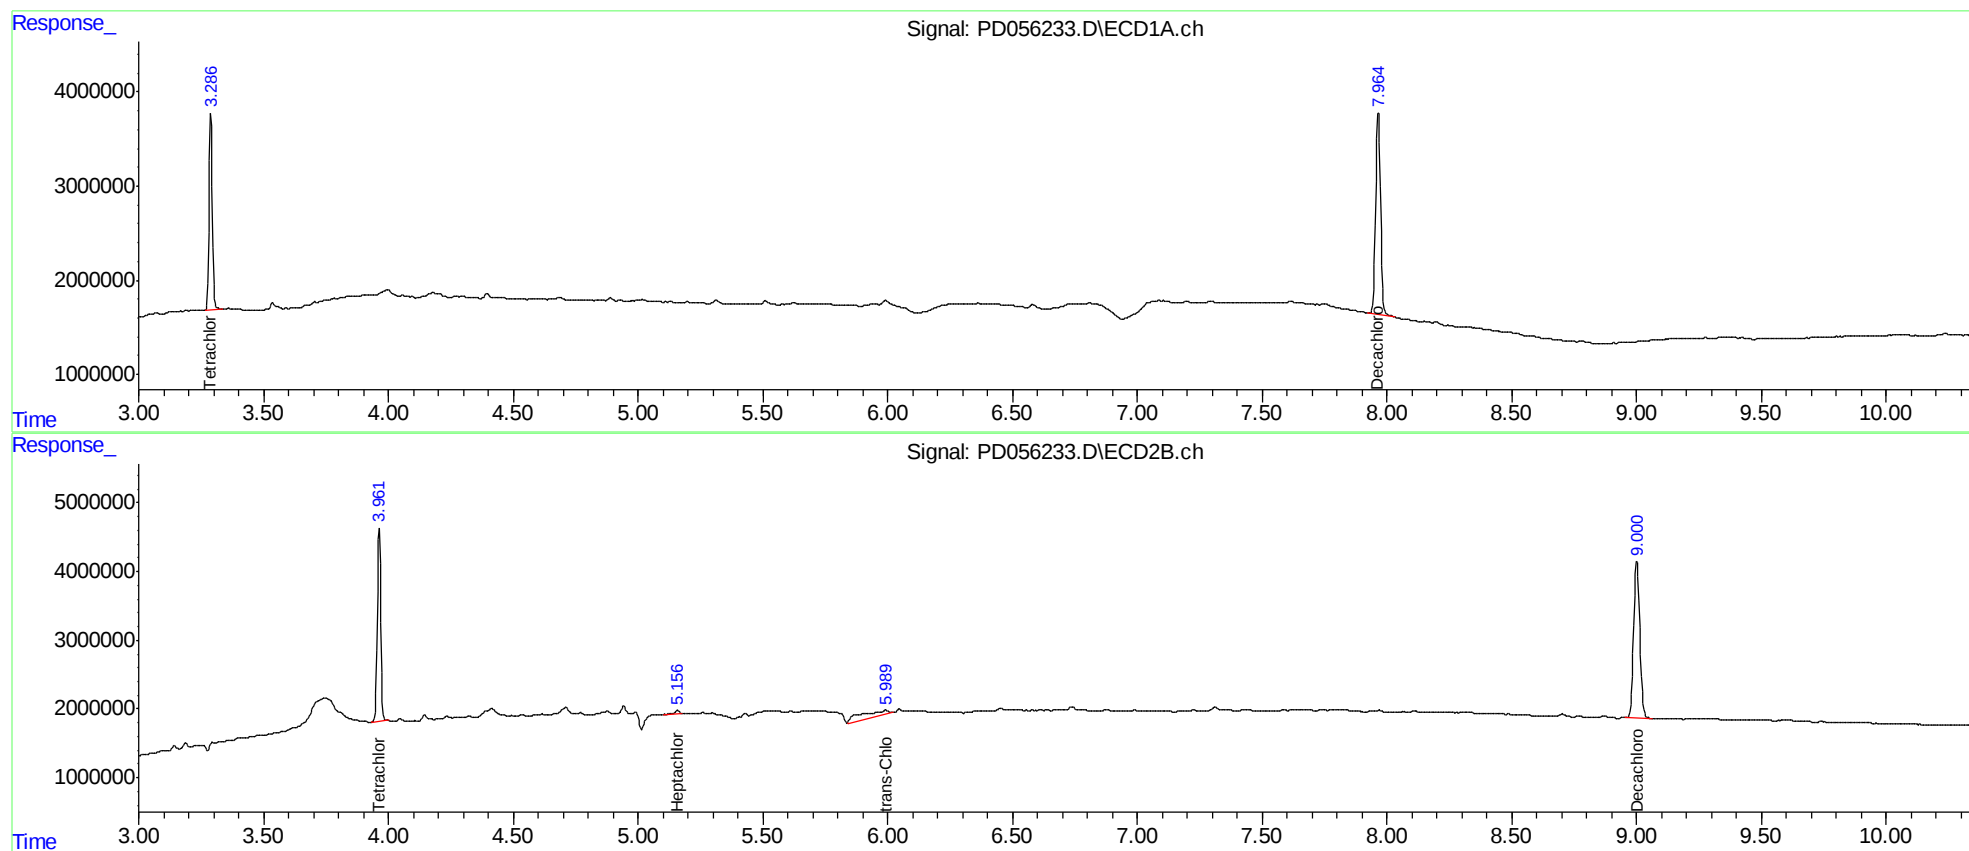


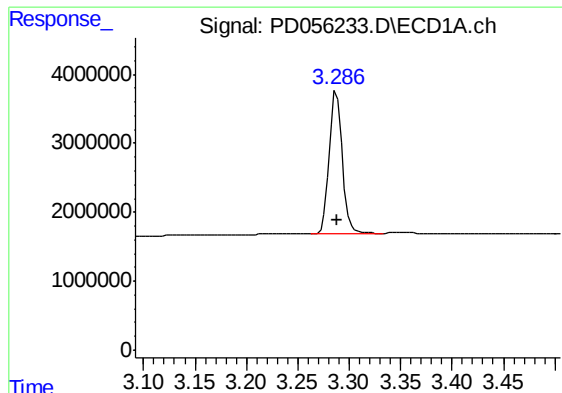

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 18502903
Conc: 22.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFLZ0

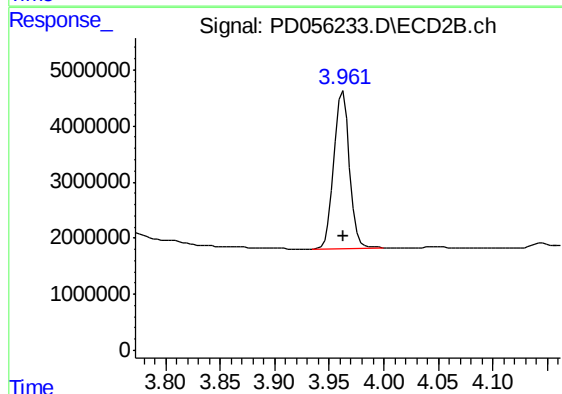


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 27800274
Conc: 23.12 ng/ml

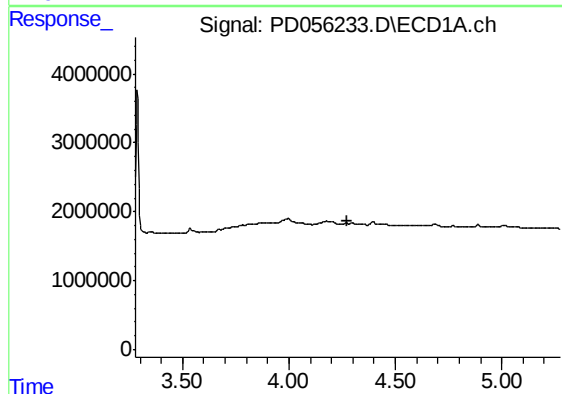


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

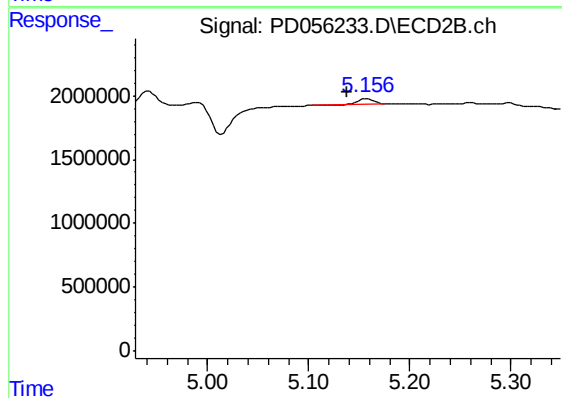

#4 Heptachlor


R.T.: 5.158 min
Delta R.T.: 0.019 min
Response: 527014
Conc: 0.32 ng/ml

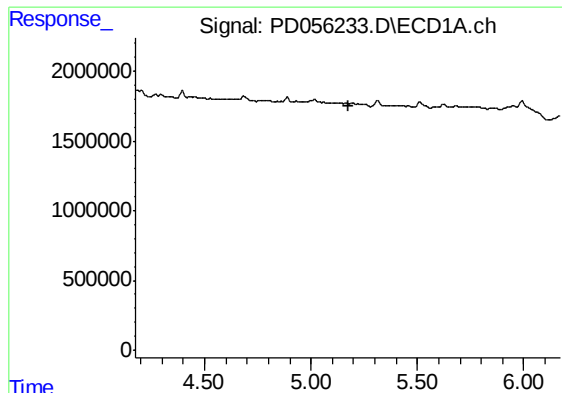

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFLZ0

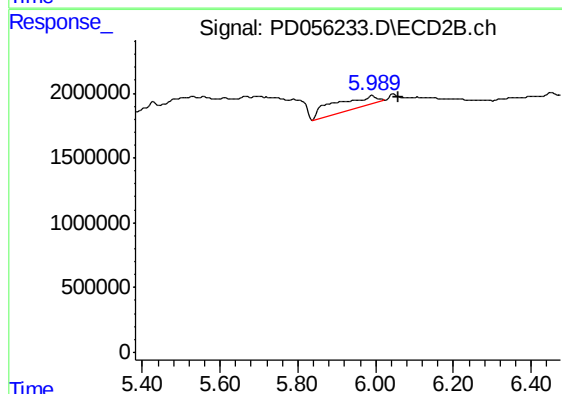


#10 trans-Chlordane

R.T.: 5.991 min
Delta R.T.: -0.069 min
Response: 6792520
Conc: 4.11 ng/ml

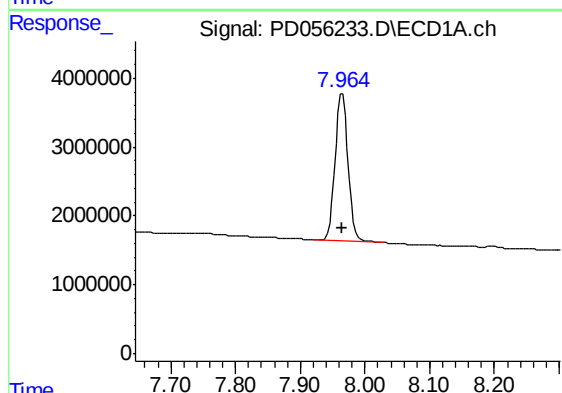

#27 Decachlorobiphenyl

R.T.: 7.965 min
Delta R.T.: 0.000 min
Response: 29201403
Conc: 32.34 ng/ml

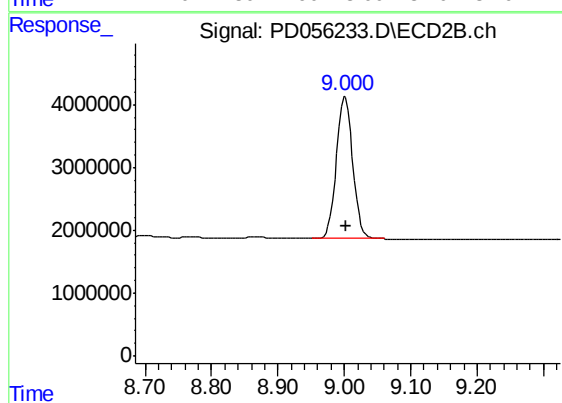

#27 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: -0.001 min
Response: 38907037
Conc: 32.34 ng/ml